MILITARY SPECIFICATION

MASK, OXYGEN, MBU-10/P

This specification is approved for use by the Department of the Air Force and is available for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 This specification covers one type of pressure-breathing oxygen mask that can be rapidly donned over a headset-microphone. The mask is designated MBU-10/P.

2. APPLICABLE DOCUMENTS

2.1 Issues of documents. The following documents of the issue in effect on date of invitation for bids or request for proposal form a part of the specification to the extent specified herein.

SPECIFICATIONS

FEDERAL

L-P-1183	Plastic Molding Material, Acrylonitrile-Butadiene-Styrene (ABS), Rigid
BB-A-1034	Air, Compressed, for Breathing Purposes
BB-N-411	Nitrogen, Technical
ZZ-R-765	Rubber, Silicone
PPP-B-636	Boxes, Shipping, Fiberboard

MILITARY

MIL-B-543	Buckles, Tongueless and Web Strap
MIL-C-5040	Cord, Nylon
MIL-W-6858	Welding, Resistance: Aluminum, Magnesium, Nonharding Steel or Alloys, Nickel Alloys, Heat-Resisting Alloys, and Titanium Alloys; Spot and Seam
MIL-F-7179	Finishes and Coatings: Protection of Aerospace Weapons Systems, Structures and Parts; General Specification for

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to the Aeronautical Systems Division, ASD/ENESS, Wright-Patterson AFB, OH 45433, by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:53Z
Check the source to verify that this is the current version before use.

MIL-T-8363	Tape and Webbing, Textile, Woven, Nylon
MIL-W-8611	Welding, Metal Arc and Gas, Steels, and Corrosion and Heat Resistant Alloys; Process for
MIL-O-27210	Oxygen, Aviator's Breathing, Liquid and Gas
MIL-V-27296	Valve, Oxygen Mask, Combination Inhalation and Exhalation
MIL-C-83501	Cord Assemblies, Electrical, Braided

STANDARDS

FEDERAL

FED-STD-595	Colors
FED-STD-601	Rubber: Sampling and Testing

MILITARY

MIL-STD-100	Engineering Drawing Practices
MIL-STD-129	Marking for Shipment and Storage
MIL-STD-130	Identification Marking of U. S. Military Property
MIL-STD-143	Standards and Specifications, Order of Precedence for Selection of
MIL-STD-781	Reliability Tests: Exponential Distribution
MIL-STD-810	Environmental Test Methods
MIL-STD-831	Test Reports, Preparation of
MIL-STD-889	Dissimilar Metals
MIL-STD-1359	Cleaning Methods and Procedures for Breathing Oxygen Equipment
MS22064	Clamp, Oxygen Hose

DRAWINGS

AIR FORCE

60D3519	Face Form - Oxygen Mask, Size Regular Narrow
64D1676	Cover-Dust, MBU-5/P Oxygen Mask

SIERRA ENGINEERING COMPANY (CODE 92114)

358-1301	Mask, Oxygen, Quick-Donning Assembly
358-1321	Cord Assembly, Lower
358-1330	Cable and Plug Assembly

(Copies of specifications, standards, drawings, and publications required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:53Z
Check the source to verify that this is the current version before use.

2.2 Other publication. The following document forms a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

AMERICAN SOCIETY FOR TESTING AND MATERIALS (ASTM)

D 624 - 54 Tear Resistance of Vulcanized Rubber

(Copies of this publication can be obtained from the American Society for Testing and Materials; 1916 Race Street; Philadelphia, Pennsylvania 19103.)

(Technical society and technical association specifications and standards are generally available for reference from libraries and are also distributed among technical groups and using Federal agencies.)

3. REQUIREMENTS

3.1 Qualification. The masks furnished under this specification shall be products which are qualified for listing on the applicable qualified products list at the time set for opening of bids (see 4.4 and 6.3).

3.2 Selection of specifications and standards. Specifications and standards for necessary commodities and services not specified herein shall be selected in accordance with MIL-STD-143.

3.3 Materials

3.3.1 Metals. Metals shall be corrosion-resistant or suitably treated to resist corrosion due to fuels, salt spray, or any atmospheric conditions likely to be met in storage or normal service.

3.3.1.1 Dissimilar metals. Unless otherwise specified herein, dissimilar metals as defined in MIL-STD-889 having metal-to-metal contact shall not be acceptable. If necessary, combinations of dissimilar metals that have relatively weak galvanic potential may be used provided that their contact surfaces are separated and protected by a passive coating. Any dissimilar metal and protective coating combination proposed to be used shall be presented, prior to fabrication or installation, to the procuring activity for acceptance.

3.3.1.2 Protective treatment. If metals that are subject to deterioration from climatic and environmental conditions likely to occur during service are used, the metals shall be protected in

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:53Z
Check the source to verify that this is the current version before use.

accordance with MIL-F-7179 against this deterioration in a manner that will not in any way prevent compliance with the performance requirements specified herein. The protective coating shall not crack, chip, or scale with age or extremes of climatic and environmental conditions.

3.3.2 Nonmetallic materials. Nonmetallic materials shall be of the ozone-resistant type. Materials that are not susceptible to fungus attack shall be used to the greatest extent possible. Materials that are susceptible to fungus attack, if used, shall be treated with a fungicidal agent.

3.3.2.1 Silicone rubber. The material for the facepiece, the delivery tube, and the microphone cable guides shall be silicone rubber. The silicone rubber shall conform to class 3a, grade 50 of ZZ-R-765 except for the brittle point and the hardness. The minimum brittle point of the silicone rubber shall be minus 56 degrees centigrade. The Shore A hardness of the silicone rubber shall be 45 (plus or minus 5). The color of the silicone rubber shall be green, approximately matching 34079 of FED-STD-595. The silicone rubber shall be smooth and free from flash, foreign materials, and imperfections. The silicone rubber shall be post-cured in a well ventilated forced air oven. The date (year and quarter) the silicone rubber was cured shall be molded on the facepiece and on the delivery tube.

3.3.2.2 Plastic. The material for the hardshell shall conform to type I of L-P-1183 and shall be green, approximately matching 34079 of FED-STD-595.

3.3.2.3 Nylon cord. The nylon cord for the cord and snap assembly shall conform to type IA of MIL-C-5040.

3.3.2.4 Webbing. The webbing for the suspension assembly shall conform to type V of MIL-T-8363 and shall be green, approximately matching 34079 of FED-STD-595.

3.4 Design. The design of the mask shall be in accordance with Drawing 358-1301 and its subsidiary drawings and as specified herein. In the event the requirements of the drawings conflict with the requirements of the text or the figures of this specification, the text and the figures of this specification shall govern.

3.4.1 Facepiece. The facepiece shall conform to Drawing 60D3519 and to figure 1. The anti-freeze chamber and the body of the facepiece shall be of one-piece construction as shown on figures 1 and 2. A 1/16-inch-diameter hole that is located as shown on figures 1 and 2

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:53Z
Check the source to verify that this is the current version before use.

shall vent the antifreeze chamber. A removable, leaktight plug shall be installed in the microphone port of the facepiece. The plug may be fabricated from metal, plastic, or hard rubber.

3.4.2 Delivery tube. The delivery tube shall be made of corrugated silicone rubber and shall conform to figure 3. The delivery tube shall have one lower cable guide that conforms to figure 4 and two upper cable guides that conform to figure 5.

3.4.3 Valve. The combination inhalation-exhalation valve shall conform to MIL-V-27296 and shall be installed in the mask as shown on figure 2.

3.4.4 Clamp. The delivery tube shall be attached to the combination inhalation-exhalation valve by means of a hose clamp that conforms to part No. 450-134A (Sierra Engineering Company, Sierra Madre, California), or an approved equal.

3.4.5 Connector. A connector that conforms to part No. 232-94A (Sierra Engineering Company, Sierra Madre, California), or an approved equal, shall be attached to the delivery tube by means of a hose clamp that conforms to MS22064-5 or other approved hose clamp.

3.4.6 Cord and snap assembly. A nylon cord and metal snap assembly shall be installed inside the delivery tube by attaching the nylon cord to the valve retention pin and the metal snap to the connector retention pin as shown in figure 6. The nylon cord shall be as specified in 3.3.2.3. The metal snap shall be size No. 2/0, 1-3/16 inches in length, 110-pound test (Pacific Marine Supply Company, Seattle, Washington), or equal.

3.4.7 Hardshell. The hardshell of the mask shall closely follow the contour of the outside of the facepiece and shall be designed to assure compliance with all of the performance requirements specified herein. The edges of the hardshell nearest the user's face shall be flared. All sharp edges of the hardshell shall be rounded.

3.4.8 Dust cover. The mask shall be equipped with a dust cover that will prevent dust, dirt, and foreign objects from entering the mask cavity when the mask is not in use. The dust cover shall be made of durable, nonbrittle, lightweight plastic material contoured to rest around the edge of the hardshell and to be retained on the hardshell at the microphone contour. The configuration of the dust cover shall conform to Drawing 64D1676. The dust cover shall not rest on the facepiece contour between the seal area and the body of the facepiece.

3.4.9 Switch. The mask shall have a microswitch that will automatically switch from the boom microphone (Microphone, Dynamic M-87/AIC specified

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:53Z
Check the source to verify that this is the currentversion before use.

in 3.10) to the mask mounted microphone (Microphone, Dynamic M-100/AIC specified in 3.11) during the donning of the mask.

3.4.10 Electrical cord assemblies. The mask shall have two electrical cord assemblies: a lower cord assembly that conforms to Drawing 358-1321 and a cable and plug assembly that conforms to Drawing 358-1330. The two electrical cord assemblies shall conform to section 3 of MIL-C 83501 with the following exceptions:

(a) The dimensions, the wiring diagram, the electrical connectors, and the insulation color coding of the lower cord assembly and of the cable and plug assembly shall conform to Drawing 358-1321 and to Drawing 358-1330, respectively.

(b) The braided jacket for covering the cord shall be composed of black nylon, 210 denier, 5 ends, 24 carriers, approximately 21 picks per inch.

(c) The performance requirements described in 3.6.18.1 and 3.6.18.2 of this specification shall apply in lieu of the performance requirements described in the paragraphs entitled "Flexing life." and "Flexing "Y" junction." in MIL-C-83501.

(d) The performance requirements described in 3.6.19 of this specification shall apply in lieu of the performance requirements described in the paragraph entitled "Isolation." in MIL-C-83501.

(e) The performance requirements described in 3.6.20.1 and 3.6.20.2 of this specification shall apply in lieu of the performance requirements described in the paragraph entitled "Conductor strain relief test." in MIL-C-83501.

(f) In the event of any other conflicts between section 3 of MIL-C-83501 and section 3 of this specification, the requirements of section 3 of this specification shall apply.

3.4.11 Hanging strap. The mask shall have a hanging strap that conforms to part No. 358-643C (Sierra Engineering Company, Sierra Madre, California), or an approved equal.

3.4.12 Buckles. The buckles for the suspension assembly shall be double-bar buckles that conform to type II, style 2, class 1, size 3/4 inch of MIL-B-543.

3.5 Construction. The mask shall be constructed so that no parts will become loose in service. It shall be built to withstand the strains, jars,

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:53Z
Check the source to verify that this is the current version before use.

vibrations, and any other conditions incident to shipment, storage, installation, and service.

3.5.1 Welding, soldering, and brazing. Welding, soldering, and brazing shall be carefully performed to insure that all joints have proper penetration, proper bead, and proper strength. Welding shall be accomplished in accordance with MIL-W-6858, MIL-W-8611, or both MIL-W-6858 and MIL-W-8611.

3.6 Performance

3.6.1 Delivery tube leakage. The delivery tube shall not leak when it is subjected to an internal pressure of 5 pounds per square inch (psi).

3.6.2 Mask leakage. The inboard facepiece leakage of the mask shall not exceed 100 milliliters per minute when a suction of 13 millimeters of mercury is applied within the facepiece of the mask.

3.6.3 Valve installation, inlet performance (low suction). The total leakage through the inlet portion of the combination inhalation-exhalation valve shall be 15 milliliters per minute or less when a suction of 0.19 millimeter of mercury is maintained at the free end of the delivery tube.

3.6.4 Valve installation, exhalation performance. A pressure of 20 millimeters of mercury in the facepiece and a pressure between 15 and 19.9 millimeters of mercury in the inlet tubing shall cause the exhalation portion of the combination inhalation-exhalation valve to open.

3.6.5 Microphone switching. The suspension assembly shall open and close smoothly, without seizing or binding. Opening of the suspension assembly at an angle of 59 degrees (plus or minus 6 degrees) as shown on Drawing 358-1301 shall be the only motion that will cause the microswitch to deactivate the boom microphone circuit and to activate the mask mounted microphone circuit. The mask mounted circuit shall remain activated from 65 degrees to a minimum of 90 degrees. This switching action shall not affect the earphone circuit of the headset-microphone H-157.

3.6.5.1 Wearing position. When the suspension assembly is in the open (wearing) position, the mask microphone circuit shall function without interruption and the boom mounted microphone circuit shall be off.

3.6.5.2 Storage position. When the suspension assembly is in the closed (storage) position, the boom microphone circuit shall function without interruption and the mask mounted microphone circuit shall be off.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:53Z
Check the source to verify that this is the current version before use.

3.6.6 Valve installation, inlet performance (high suction). The total leakage through the inlet portion of the combination inhalation-exhalation valve shall be 150 milliliters per minute or less when a suction of 22.4 millimeters of mercury is applied and maintained at the free end of the delivery tube.

3.6.7 Valve installation, exhalation resistance. The exhalation resistance of the mask, at a flow of 100 liters per minute, shall not be greater than 4.67 millimeters of mercury.

3.6.8 Delivery tube strength. The delivery tube shall not tear or separate from the end connections when it is subjected to a straight pull of 63 pounds (plus or minus 1 pound) for 3 seconds (plus or minus 2 seconds). After this pull has been exerted on the delivery tube, the delivery tube shall meet the requirements specified in 3.6.1.

3.6.9 Nape hanging strap strength. While the mask is supported by its nape hanging strap, the mask shall withstand a force of 20 pounds, applied at the connector end of the delivery tube, without damage to the mask and without interruption of the boom microphone circuit.

3.6.10 Reliability. The suspension assembly shall have a mean cycles between failures (MCBF) of not less than 1,000 cycles at a 90 percent lower confidence limit.

3.6.11 Maintainability. No corrective maintenance task time for the mask shall exceed 20 minutes of maintenance downtime.

3.6.12 Environmental. The mask, while it is subjected to temperatures in the range of minus 40 degrees Fahrenheit to plus 160 degrees Fahrenheit, shall meet the requirements specified in 3.6.5.

3.6.13 Subjective use. The mask shall not have any performance characteristics or any other properties that might be detrimental or objectionable for human use.

3.6.14 Tear resistance. The facepiece shall have a minimum tear resistance of 150 pounds per inch.

3.6.15 Hardness. The facepiece shall have a Shore A hardness of 45 (plus or minus 5).

3.6.16 Toxicity. The facepiece shall not contain any chemicals or any other materials that have toxic properties.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:53Z
Check the source to verify that this is the current version before use.

3.6.17 Hardshell flexibility. When the hardshell is subjected to compression loading, the hardshell shall withstand a decrease in width of 1/2 inch without visible cracking or fracture.

3.6.18 Flexing life

3.6.18.1 Legs. The legs of the lower cord assembly that conforms to Drawing 358-1321 and the legs of the cable and plug assembly that conforms to Drawing 358-1330 shall meet the following requirements: All legs, 5 inches or more in length with four or more conductors, of the assemblies shall have a mean flex life of 50,000 flexes. All legs, 5 inches or more in length with three or less conductors, of the assemblies shall have a mean flex life of 25,000 flexes. The required number of flexes shall be performed without evidence of damage to the outside jacket, of damage to the insulation of the individual conductors, and of electrical discontinuity.

3.6.18.2 "Y" junction. The lower cord assembly that conforms to Drawing 358-1321 shall have a mean flex life at the "Y" junction of 25,000 flexes. The required number of flexes shall be performed without any evidence of damage or of discontinuity. (Note: The cable and plug assembly that conforms to Drawing 353--1330 will not be subject to this requirement.)

3.6.19 Isolation. The lower cord assembly that conforms to Drawing 358-1321, less the connectors, shall meet the isolation requirements listed in table I. (Note: The cable and plug assembly that conforms to Drawing 358-1330 will not be subjected to this requirement.)

TABLE I. Isolation.

Frequency (Hertz)	Electrostatic Isolation (Minimum Decibels)	Electromagnetic Isolation (Minimum Decibels)
20,000	100	69
10,000	106	75
5,000	112	81

3.6.20 Conductor strain relief with connectors

3.6.20.1 Cable and plug assembly. The cable and plug assembly that conforms to Drawing 358-1330 shall not show any signs of slippage of the braided jacket or of electrical failure and shall meet the performance

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:53Z
Check the source to verify that this is the current version before use.

requirements specified in the paragraph entitled "Continuity." in MIL-C-83501 when tensile load is applied between the connectors and the cable.

3.6.20.2 Lower cord assembly. The lower cord assembly that conforms to Drawing 358-1321 shall not show any signs of slippage of the braided jacket or electrical failure and shall meet the performance requirements specified in the paragraph entitled "Continuity." of MIL-C-83501 and the performance requirements specified in 3.6.19 of this specification when tensile load is applied between the connectors and the cable.

3.7 Part numbering of interchangeable parts. All parts having the same manufacturer's part number shall be functionally and dimensionally interchangeable. The drawing number requirements of MIL-STD-100 shall govern the manufacturer's part numbers and changes thereto.

3.8 Weight. The weight of the completely assembled mask shall not exceed 2.25 pounds.

3.9 Marking

3.9.1 Identification of product. The facepiece and the suspension assembly shall be marked for identification in accordance with MIL-STD-130.

3.9.1.1 Facepiece. The following specific information shall be marked on the facepiece.

Regular Narrow
Manufacturer 1/
Date of Manufacture (Quarter and Year) 1/

1/ The manufacturer shall include the applicable information.

3.9.1.2 Suspension assembly. The following specific information shall be marked on the suspension assembly:

Mask, Oxygen, MBU-10/P
Manufacturer 1/

1/ The manufacturer shall include the applicable information.

3.9.2 Delivery tube. The following words shall be molded into the rubber of the mask end of the delivery tube: MASK END. The date of manufacture (quarter and year) shall be molded on either end of the delivery tube.

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:53Z
Check the source to verify that this is the current version before use.

3.10 Government-loaned property. When specified (see 6.2), the following items will be loaned by the Government to the manufacturer of the mask.

Item No.	Item Description	Quantity
1	Headest-Microphone H-157 consisting of the Headset, Electrical H-158/AIC and the Microphone, Dynamic M-87/AIC	1

3.11 Government-furnished property. When specified (see 6.2), the following item (mask mounted microphone) will be furnished by the Government to the manufacturer of the mask.

Item Description	Quantity Required
Microphone, Dynamic M-100/AIC	1 per mask

3.12 Workmanship. The mask shall be constructed in accordance with good commercial practice and shall be free from any defects that might affect appearance or functionability. The mask shall be clean; dry; and free from oil, grease, and any other foreign matter. All metal and plastic parts shall be smooth and free of sharp edges. All excess flash shall be properly trimmed. The facepiece and its related parts shall be smooth and free from blisters, porous areas, cracks, abrasions, bubbles, and foreign material.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.2 Classification of inspection. The inspection required by this specification is classified as follows:

(a) Qualification inspection

(b) Quality conformance inspection.

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:53Z
Check the source to verify that this is the current version before use.

4.3 Test conditions

4.3.1 Atmospheric conditions. Unless otherwise specified all tests required by this specification shall be made at an atmospheric pressure of 28 to 32 inches of mercury, at a temperature of 77 degrees (plus or minus 18 degrees) Fahrenheit, and at a relative humidity of 80 percent or less. Where tests are made with atmospheric pressure or temperature substantially different from these values, proper allowance shall be made for the change in instrument reading.

4.3.2 Gas. The gas used for the qualification tests shall be oxygen that conforms to type I of MIL-0-27210. The gas used for the quality conformance tests shall be oxygen that conforms to type I of MIL-0-27210; water-pumped nitrogen that conforms to type I, grade B, class 1 of BB-N-411; or compressed air that conforms to grade A or C of BB-A-1034. If the gas used is nitrogen or compressed air, appropriate density correction factors shall be applied to the flowmeter used.

4.4 Qualification inspection. Unless otherwise specified herein (see 4.4.4), the qualification inspection shall consist of all of the test methods described under 4.6 of this specification and of all the methods of examination and test described in MIL-C-83501. The qualification samples specified in 4.4.5 shall be subjected to the qualification inspection as specified in 4.4.1 through 4.4.4.

4.4.1 Masks. Four completely assembled masks shall be subjected to the test methods described in 4.6.1 through 4.6.13 of this specification. Two completely assembled masks shall be subjected to the test methods described in 4.6.1 through 4.6.6 and in 4.6.14.

4.4.1.1 Acceptance for reliability. The acceptance for the reliability testing described in 4.6.11 shall be judged on the basis of the accept-reject criteria of test plan I of MIL-STD-781. Recording, data handling, and reporting procedures for the reliability testing shall be in accordance with MIL-STD-781.

4.4.2 Facepiece. The extra facepiece and the four sheets of silicone rubber shall be subjected to the test methods described in 4.6.15 through 4.6.17 of this specification.

4.4.3 Hardshells. The three extra hardshells shall be subjected to the hardshell flexibility test described in 4.6.18 of this specification.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:53Z
Check the source to verify that this is the current version before use.

4.4.4 Cord assemblies. The five extra terminated cord assemblies and the five extra unterminated cord assemblies shall be subjected to the examinations and tests specified for first article inspection in section 4 of MIL-C-83501 with the following exceptions:

(a) The test methods described in 4.6.19.1 and 4.6.19.2 of this specification shall apply in lieu of the test methods described under "Flexing life." in MIL-C-83501.

(b) The test method described in 4.6.20 of this specification shall apply in lieu of the test method entitled "Isolation." in MIL-C-83501.

(c) The test methods described in 4.6.21.1 and 4.6.21.2 of this specification shall apply in lieu of the test method entitled "Conductor strain relief cords assembled with connectors." in MIL-C-83501.

4.4.5 Qualification samples. The qualification samples shall be representative of the production equipment and shall be identified with the manufacturer's part number and any other information required by the qualifying activity (see 6.3). The qualification samples shall consist of the following items:

(a) Six completely assembled masks

(b) One extra facepiece

(c) Three extra hardshells

(d) Four sheets (6 inches by 6 inches by 0.06 inch each) of silicone rubber that is identical in composition and cure to the silicone rubber used in the facepieces

(e) Five extra terminated cord assemblies

(f) Five extra unterminated cord assemblies.

4.4.6 Samples and reports for qualifying activity. The following items shall be furnished to the qualifying activity (see 6.3):

(a) The tested qualification samples

(b) Three copies of a qualification test report that conforms to MIL-STD-831 and that includes the results of all qualification tests and a detailed statement of compliance or noncompliance with each requirement of this specification, identified by the applicable paragraph number

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:53Z
Check the source to verify that this is the current version before use.

(c) Three copies of a silicone rubber report that shall contain the following information:

(1) Compound number and name of manufacturer

(2) Composition of compound, including fillers and catalysts, giving parts by weight of each constituent

(3) Mixing and curing instructions

(4) Any other information that the manufacturer desires to furnish for better identification of the material or for showing that the material has desirable characteristics for oxygen mask usage.

4.5. Quality conformance inspection. Unless otherwise specified herein (see 4.5.1), the quality conformance inspection shall consist of the following:

(a) Individual tests

(b) Sampling tests.

4.5.1 Electrical cord assemblies. The lower cord assembly that conforms to Drawing 358-1321 and the cable and plug assembly that conforms to Drawing 358-1330 shall be subjected to the quality conformance inspection described in section 4 of MIL-C-83501 with the following exceptions:

(a) The test methods described in 4.6.19.1 and 4.6.19.2 of this specification shall apply in lieu of the test methods described under "Flexing life." in MIL-C-83501.

(b) The test method described in 4.6.20 of this specification shall apply in lieu of the test method entitled "Isolation." in MIL-C-83501.

(c) The test methods described in 4.6.21.1 and 4.6.21.2 of this specification shall apply in lieu of the test method entitled "Conductor strain relief cords assembled with connectors." in MIL-C-83501.

(d) In the event of any other conflicts between section 4 of MIL-C-83501 and section 4 of this specification, the requirements of section 4 of this specification shall apply.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:53Z
Check the source to verify that this is the current version before use.

4.5.2 Individual tests. Each mask shall be subjected to the following test methods as described under 4.6 of this specification:

(a) Examination of product

(b) Delivery tube leakage

(c) Mask leakage

(d) Valve installation, inlet performance (low suction)

(e) Valve installation, exhalation performance

(f) Microphone switching.

4.5.3 Sampling tests

4.5.3.1 Plan A. Two masks shall be selected at random from each lot of 1,000 masks, or fraction thereof, which have been manufactured essentially under the same conditions and at the same time. Each mask that is selected as a sample shall be subjected to the following test methods as described under 4.6 of this specification:

(a) Valve installation, inlet performance (high suction)

(b) Valve installation, exhalation resistance

(c) Delivery tube strength.

4.5.3.2 Plan B. One facepiece shall be selected at random from all of the facepieces that have been manufactured from the same batch (see 6.4) of silicone rubber compound. Each facepiece selected as a sample shall be subjected to the following tests as described under 4.6 of this specification:

(a) Tear resistance

(b) Hardness.

4.5.3.3 Plan C. Four sheets of silicone rubber shall be fabricated from each batch (see 6.4) of silicone rubber compound. Each sheet of silicone rubber shall be 6 inches by 6 inches by 0.06 inch and shall be identical in composition and cure to the silicone rubber used in the facepiece. Each sheet of silicone rubber shall be subjected to the following tests as described under 4.6 of this specification:

(a) Tear resistance

(b) Hardness.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:53Z
Check the source to verify that this is the current version before use.

4.5.3.4 Plan D. If the hardshells are not molded in an essentially continuous operation, three hardshells shall be selected at random from all of the hardshells that have been molded under the same conditions, at substantially the same time, and from the same batch (see 6.4) of plastic molding material. Each hardshell that is selected as a sample shall be subjected to the hardshell flexibility test described in 4.6.18.

4.5.3.5 Plan E. If the hardshells are molded in an essentially continuous operation, three hardshells shall be selected at random from each day's production of each mold cavity. Each hardshell that is selected as a sample shall be subjected to the hardshell flexibility test described in 4.6.18.

4.5.3.6 Rejection and retest

4.5.3.6.1 Sampling plans A, B, C, and D. If a sample selected in accordance with sampling plan A, B, C, or D fails to meet the specification, acceptance of all the items represented by the sample shall be withheld until the extent and cause of failure have been determined and corrected. The contractor shall explain fully to the Government representative and notify the procuring activity in writing the cause of failure, the action taken to preclude recurrence, and the impact the failure may have on scheduled deliveries. After correction, all of the sampling tests shall be repeated.

4.5.3.6.2 Sampling plan E. If a sample selected from a production run in accordance with sampling plan E fails to meet the specification, no items still on hand or later produced shall be accepted until the extent and cause of failure have been determined. The contractor shall explain fully to the Government representative and notify the procuring activity in writing the cause of failure, the action taken to preclude recurrence, and the impact this failure may have on scheduled deliveries.

4.5.3.7 Continuation of tests. For production reasons, individual tests or other sampling plans may be continued pending the investigation of a sampling test failure. Final acceptance of the items represented by the samples shall not be made until it is determined that all items meet all the requirements of the specification.

4.5.4 Defects in items already accepted. The investigation of a test failure could indicate that defects may exist in items already accepted. If so, the contractor shall fully advise the procuring activity of all defects likely to be found and the methods of correcting them.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:53Z
Check the source to verify that this is the current version before use.

4.6 Test methods

4.6.1 Examination of product. The completely assembled mask shall be examined to determine conformance to the requirements of this specification with respect to materials, design, construction, dimensions, markings, and workmanship.

4.6.2 Delivery tube leakage. One end of the delivery tube shall be plugged. An air pressure of 5 psi shall be applied to the other end of the delivery tube. The delivery tube shall be submerged just under the surface of water and observed. Bubbles rising from the delivery tube after it has been submerged 10 to 15 seconds shall be cause for rejection.

4.6.3 Mask leakage. The mask (with the combination inhalation-exhalation valve correctly installed) shall be placed on a suitable test stand and adjusted so that there is no leakage around the face seal. The free end of the mask tubing shall be plugged. A suction of 13 millimeters of mercury shall be applied within the facepiece of the mask. While this suction is applied, the inboard facepiece leakage shall not exceed 100 milliliters.

4.6.4 Valve installation, inlet performance (low suction). The inlet portion of the combination inhalation-exhalation valve shall be completely dry during test. A suction of 0.19 millimeter of mercury shall be applied and maintained at the free end of the delivery tube. While this suction is maintained, the inlet portion of the combination inhalation-exhalation valve shall be inspected for imperfect seating of the flapper on the seat and for leaks around the valve seat. The total leakage through the inlet portion of the combination inhalation-exhalation valve shall be not more than 15 milliliters per minute. If necessary, a suitable means to prevent collapse of the hose may be used.

4.6.5 Valve installation, exhalation performance. The mask shall be placed on a suitable test stand. All suction and pressure in the mask from the previous test shall be exhausted. A pressure of 20 millimeters of mercury shall be applied at the mask tubing. The pressure at the mask tubing shall then be reduced gradually, causing the inlet portion of the combination inhalation-exhalation valve to close and causing a pressure differential to be applied across the exhalation portion of the combination inhalation-exhalation valve. The exhalation portion of the combination inhalation-exhalation valve shall open with a pressure in the tube between 15 and 19.9 millimeters of mercury. If extreme pressure in encountered, the inlet portion of the combination inhalation-exhalation valve shall be rechecked for leakage. If the combination inhalation-exhalation valve is properly seated and the mask

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:53Z
Check the source to verify that this is the current version before use.

still fails to function properly, the combination inhalation-exhalation valve shall be replaced, and the test shall be repeated.

4.6.6 Microphone switching. The suspension assembly of the mask shall be operated. The angle at which the microswitch activates shall be determined and shall be as specified in 3.6.5.

4.6.7 Valve installation, inlet performance (high suction). The inlet portion of the combination inhalation-exhalation valve shall be completely dry during this test. A suction of 22.4 millimeters of mercury shall be applied and maintained at the free end of the delivery tube. While this suction is maintained, the inlet portion of the combination inhalation-exhalation valve shall be inspected for imperfect seating of the flapper on the seat and for leaks around the valve seat. The total leakage through the inlet portion of the combination inhalation-exhalation valve at this suction shall be not more that 150 milliliters per minute. If necessary, a suitable means to prevent collapse of the hose may be used.

4.6.8 Valve installation, exhalation resistance. The mask (with the combination inhalation-exhalation valve installed) shall be placed on a suitable test stand. At an exhalation flow of 100 liters per minute, the pressure inside the mask shall not exceed ambient pressure by more than 4.67 millimeters of mercury.

4.6.9 Delivery tube strength. The cord and snap assembly shall be attached to the mask before this test is commenced. One end of the delivery tube shall be attached to the combination inhalation-exhalation valve mounted on the mask body. The other end of the delivery tube shall be connected to a fitting that simulates the connector specified in 3.4.5. The clamps for the connections shall be of the type specified herein. One of the end connections shall be attached to a support. A weight of 63 pounds (plus or minus 1 pound) shall be attached to the other connection so that a straight pull will be exerted on the tubing for a period of 3 seconds (plus or minus 2 seconds). The tubing shall not tear and shall not separate from the end connections. Upon completion of this test, the delivery tube shall be subjected to the delivery tube leakage test described in 4.6.2.

4.6.10 Nape hanging strap strength. The mask shall be freely supported by the nape hanging strap. A weight of 20 pounds (plus or minus 1/2 pound) shall be hung from the connector end of the delivery tube. While this force is applied, the boom microphone electrical circuit shall be continuous.

4.6.11 Reliability. The suspension assembly of the mask shall be subjected to repeated cycling. After each 250 cycles, the mask shall

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:53Z
Check the source to verify that this is the current version before use.

be tested as specified in 4.6.6. Failure shall be identified as the inability of the mask to meet the requirements specified in 3.6.5. A cycle shall consist of the following steps:

(a) Open the suspension assembly to the wearing position.

(b) Close the suspension assembly to the storage position.

4.6.12 Maintainability verification. Time studies of all corrective maintenance tasks for all expected failure modes shall be conducted by simulating failures. Timing of each maintenance task to determine average values shall be performed at least three times. Only maintenance tasks that are related to field level maintenance shall be considered. The time to accomplish each maintenance task shall include time for preparation, recognition, fault location, removal (based only on the installation provisions of the item), fault correction, adjustment and realignment, final test, and replacement but shall exclude supply time and administrative time. Redetermination of the average time required, in the case of repetitive subtasks that occur by the nature of the sequence of the maintenance actions (e. g. removal), shall not be necessary.

4.6.13 Environmental. The mask shall be subjected to the high temperature and the low temperature tests. The mask shall be allowed to reach stabilized conditions after each step, before proceeding to the next step, of the high temperature and the low temperature tests.

4.6.13.1 High temperature. The mask shall be subjected to a high temperature test in accordance with method 501, procedure II of MIL-STD-810. The operating parameters specified in 3.6.5 shall be used in lieu of the pretest performance record specified in MIL-STD-810. The temperature for step 7 shall be 160 degrees Fahrenheit. The suspension assembly shall be cycled (see 4.6.11) once every 10 minutes for 4 hours during step 8.

4.6.13.2 Low temperature. The mask shall be subject to a low temperature test in accordance with method 502, procedure I of MIL-STD-810. The operating parameters specified in 3.6.5 shall be used in lieu of the pretest performance record specified in MIL-STD-810. The temperature for steps 2 and 4 shall be minus 40 degress Fahrenheit. The time period for step 2 shall be 4 hours. The suspension assembly shall by cycled (see 4.6.11) once every 10 minutes for 4 hours during step 4.

4.6.14 Subjective use. The mask shall be used by human subjects for up to 2 hours at altitudes from ground level to 40,000 feet at temperatures from minus 40 degrees Fahrenheit to plus 160 degrees Fahrenheit or any combination of such altitude and temperature. Subjective use

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:53Z
Check the source to verify that this is the current version before use.

tests are optional tests to be conducted at the discretion of and by the Government when the mask appears to have performance characteristics or any other properties that might be detrimental or objectionable for human use.

4.6.15 Tear resistance. The tear resistance of the sheets of silicone rubber and of sections of silicone rubber cut from the sealing area of the facepiece shall be determined in accordance with die B of ASTM D 624 - 54. The minimum test resistance of the silicone rubber shall be 150 pounds per inch.

4.6.16 Hardness. The hardness of the sheets of silicone rubber and of sections of silicone rubber cut from the sealing area of the facepiece in both the nose and cheek areas shall be determined in accordance with method 3021 of FED-STD-601. The Shore A hardness of the silicone rubber shall be 45 (plus or minus 5).

4.6.17 Toxicity. Toxicity shall be determined from the chemicals used in the formation of the silicone rubber compound.

4.6.18 Hardshell flexibility. The hardshell shall be placed between the heads of a suitable compression testing machine with the heads contacting the sides of the hardshell at the point of maximum width. A suitable means of measuring the decrease in width of the hardshell under load shall be provided. The rate of head travel shall be 0.20 to 0.25 inch per minute. The hardshell shall be deformed until failure or until the required decrease in width is attained, whichever occurs first. The hardshell shall withstand at least a 1/2-inch decrease in width without visible cracking or breaking.

4.6.19 Flexing life

4.6.19.1 Legs. All legs, 5 inches or more in length, of the lower cord assembly that conforms to Drawing 358-1321 and of the cable and plug assembly that conforms to Drawing 358-1330 shall conform to 3.6.18.1 when tested as follows:

(a) Samples of the cable shall be clamped and suspended through holes in a metal bar having a rectangular cross section of 1/2 inch by 5/8 inch. The clamping point shall be immediately above the metal bar; the cord clamp shall rest on top of the metal bar. The cord shall be clamped in such a manner that it will not turn in the hole during the flexing. The through holes in the metal bar shall be 5/8 inch in length and 0.005 to 0.010 in diameter greater than the diameter of the cord which is undergoing test. The through holes in the metal bar shall incorporate a 1/8-inch radius at the end from which the cord emerges (bending point).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:53Z
Check the source to verify that this is the current version before use.

(b) A 3-pound weight shall be hung from the legs of the assemblies with four or more conductors. A 1-pound weight shall be hung from the legs of the assemblies with three or less conductors. The weight shall be attached at a point 4 to 12 inches below the bar to assure that the cord leg is held in a vertical position.

(c) Each conductor of each sample cord; a small low-current-drain 6-volt lamp; and a suitable power source shall be connected in series to indicate electrical continuity (see the figure entitled "Monitor Circuit for Cord Flex Tester" in MIL-C-83501). The metal bar, supported horizontally, shall then be rotated about its longitudinal axis back and forth through an angle of 120 degrees (60 degrees each side of vertical) at a rate of approximately 85 cycles per minute. The arithmetical mean of the flexing cycles of the samples of cord before electrical discontinuity occurs shall be taken as the flexing life of the cord.

4.6.19.2 "Y" junction. Each of the two "y" junctions of the lower cord assembly that conforms to Drawing 358-1321 shall conform to 3.6.18.2 when tested in accordance with the figure entitled ""Y" Joint Flexing Test Set-Up" in MIL-C-83501 and as follows:

(a) The samples shall be clamped and suspended through holes in a metal bar having a rectangular cross section of 1/2 inch by 5/8 inch. The samples shall be clamped in the metal bar so that the samples will be suspended entirely in the vertical position. The samples shall be positioned so that the "y" joint division is at the point where the cord emerges below the metal bar. The cord shall be clamped in such a manner that it will not turn in the hole during flexing. The through holes in the metal bar shall be 5/8 inch in length and 0.005 to 0.010 inch in diameter greater than the diameter of the cord samples. The through holes in the metal bar shall incorporate a 1/8-inch radius at the side from which the cord emerges (bent point).

(b) A length of nylon cord shall be tied to each of the two "y" ends. A 1-pound weight shall be attached to the end of each. Polished drill rods that are 1/2-inch diameter shall be positioned so that the "y" joint is spread open 60 degrees (30 degrees either side of vertical).

(c) The metal bar shall be supported horizontally so that it will rotate about the longitudinal axis going through the point where the cord samples emerge from the bar. The metal bar shall be rotated back and forth through an angle of 120 degrees (60 degrees each side of vertical) at a flexing rate of approximately 85 cycles per minute.

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:53Z
Check the source to verify that this is the current version before use.

(d) Each conductor of each sample cord shall have a low-current-drain monitor circuit (6 VDC source) connected in series to indicate electrical continuity. The arithmetical mean of the flexing of the samples before electrical discontinuity shall be taken as the flexing life.

4.6.20 Isolation. The electrostatic isolation of the lower cord assembly that conforms to Drawing 358-1321 shall be determined in accordance with figure 7. The electromagnetic isolation of the lower cord assembly that conforms to Drawing 358-1321 shall be determined in accordance with figure 8. The electrostatic isolation and the electromagnetic isolation of the lower cord assembly shall be within the limits specified in table I.

4.6.21 Conductor strain relief with connectors. The cable and plug assembly that conforms to Drawing 358-1330 shall be subjected to the test described in 4.6.21.1. Each end of lower cord assembly that conforms to Drawing 358-1321 shall be subjected to the test described in 4.6.21.2.

4.6.21.1 Cable and plug assembly. With the connectors held stationary, the cord shall be gripped at a point at least 3 inches from the connector under test in such a manner that there shall not be any damage to the cord or slippage in the grip. A straight pull in a manner to avoid a sudden jerk on the connector shall be applied to the cable as follows:

(a) A pull of 25 pounds shall be applied to the cable in the direction of the axis of the telephone plug U-174/U for a minimum of 2 minutes.

(b) A pull of 25 pounds shall be applied to the cable in the direction of the axis of the telephone jack U-92A/U for a minimum of 2 minutes.

(c) A pull of 8 pounds shall be applied to the cable in the direction of the axis of the plug connector U-173/U for a minimum of 30 minutes.

(d) A pull of 8 pounds shall be applied to the cable in the direction of the axis of the connector leading to the automatic switch for a minimum of 30 minutes.

4.6.21.2 Lower cord assembly. With the connector held stationary, the cord shall be gripped at a point at least 3 inches from the connector under test in such a manner that there shall not be any damage to the

Source: https://assist.dla.mil -- Downloaded: 20260-26T04:53Z
Check the source to verify that this is the current version before use.

cord or slippage in the grip. A straight pull of 8 pounds shall be applied to the cable, in a manner to avoid a sudden jerk on the connector, in the direction of the cord-connector axis for a minimum of 30 minutes.

5. PACKAGING

5.1 Preservation and packaging

5.1.1 Cleaning and drying. Cleaning and drying of the masks shall be in accordance with MIL-STD-1359.

5.1.2 Levels A and C. Preservation and packaging of the masks for levels A and C shall be the same and shall be in accordance with MIL-STD-1359.

5.2 Packing. Packing shall be level A, B, or C as specified (see 6.2).

5.2.1 Level A. Masks that have been cleaned, preserved, and packaged as specified in 5.1.1 and 5.1.2 shall be packed in a weather-resistant shipping container that conform to PPP-B-636. The grade of each shipping container, determined by the gross weight and size, shall be limited to the applicable special requirements table of the specification. Where practicable the exterior shipping container shall be of uniform shape and size and of minimum tube and tare. Closure and strapping of the shipping containers shall be in accordance with the appendix of the PPP-B-636.

5.2.2 Level B. Level B packing shall be the same as level A packing except that domestic shipping containers may be used.

5.2.3 Level C. Masks that have been cleaned, preserved, and packaged as specified in 5.1.1 and 5.1.2 shall be packed in shipping containers that will be acceptable to the carrier at the lowest rates and insure safe transportation to the point of delivery. The shipping containers shall comply with the rules and regulations applicable to the mode of transportation.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:53Z
Check the source to verify that this is the current version before use.

5.3 Marking. In addition to any marking required by the contract, interior and exterior containers shall be marked in accordance with MIL-STD-1359 and MIL-STD-129.

6. NOTES

6.1 Intended use. The mask covered by this specification is intended to dispense gaseous oxygen to aircrewmembers during unpressurized emergency descents from altitudes of 40,000 feet or lower.

6.2 Ordering data. Procurement documents should specify the following:

(a) Title, number, and date of this specification

(b) Property loaned or furnished by the Government (see 3.10 and 3.11)

(c) Selection of applicable levels of preservation and packaging and packing (see 5.1.2 and 5.2).

6.3 Qualification. With respect to products requiring qualification, awards will be made only for products which are, at the time set for opening of bids, qualified for inclusion in the applicable Qualified Products List whether or not such products have actually been so listed by the date. The attention of the contractors is called to these requirements, and manufacturers are urged to arrange to have the products that they propose to offer to the Federal Government tested for qualification in order that they may be eligible to be awarded contracts or orders for the products covered by this specification. The activity responsible for the Qualified Products List is the Aeronautical Systems Division (ASD/ENECE), Wright Patterson Air Force Base, Ohio 45433, and information pertaining to qualification of products may be obtained from the activity.

6.4 Batch. A batch of silicone rubber compound shall consist of the silicone rubber compound that is manufactured at one time by the manufacturer of the silicone rubber compound. A batch of the plastic molding material shall consist of the plastic molding material that is manufactured at one time by the manufacturer of the plastic molding material.

Custodian:
Air Force - 11

Reviewer:
Air Force - 99

Preparing activity:
Air Force - 11

Project No. 1660-F135

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:53Z
Check the source to verify that this is the current version before use.

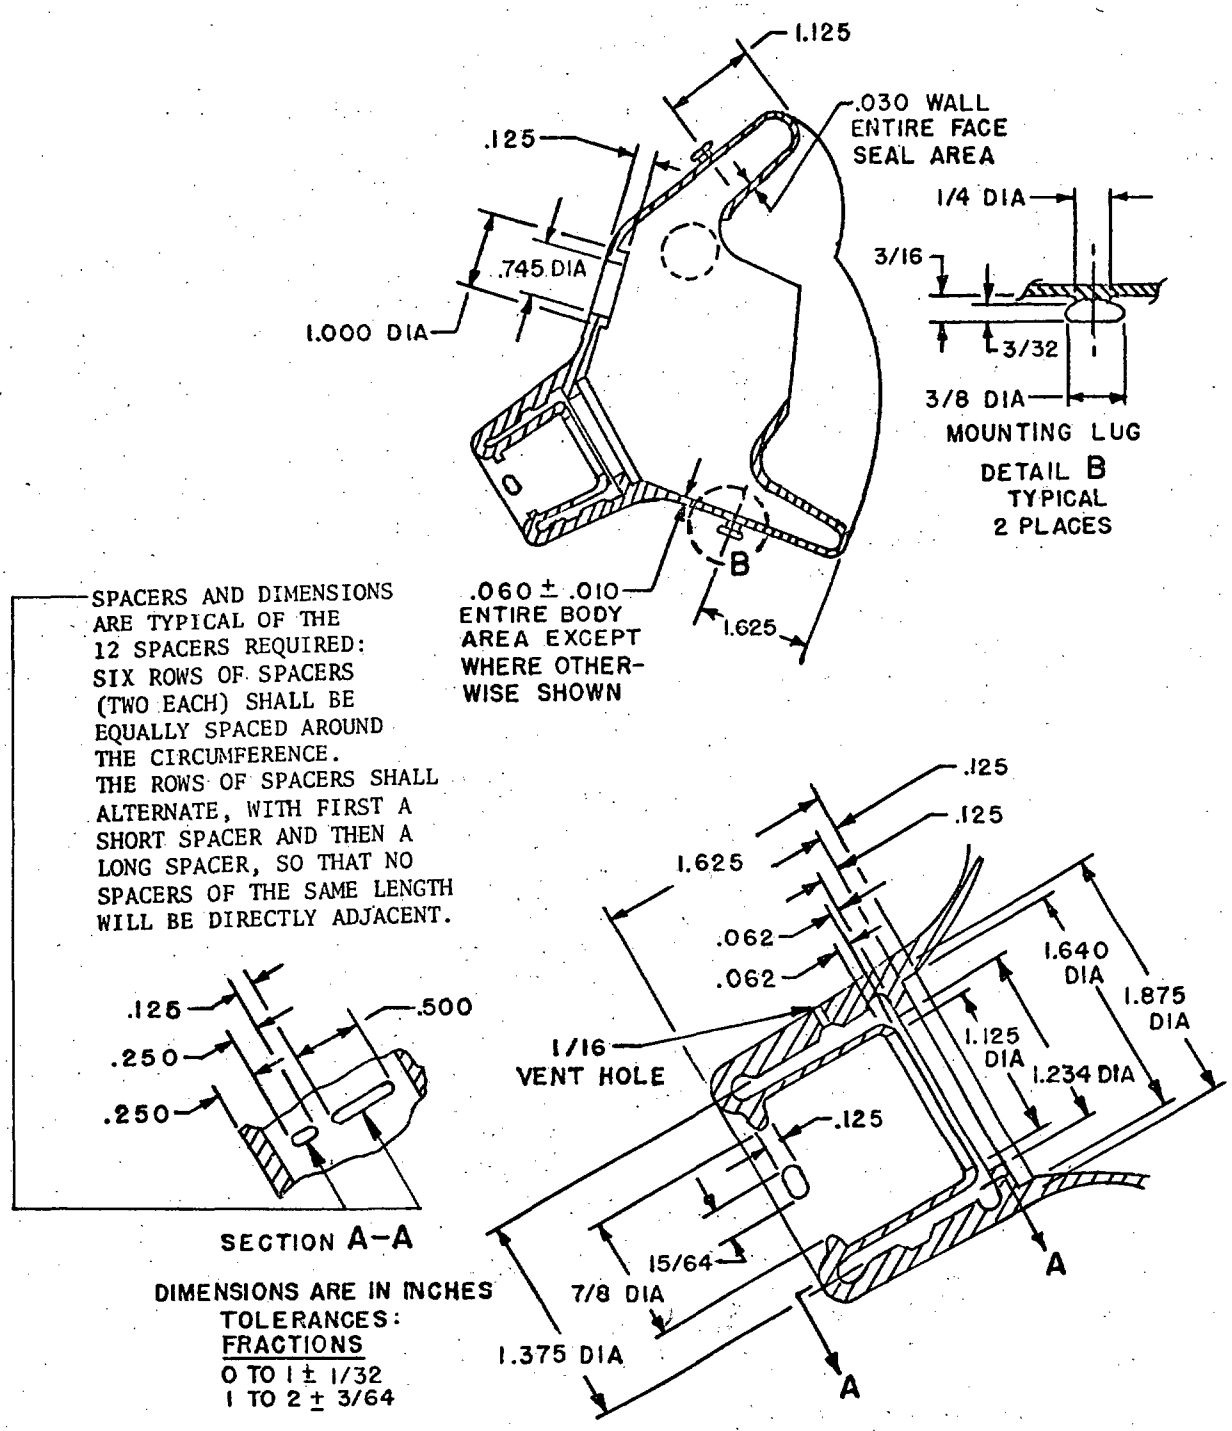


FIGURE 1. Facepiece.

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:53Z
Check the source to verify that this is the current version before use.


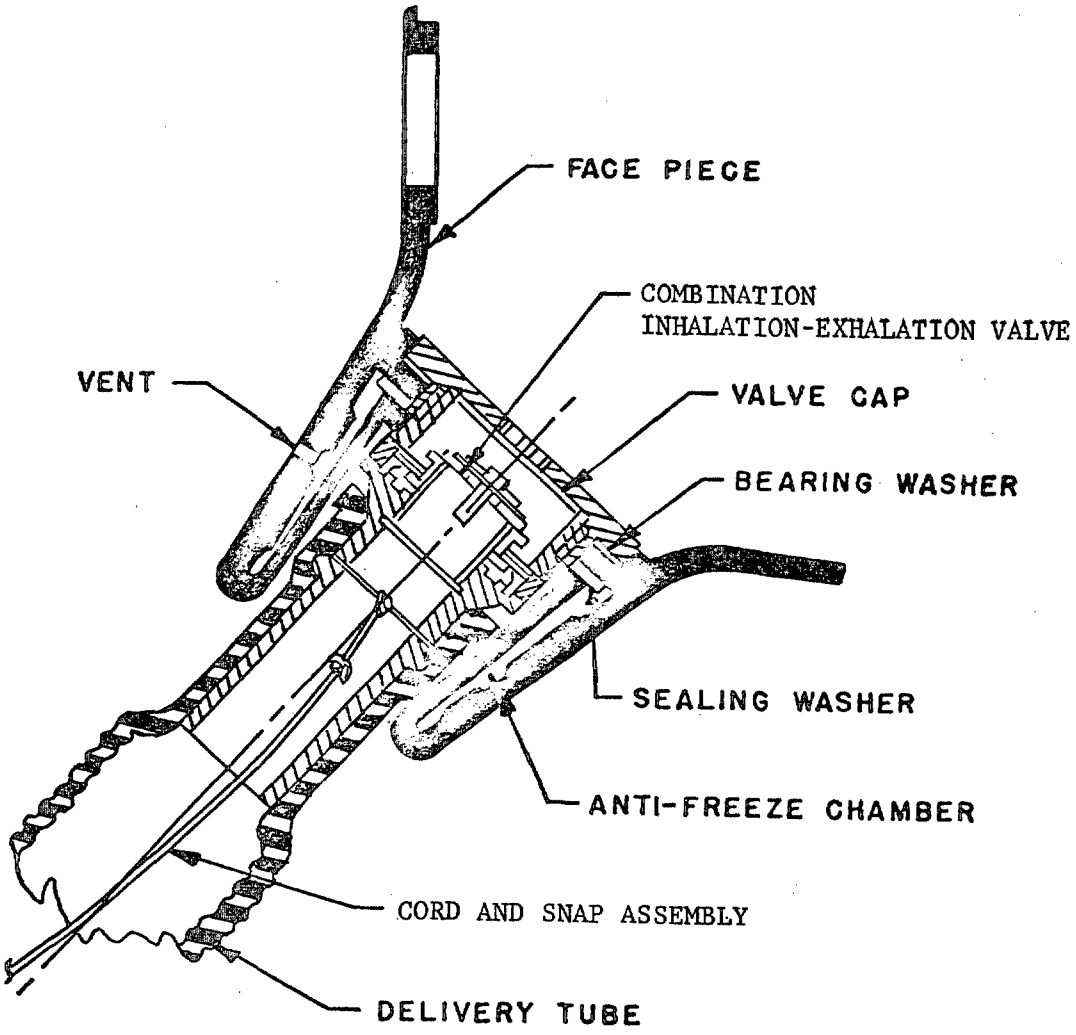


FIGURE 2. Valve installation.

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:53Z
Check the source to verify that this is the currentversion before use.

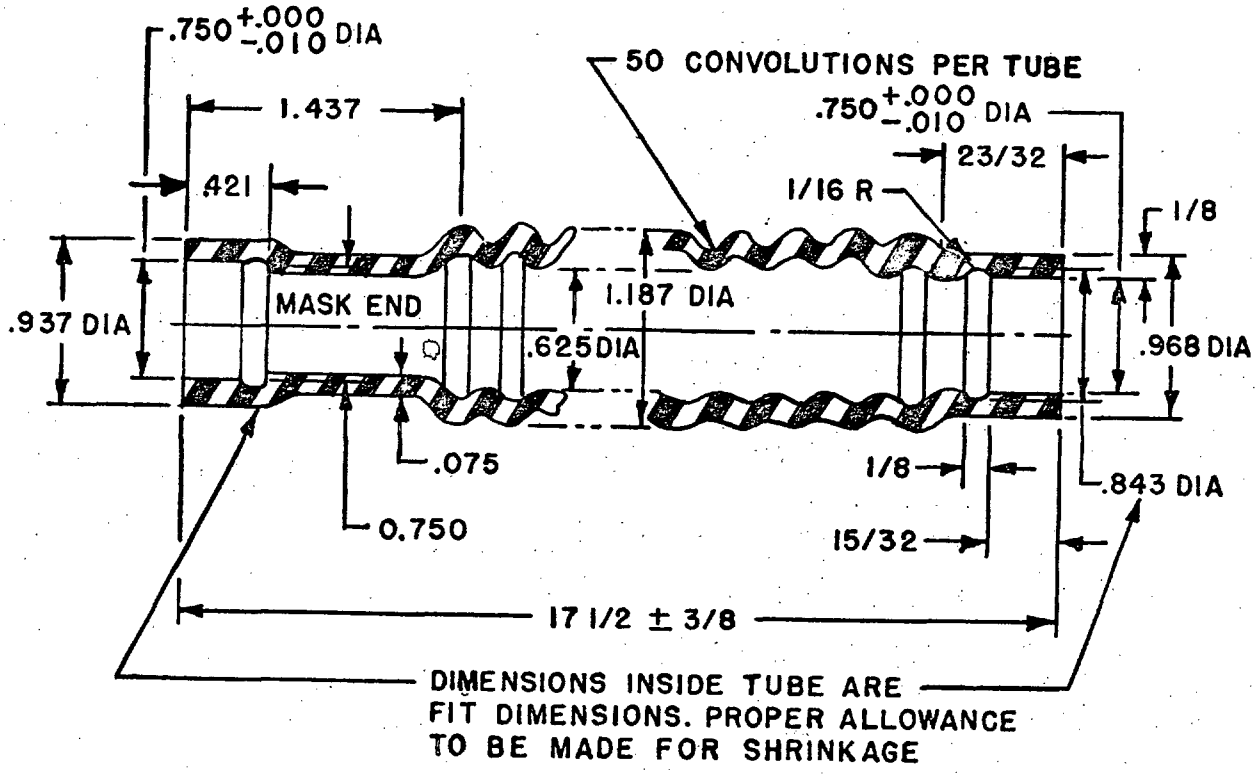


DIMENSIONS IN INCHES

TOLERANCES:

FRACTIONS	DECIMALS
± 1/32	± .010

FIGURE 3. Delivery tube.


Source: https://assist.dla.mil -- Downloaded: 202610-26T04:53Z
Check the source to verify that this is the current version before use.

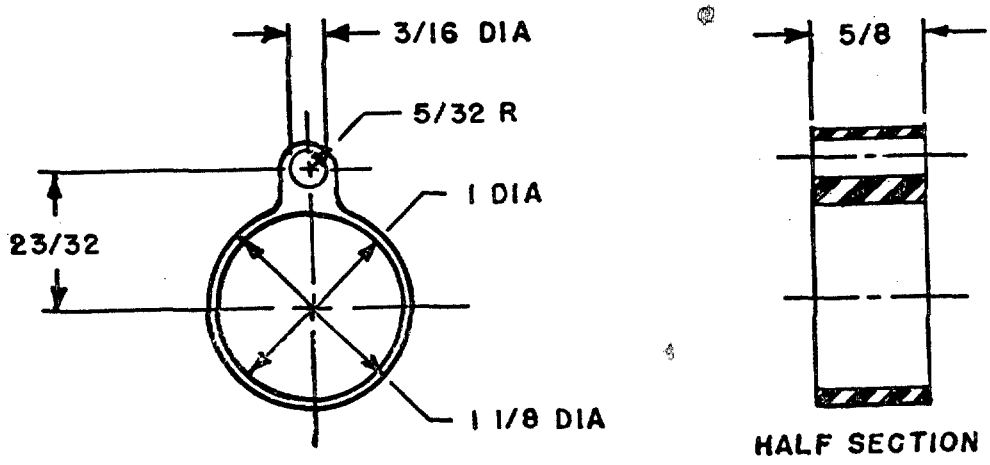

DIMENSIONS IN INCHES
UNLESS OTHERWISE SPECIFIED, TOLERANCE FOR ALL DIMENSIONS ±1/64

FIGURE 4. Lower cable guide.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:53Z
Check the source to verify that this is the current version before use.

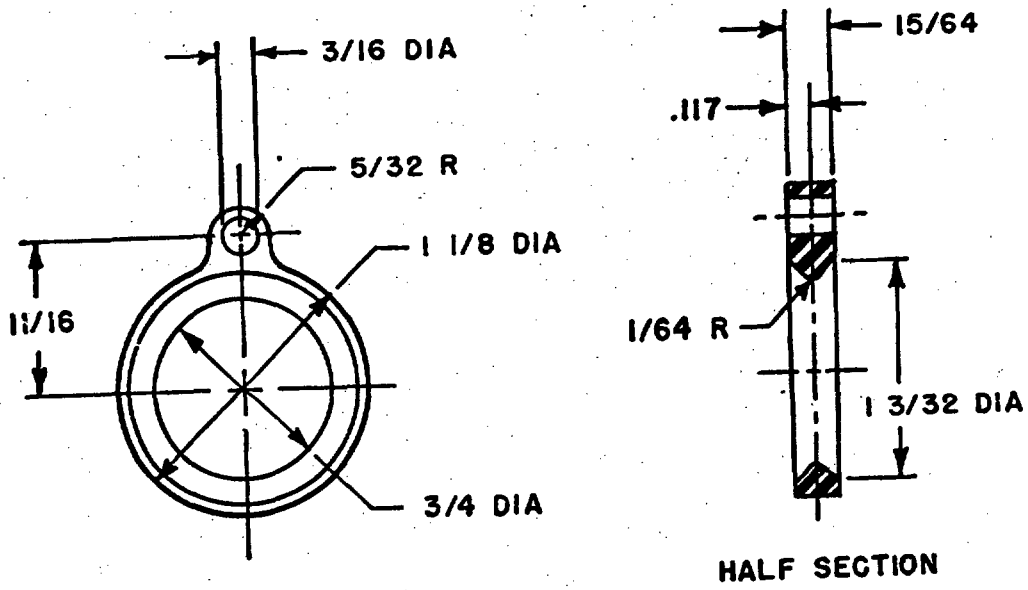

DIMENSIONS IN INCHES
UNLESS OTHERWISE SPECIFIED, TOLERANCE FOR ALL DIMENSIONS ±1/64

FIGURE 5. Upper cable guide.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:53Z
Check the source to verify that this is the current version before use.

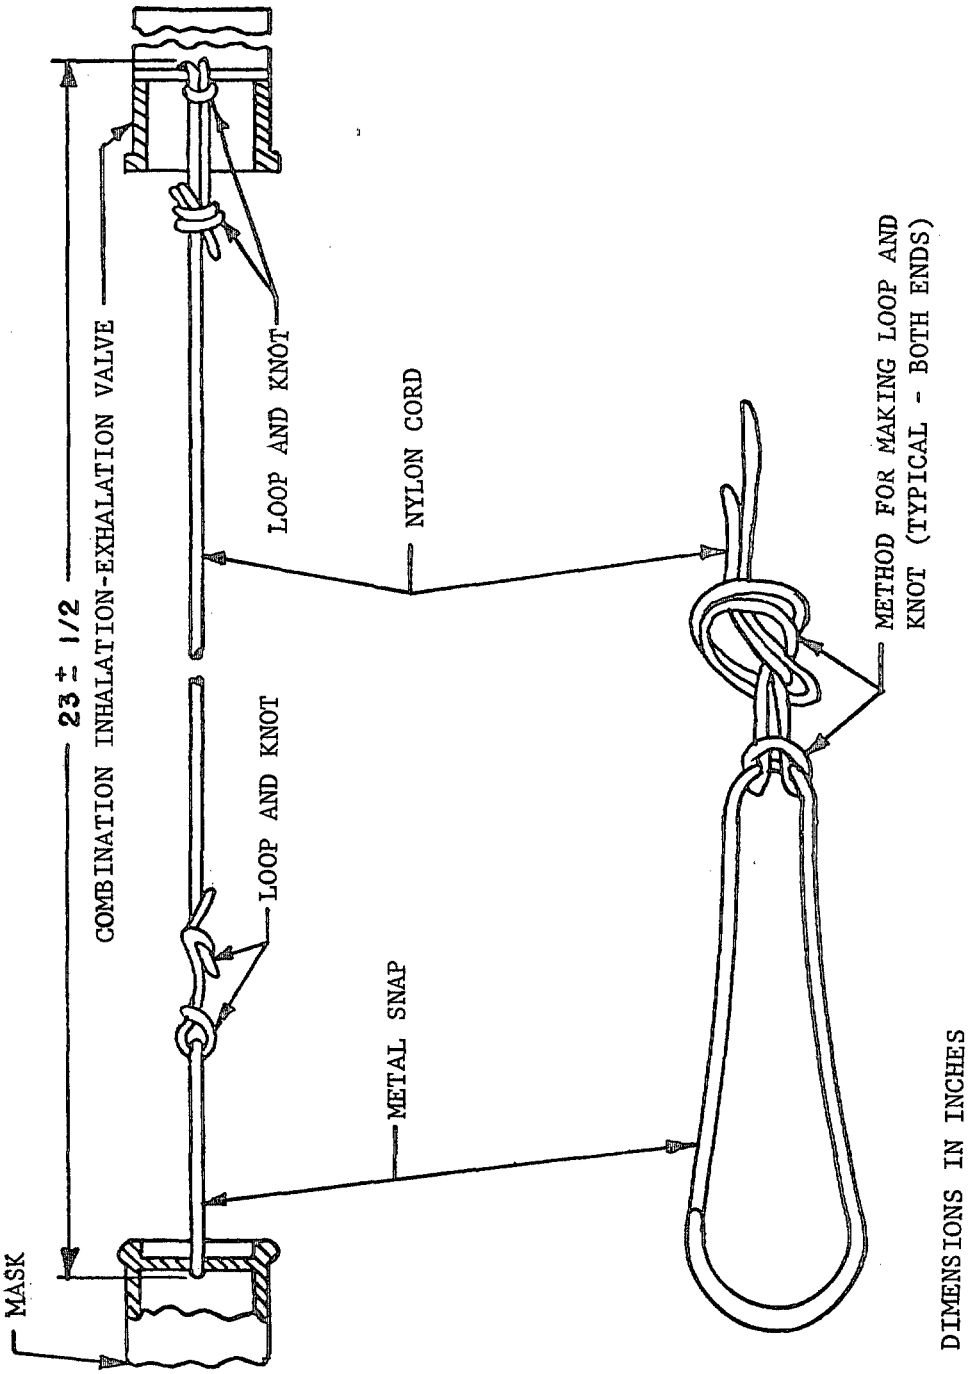


FIGURE 6. Cord and snap assembly.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:53Z
Check the source to verify that this is the current version before use.

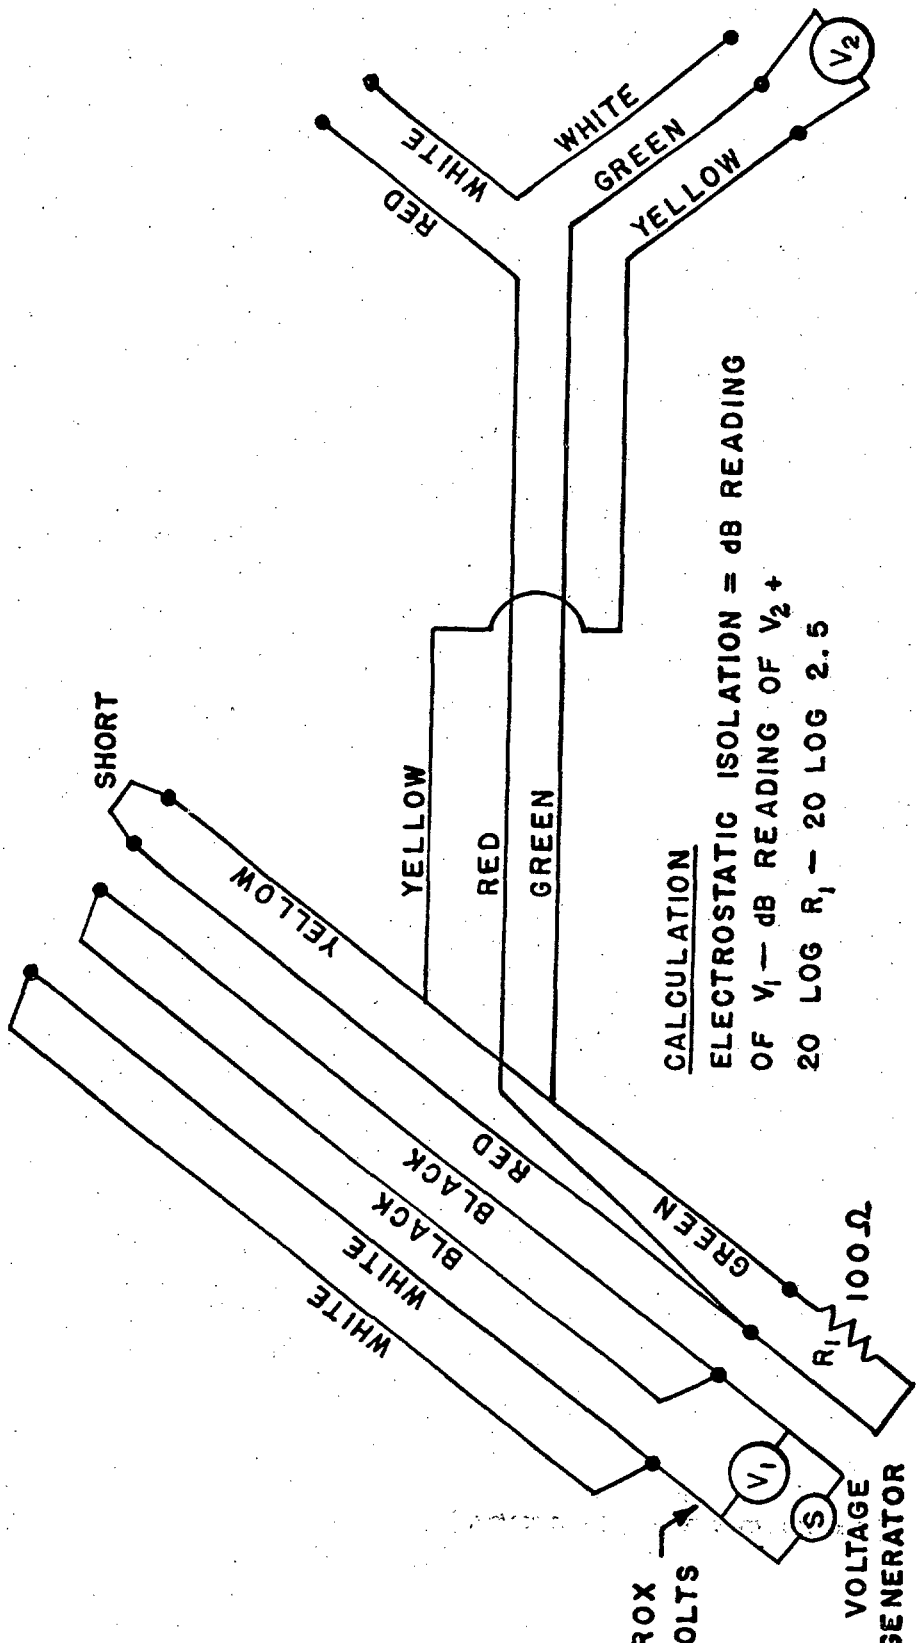


FIGURE 7. Electrostatic isolation test.

Source: https://assist.dla.mil -- Downloaded: 2026-10-16T14:53Z
Check the source to verify that this is the current version before use.

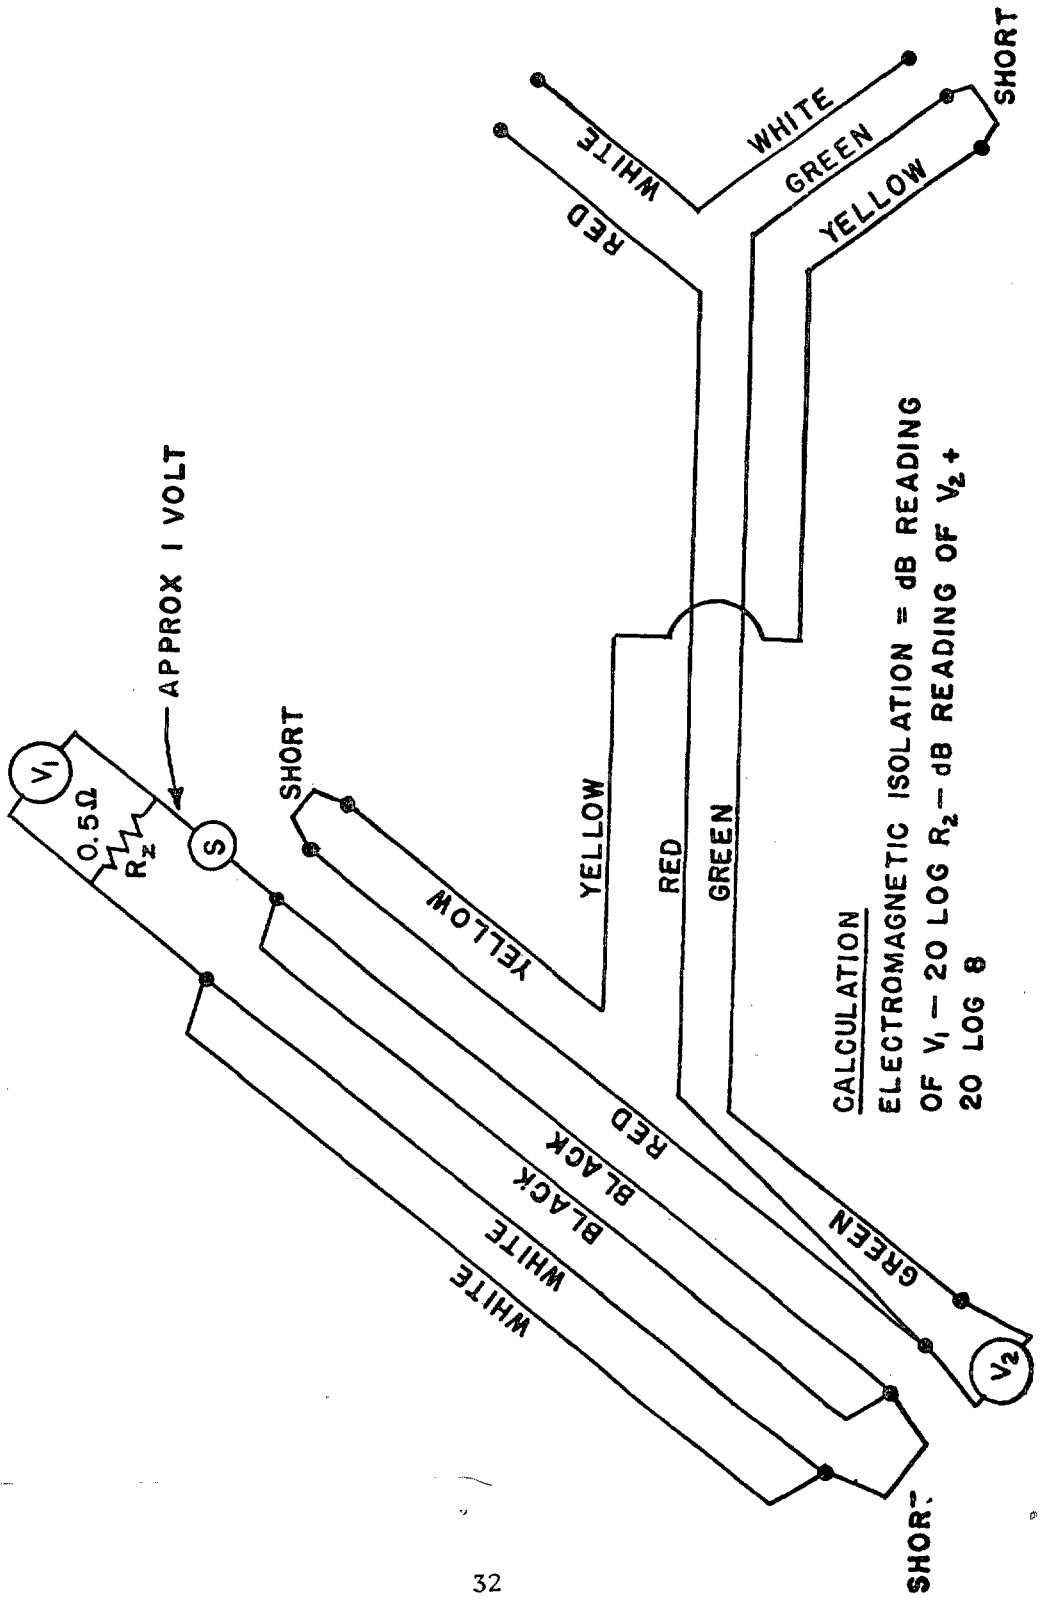


FIGURE 8. Electromagnetic isolation test.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:53Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS: This form is provided to solicit beneficial comments which may improve this document and enhance its use. DoD contractors, government activities, manufacturers, vendors, or other prospective users of the document are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity. A response will be provided to the submitter, when name and address is provided, within 30 days indicating that the 1426 was received and when any appropriate action on it will be completed.

NOTE: This form shall not be used to submit requests for waivers, deviations or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

DOCUMENT IDENTIFIER *(Number)* AND TITLE

NAME OF ORGANIZATION AND ADDRESS OF SUBMITTER

☐ VENDOR ☐ USER ☐ MANUFACTURER

1. ☐ HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE? ☐ IS ANY PART OF IT TOO RIGID, RESTRICTIVE, LOOSE OR AMBIGUOUS? PLEASE EXPLAIN BELOW.

A. GIVE PARAGRAPH NUMBER AND WORDING

B. RECOMMENDED WORDING CHANGE

C. REASON FOR RECOMMENDED CHANGE(S)

2. REMARKS

SUBMITTED BY *(Printed or typed name and address — Optional)*

TELEPHONE NO.

DATE

DD FORM 1426 1 OCT 76 PREVIOUS EDITION WILL BE USED.

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:53Z
Check the source to verify that this is the current version before use.