A-A-51916A
19 May 1989
SUPERSEDING
A-A-0051916(DM)
1 May 1987

COMMERCIAL ITEM DESCRIPTION

FORCEPS, COAGULATION (Gerald)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers one size and type of Gerald coagulation forceps for use in electrosurgery using a bipolar coagulator.

Salient characteristics:

General. The forceps shall be suitable for use under irrigation fluids and in a bloody surgical field.

Material. Forceps shall be manufactured from Class 6 or Class 4 corrosion-resistant steel of composition in accordance with American Society for Testing and Materials (ASTM) Designation F899. Connector pins shall be manufactured from Class 3 corrosion-resistant steel in accordance with ASTM Designation F899.

Hardness. Forceps manufactured from Class 6 corrosion resistant steel shall have a Rockwell Hardness B Scale (HRB) of 90 to 110. Forceps manufactured from Class 4 corrosion resistant steel shall have a Rockwell Hardness C Scale (HRC) of 40 to 47 when tested in accordance with ASTM Designations E18 or E92 whichever is applicable. Conversion of hardness values shall be in accordance with ASTM Designation E140.

Style and design. Forceps shall be in accordance with Figure 1. Forceps tips shall be well-rounded and shall meet exactly when the forceps are closed in the normal manner (i.e., with no lateral pressure exerted by the user). Connector pin tips shall also be well rounded.

Epoxy and plastic materials used in the manufacture of the forceps shall be capable of repeated steam sterilization.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:02Z
Check the source to verify that this is the current version before use.

Passivation. The metal parts of the forceps shall be passivated.

Finish. The finish of the forceps shall be mirror or satin. The finish shall be uniform and free from burrs, pits, rough areas, and grind or tool marks.

Corrosion resistance. Forceps shall show no signs of corrosion when tested in accordance with ASTM Designation F1089.

Identification marking and labeling. Forceps shall be permanently marked with the contractor's name or registered trademark and the word "stainless." In addition, forceps of foreign manufacture shall bear the name of the country of manufacture.

Workmanship. Forceps shall be free from defects which detract from its appearance or impair its serviceability.

Product Quality Level

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Each (EA). One forceps, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:02Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual) or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemcial properities) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for examination purposes shall be one forceps. Sampling shall be inspection level II with an acceptable quality level (AQL) of 1.0.

Examination. Forceps shall be examined to determine compliance with all requirements contained in this specification.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one forceps. Sampling shall be inspection level S-2 with an AQL of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Electrical tests. Forceps shall be tested for continuity (connector pins-to-tip) and resistance (across insulated surfaces).

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specification, standard, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:02Z
Check the source to verify that this is the current version before use.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerance specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:02Z
Check the source to verify that this is the current version before use.

NOTE 1: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-188-5340	FORCEPS, COAGULATION, Gerald, Bipolar, Straight, 7-1/4 inch (18.4 cm) Long, 0.87 mm Wide Tip

NOTE 2: The forceps shall be suitable for use with the following National Stock Number:

NSN	ITEM IDENTIFICATION
6515-01-139-7942	CORD, ELECTROSURGICAL, Bipolar

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM


CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPOAS

PGC 59952

Project No. 6515-4605

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:02Z
Check the source to verify that this is the current version before use.

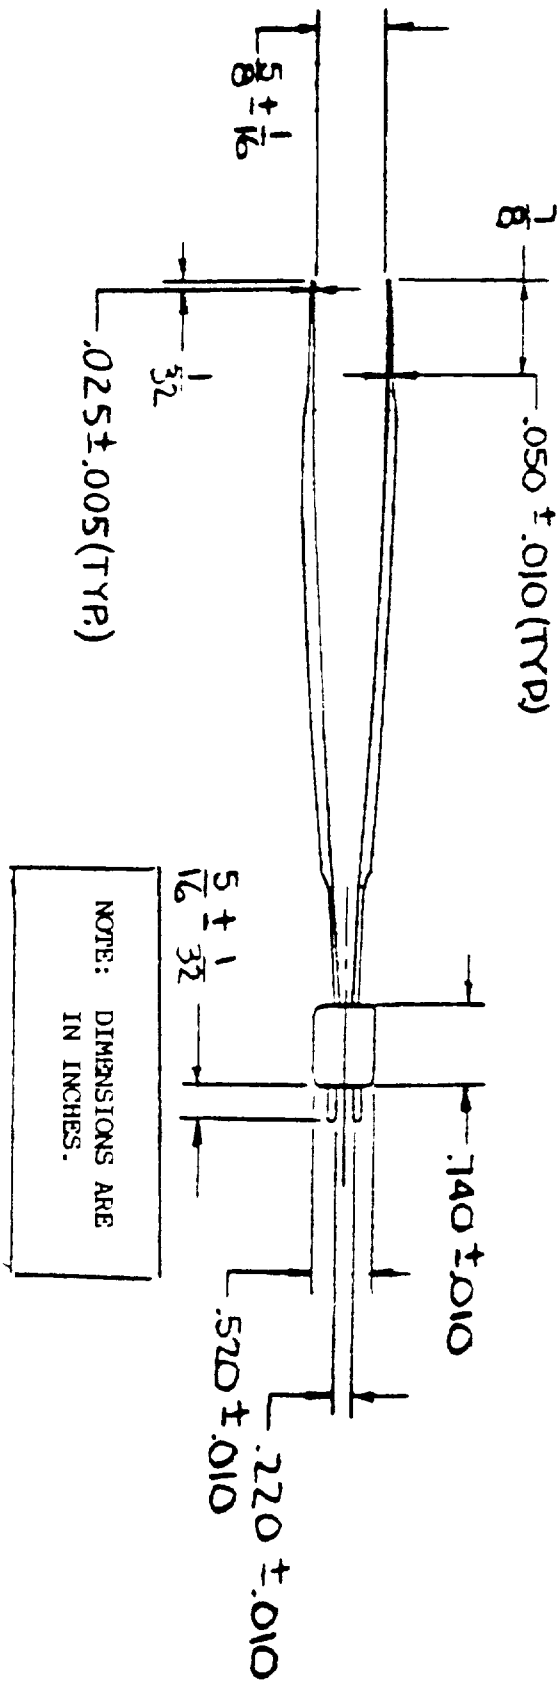

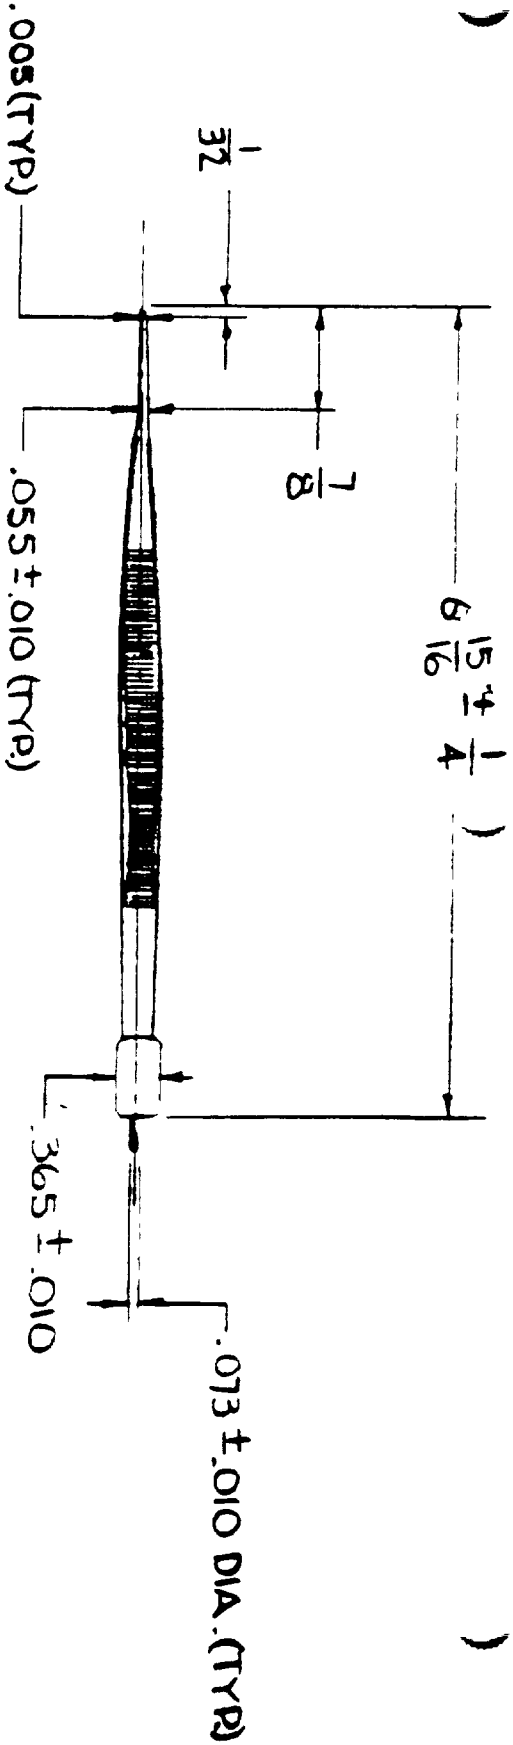


FIGURE 1. FORCEPS, COAGULATION (GERALD)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:02Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems Enter in block 6 any remarks not related to a specific paragraph of the document If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered

NOTE This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements

(Fold along this line)

(Fold along this line)

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 Alexandria, VA

POSTAGE WILL BE PAID BY

Commander
Defense Personnel Support Center
ATTN: DPSC-RSTC
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:02Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1 DOCUMENT NUMBER	2 DOCUMENT TITLE
A-A-51916A	FORCEPS, COAGULATION (Gerald)

3a NAME OF SUBMITTING ORGANIZATION	4 TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
b ADDRESS *(Street, City, State, ZIP Code)*	☐ USER
	☐ MANUFACTURER
	☐ OTHER *(Specify)* _____

5 PROBLEM AREAS

a Paragraph Number and Wording

b Recommended Wording

c Reason/Rationale for Recommendation

6 REMARKS

7a NAME OF SUBMITTER *(Last, First, MI)* – Optional	b WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8 DATE OF SUBMISSION *(YYMMDD)*

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:02Z
Check the source to verify that this is the current version before use.