METRIC

A-A-51922A
6 April 1992
SUPERSEDING
A-A-0051922(DM)
10 February 1988

COMMERCIAL ITEM DESCRIPTION

DIAPHRAGM, VAGINAL (Arcing)

The General Services Administration has authorized the use of this commercial item description as a replacement for Military Specification MIL-D-36691 which is cancelled.

This commercial item description covers five sizes of arcing vaginal diaphragms.

Salient Characteristics:

Classification. Diaphragms shall be of the following types:

Type I - Compressible at any point along the rim
Type II - Compressible at two marked pressure points on the rim.

General. The diaphragm shall meet the requirements of ASTM D3899 for Type 3 diaphragms. The diaphragm shall be an arcing type, and shall be in accordance with Figure 1. Correct diaphragm placement shall be achieved without an inserter.

The diaphragm spring shall be manufactured in such a manner as to resist distortion, saddling, or permanent deformation when the diaphragm is repeatedly folded and unfolded.

The Type I diaphragm spring shall be a continous steel coiled spring. The Type II rim or perphery shall contain a conventional steel arcing pegs with an insert. Both Type I and Type II springs shall be completely encapsulated in rubber.

The Type II diaphragm shall have two permanent markings on the rim indicating the pressure points for folding.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

The diaphragm shall include a reusable rigid plastic carrying case.

Material. Diaphragm shall be fabricated from silicone or other suitable synthetic rubber.

Contraceptive jelly. Only type II diaphragms shall be supplied with a minimum of 26 grams of contraceptive jelly.

Instructions. Each diaphragm shall be provided with an instruction booklet detailing function of the diaphragm, when the diaphragm should be inserted and removed, technicques for correct insertion and removal with appropriate anatomy illustrations, and instructions for proper care of the diaphragm.

Tests and examinations. Diaphragms shall be tested and examined in accordance with all applicable inspections and sampling levels of ASTM Designation D3899.

In addition, rubber material shall be tested in accordance with the Muscle Implatation Test and Intracutaneous Tests of the United States Pharmacopeia(See certificate of biocompatibility). Diaphragm shall be non-toxic and non-pyrogenic in accordance with United States Pharmacopeia (USP) requirements.

Workmanship. The diaphragm shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One diaphragm of the type and millimeter (mm) specified, constitutes one unit.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Certificate of biocompatibility. A certificate of compliance, stipulating that offered items meet the biocompatibility test, shall be acceptable, provided that the contractor has supplied acceptable items to the Government within the past three years and that there has been no changes to material, formulation and the method of processing since actual testing was performed. The certificate shall include the date the testing was performed, the test method and results, the name and title of the person evaluating the results, the current contract number and National Stock Number (NSN), a statement certifying that material processing and formulation have not changed since the time that biocompatibility was performed and the signature and title of the person making the certification.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers'own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

NOTE: The following National Stock Numbers, Types and Item Identifications are covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION	TYPE
6515-00-935-1025	DIAPHRAGM, VAGINAL, Rubber, Contoured, Arcing, 70 mm	I
6515-00-935-1026	DIAPHRAGM, VAGINAL, Rubber, Contoured, Arcing, 75 mm	I
6515-00-935-1028	DIAPHRAGM, VAGINAL, Rubber, Contoured, Arcing, 80 mm	I

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION	TYPE
6515-01-044-5531	DIAPHRAGM, VAGINAL, Rubber, Contoured, Arcing, 80 mm	II
6515-01-044-8310	DIAPHRAGM, VAGINAL, Rubber, Contoured, Arcing, 70 mm	II
6515-01-044-8311	DIAPHRAGM, VAGINAL, Rubber, Contoured, Arcing, 75 mm	II
6515-01-047-3902	DIAPHRAGM, VAGINAL, Rubber, Contoured, Arcing, 65 mm	I
6515-01-048-9692	DIAPHRAGM, VAGINAL, Rubber, Contoured, Arcing, 85 mm	I

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM


CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project No. 6515-4930
Location: AA51922/S11


Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

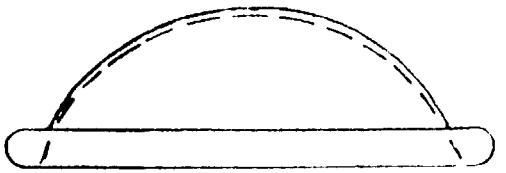


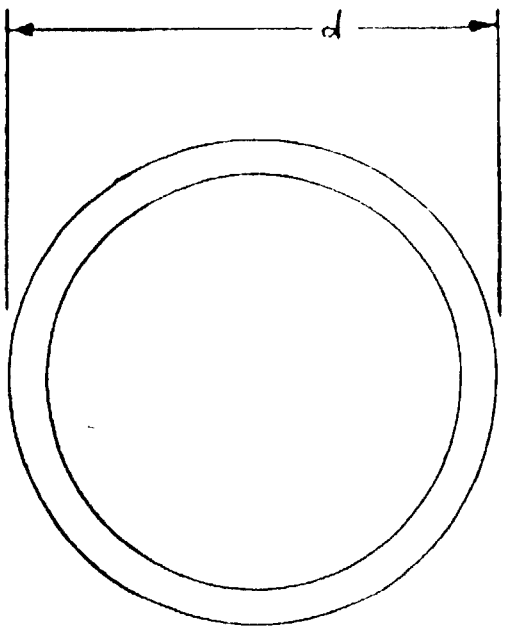

UNFOLDED

d = LABEL MILLIMETER SIZE ± 2 MM

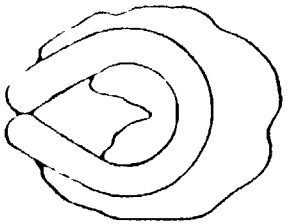

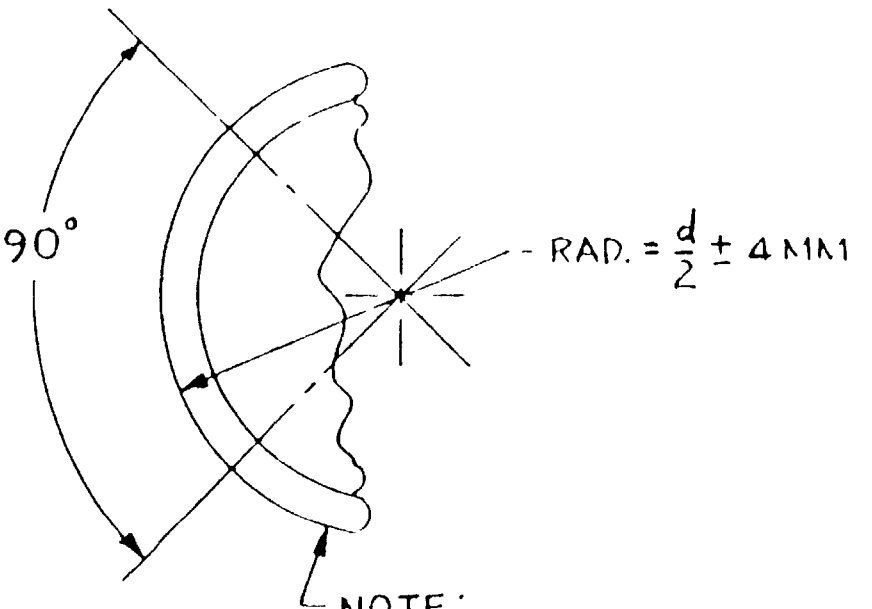

NOTE:
ENDS MAY DEVIATE
FROM RADIUS SHOWN.

FOLDED

FIGURE 1 ARCING DIAPHRAGM

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER	2 DOCUMENT DATE (YYMMDD)
	A-A-51922A	6 April 1992

3 DOCUMENT TITLE
DIAPHRAGM, VAGINAL (Arcing)

4 NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5 REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code) (1) Commercial	(2) AUTOVON
Defense Personnel Support Center ATTN: DPSC-MSE	(215)7372870	444-2870
c. ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.