A-A-51940A
13 November 1989
SUPERSEDING
A-A-0051940 (DM)
15 JUNE 1987

COMMERCIAL ITEM DESCRIPTION

RETRACTOR, ORAL (Obwegeser, 14 by 70 mm Curved Downward)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a retractor of Obwegeser design, suitable for use in oral surgery procedures.

Salient characteristics:

General. The retractor shall be in accordance with the applicable requirements as specified herein.

Material. The retractor shall be fabricated of Class 4, martensitic stainless steel shown in Table 2 of ASTM-F899. After proper heating, the finished Rockwell hardness shall be C45 to C50, as specified in ASTM-E18. The retractor shall have a satin or matte finish. The matte finish shall exhibit a uniform nondirectional surface texture equivalent to that produced by lightly blasting the prepared surface with fine abrasives under pressure. The retractor shall be properly passivated. The retractor shall comply with the Boil and Copper Sulfate tests of ASTM-F1089, for Class 4 stainless steel.

Style, design and dimensions. The retractor shall be an Obwegeser Number 167 with a blade curved downward. The retractor shall be in accordance with Figure 1 for style, design and dimensions.

Marking. The retractor shall be marked with the name or registered trademark of the contractor. The retractor shall have the word "stainless" marked on the instrument. If the retractor is of foreign manufacture, the instrument shall be marked with the country of origin.

Workmanship. The retractor shall be free of burs, cracks, rough edges or any other defects that will detract from its appearance or impair its serviceability.

Unit. Each (EA). One retractor, as specified, constitutes one unit.

AMSC N/A FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

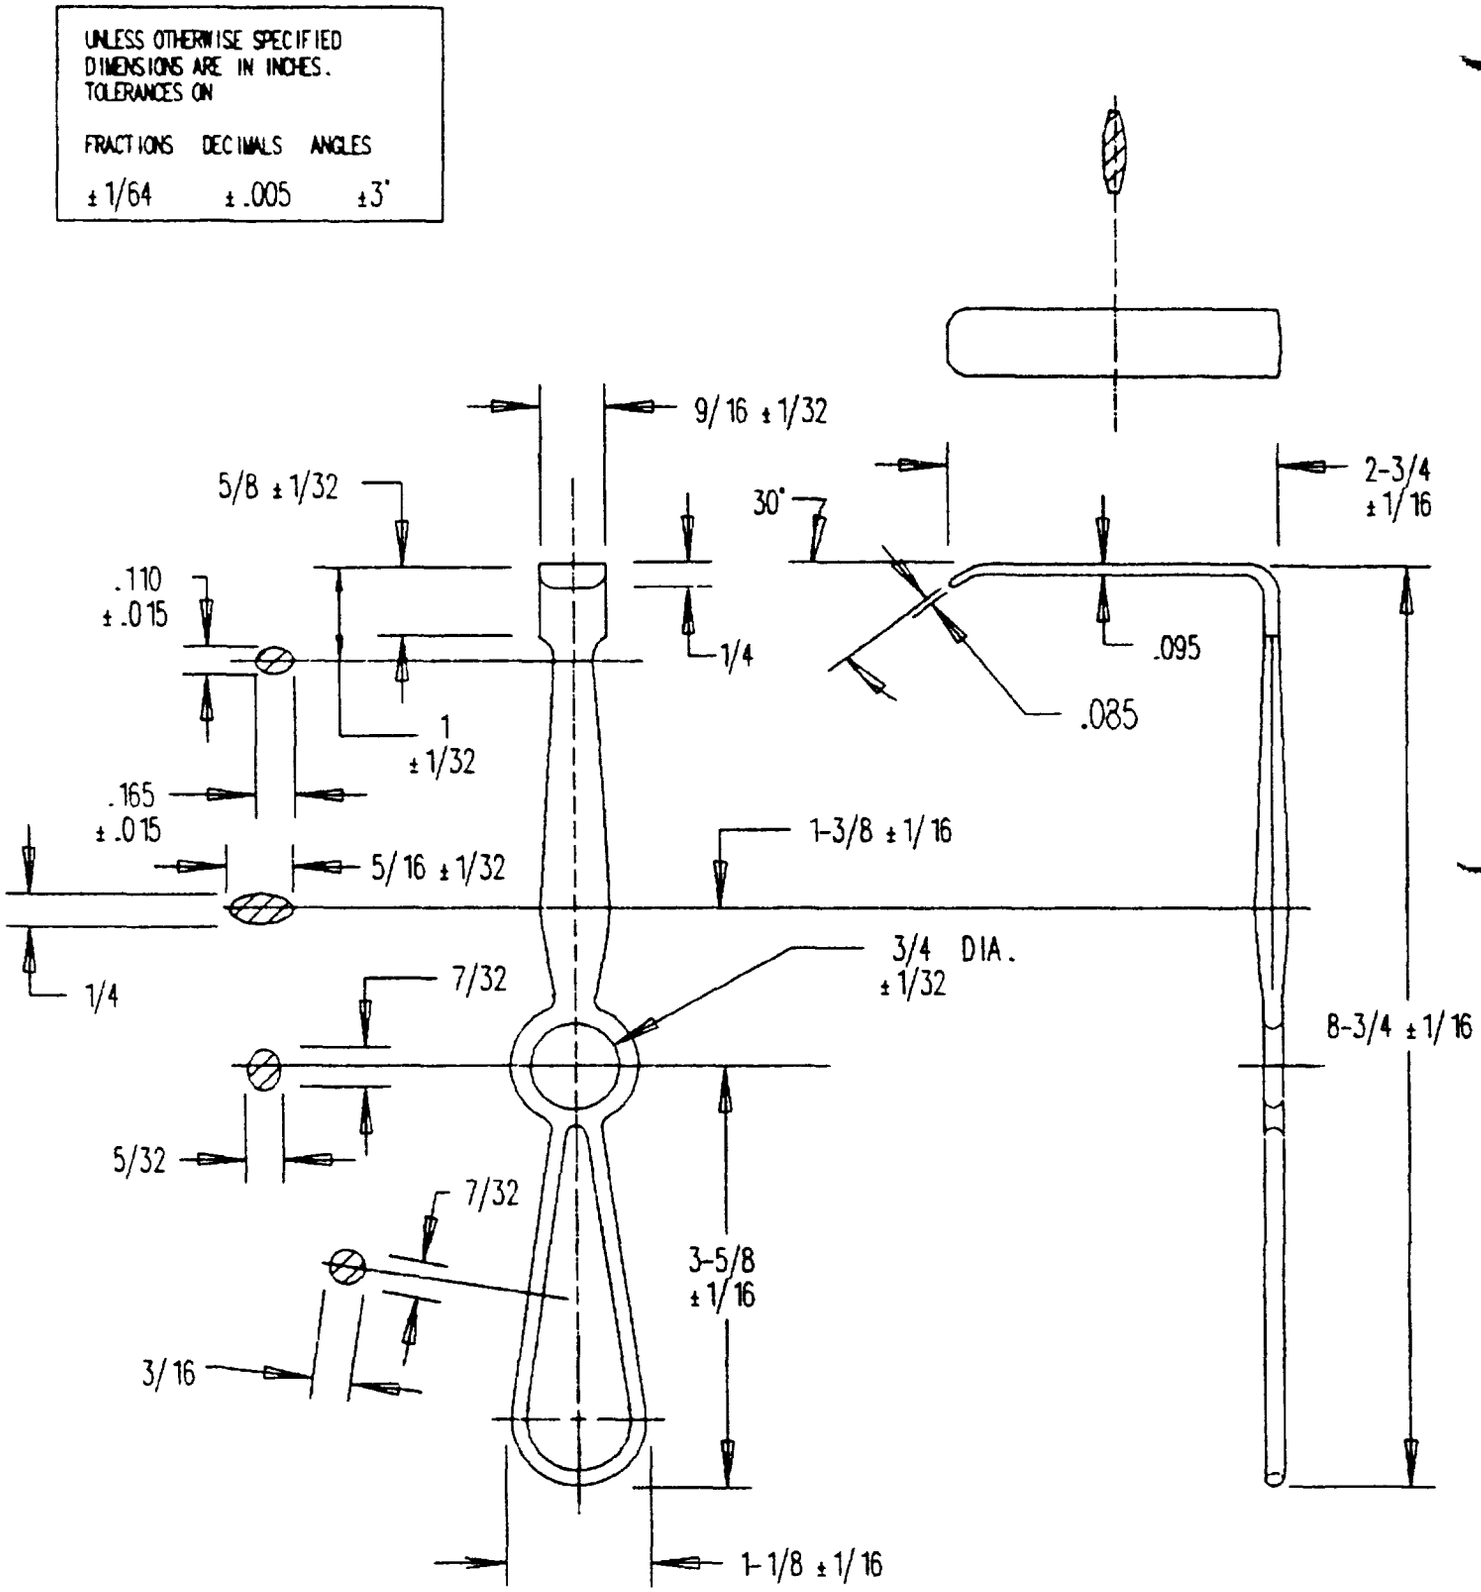


FIGURE 1
RETRACTOR, ORAL, OBWEGESER DESIGN

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

Unit package. Each retractor shall be wrapped in an anti-corrosive material and packed in a durable pouch or box.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more tests characteristics.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, with an inspection level of II except for dimensions the inspection level shall be S-1. Examination shall include but not limited to the following:

Defects

Design not as specified.
Retractor finish not as specified.
Operative end not free from cracks, grind marks, burrs, feathers, or other imperfections.
Retractor dimensions not as specified.
Instrument not permanently and legibly marked with name or trademark of the contractor or stainless.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105. The unit of product for test purposes shall be one retractor, with an inspection level of S-1.

Contractor certification. The contractor shall certify that the product offered meets the salient characterisitcs of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch/pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met. If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable. The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administraction to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Note: The following National Stock Number is covered by this document:

National Stock Number	Item Identification
6520-01-137-8455	RETRACTOR, ORAL, OBWEGESER DESIGN

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6520-2113

59802

Location: NCR Disk #CID 6

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE: This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
Attn: DPSC-RSTE
2800 South 20th Street
Philadelphia, PA 19101

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-51940A	RETRACTOR, ORAL (Obwegeser 14 by 70 mm Curved Downward)

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR ☐ USER ☐ MANUFACTURER ☐ OTHER *(Specify)* _____
b. ADDRESS *(Street, City, State, ZIP Code)*	

5. PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

DD FORM 82 MAR 1426 PREVIOUS EDITIONS ARE OBSOLETE

Source: https://assist.dla.mil - Downloaded: 2026-04-26T09:03Z
Check the source to verify that this is the current version before use.