INCH-POUND

A-A-54897
23 July 1993

COMMERCIAL ITEM DESCRIPTION

BRACE, BIT, BONE, CRANIAL, HUDSON, AND BURS, DRILL AND EXTENSION

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Military Specification MIL-B-37246, which is cancelled.

This Commercial Item Description covers a cranial bone brace of the Hudson design and associated burs, drills and extension used in neurological surgery.

Salient characteristics:

The brace, burs, drills and extension shall be in accordance with the applicable requirements of ASTM 899-84, and the following options under that specification:

Material. The brace shall be fabricated from Class 3, Types 302, 303, or 304 or Class 4, Type 420 material. The extension shall be fabricated from Class 3, Types 302, 303 or 304 or Class 4, Type 420 material. The four burs shall be fabricated from Class 4, Type 420F material, except that the minimum carbon content shall be 0.30 percent.

The drill shall be fabricated from Class 4, Type 420 material except the minimum carbon content shall be 0.30 percent.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Hardness. Hardness shall be as indicated for the following types of steel:

Type 302, 303, or 304	Rockwell RB 75-100
Type 420	Rockwell RC 40-45, after proper stress relieving
Type 420F	Rockwell RC, 50-55, after proper stress relieving
Type 440C	Rockwell Hardness 58 (to 62 C) after proper stress relieving.

Style, design and dimensions. Shall be in accordance with Figure 1 of this specification and as follows:

The Brace, Bit, Bone, Cranial, Hudson shall be a cranial drill brace of the Hudson design, suitable for use in surgical procedures of the human skull. The brace shall be constructed to adequately accommodate the burs, drills, and extension described in this specification. The brace shall be supplied with a set screw for fastening the burs, drill and extension into the chuck of the brace.

The Extension, Bone Bit Brace, Cranial, Hudson, 4 inch shall be an extension attachment for use with cranial drill brace of the Hudson design. The extension shall be supplied with a set screw for fastening the burs and drill described in this specification. The proximal end of the extension shall be designed to fit into the chuck of the drill base specified. The extension shall be suitable for surgical procedures involving the human skull.

The Bur, Cranial, Hudson, 14 millimeters (mm) shall be a cranial bur of the Hudson design. The bur shall have 9 flutes, 14 mm in diameter. The bur shall be suitable for use with the Hudson Cranial Brace in enlarging trephine openings in the human skull.

The Bur, Cranial, Hudson, 20 mm shall be a cranial bur of the Hudson design. The bur shall have 8 flutes, 20 mm in diameter. The bur shall be suitable for use with the Hudson Cranial Brace in enlarging trephine openings in the human skull.

The Bur, Cranial, Hudson, 16 mm shall be a cranial bur of the Hudson design. The bur shall have 8 flutes, 16 mm in diameter. The bur shall be suitable for use with the Hudson Cranial brace in enlarging trephine opening in the human skull.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

The Bur, Cranial, Hudson, 9 mm shall be a cranial bur of the Hudson design. The bur shall have 6 flutes, 9 mm in diameter. The bur shall be suitable for use with the Hudson Cranial Brace in enlarging trephine openings in the human skull.

The Drill, Flat, Cranial, Cushing, 3/8 inch shall be a flat, cranial perforating drill of the Cushing design. The drill shall be suitable for use with the Hudson Cranial Brace in trephining openings in the human skull.

Finish. Finish shall be mirror or mirror and satin.

Passivation. All material shall be properly passivated.

Identification marking and labeling. The brace, burs, drills and extension shall be legibly marked with the contractor's name of trademark and the word "stainless". Foreign manufactured items shall be legibly marked with the name of the country of origin.

Certificate of biocompatibility. A certificate of compliance, stipulating that offered items meet the biocompatibility test, shall be acceptable, provided that the contractor has supplied acceptable items to the Government within the past three years and that there has been no changes to material, formulation and the method of processing since actual testing was performed. The certificate shall include the date the testing was performed, the test method and results, the name and title of the person evaluating the results, the current contract number and National Stock Number, a statement certifying that material processing and formulation have not changed since the time that biocompatibility was performed and the signature and title of the person making the certification.

Workmanship. The brace, burs, drill and extension shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA).

For 6515-00-312-4125, One cranial bur with a 9 flutes, 14 mm in diamter, as specified, constitutes one unit.

For 6515-00-312-4130, One cranial bur with a 8 flutes, 20 mm in diameter, as specified, constitutes one unit.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

For 6515-00-312-4260, One bone bit brace extension, as specified, constitutes one unit.

For 6515-00-515-2113, One cranial drill brace, as specified, constitutes one unit.

For 6515-00-515-2114, One cranial bur, with a 6 flutes, 9 mm in diameter, as specified, constitutes one unit.

For 6515-00-515-2115, One cranial bur with a 8 flutes, 16 mm in diameter, as specified, constitutes one unit.

For 6515-00-515-2116, One flat drill, as specified, constitutes one unit.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspection are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for examination purposes shall be one brace; bur; drill; or extension as specified. Sampling shall be inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for test purposes shall be one brace, or drill, or bur or extension. Sampling shall be inspection level S-2 with an AQL of 1.0.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

NOTE: The following National Stock Numbers and their respective Item Identifications are covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION
6515-00-312-4125	BUR, CRANIAL, HUDSON, 14 mm
6515-00-312-4130	BUR, CRANIAL, HUDSON, 20 mm
6515-00-312-4260	EXTENSION, BONE BIT BRACE CRANIAL, HUDSON, 4 inch
6515-00-515-2113	BRACE, BIT, BONE, CRANIAL, HUDSON
6515-00-515-2114	BUR, CRANIAL, HUDSON, 9 mm
6515-00-515-2115	BUR, CRANIAL, HUDSON, 16 mm
6515-00-515-2116	DRILL, FLAT, CRANIAL, CUSHING, 3/8 inch

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project Number: 6515-5640
Location: c:\word\doc\eric\bracecid

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

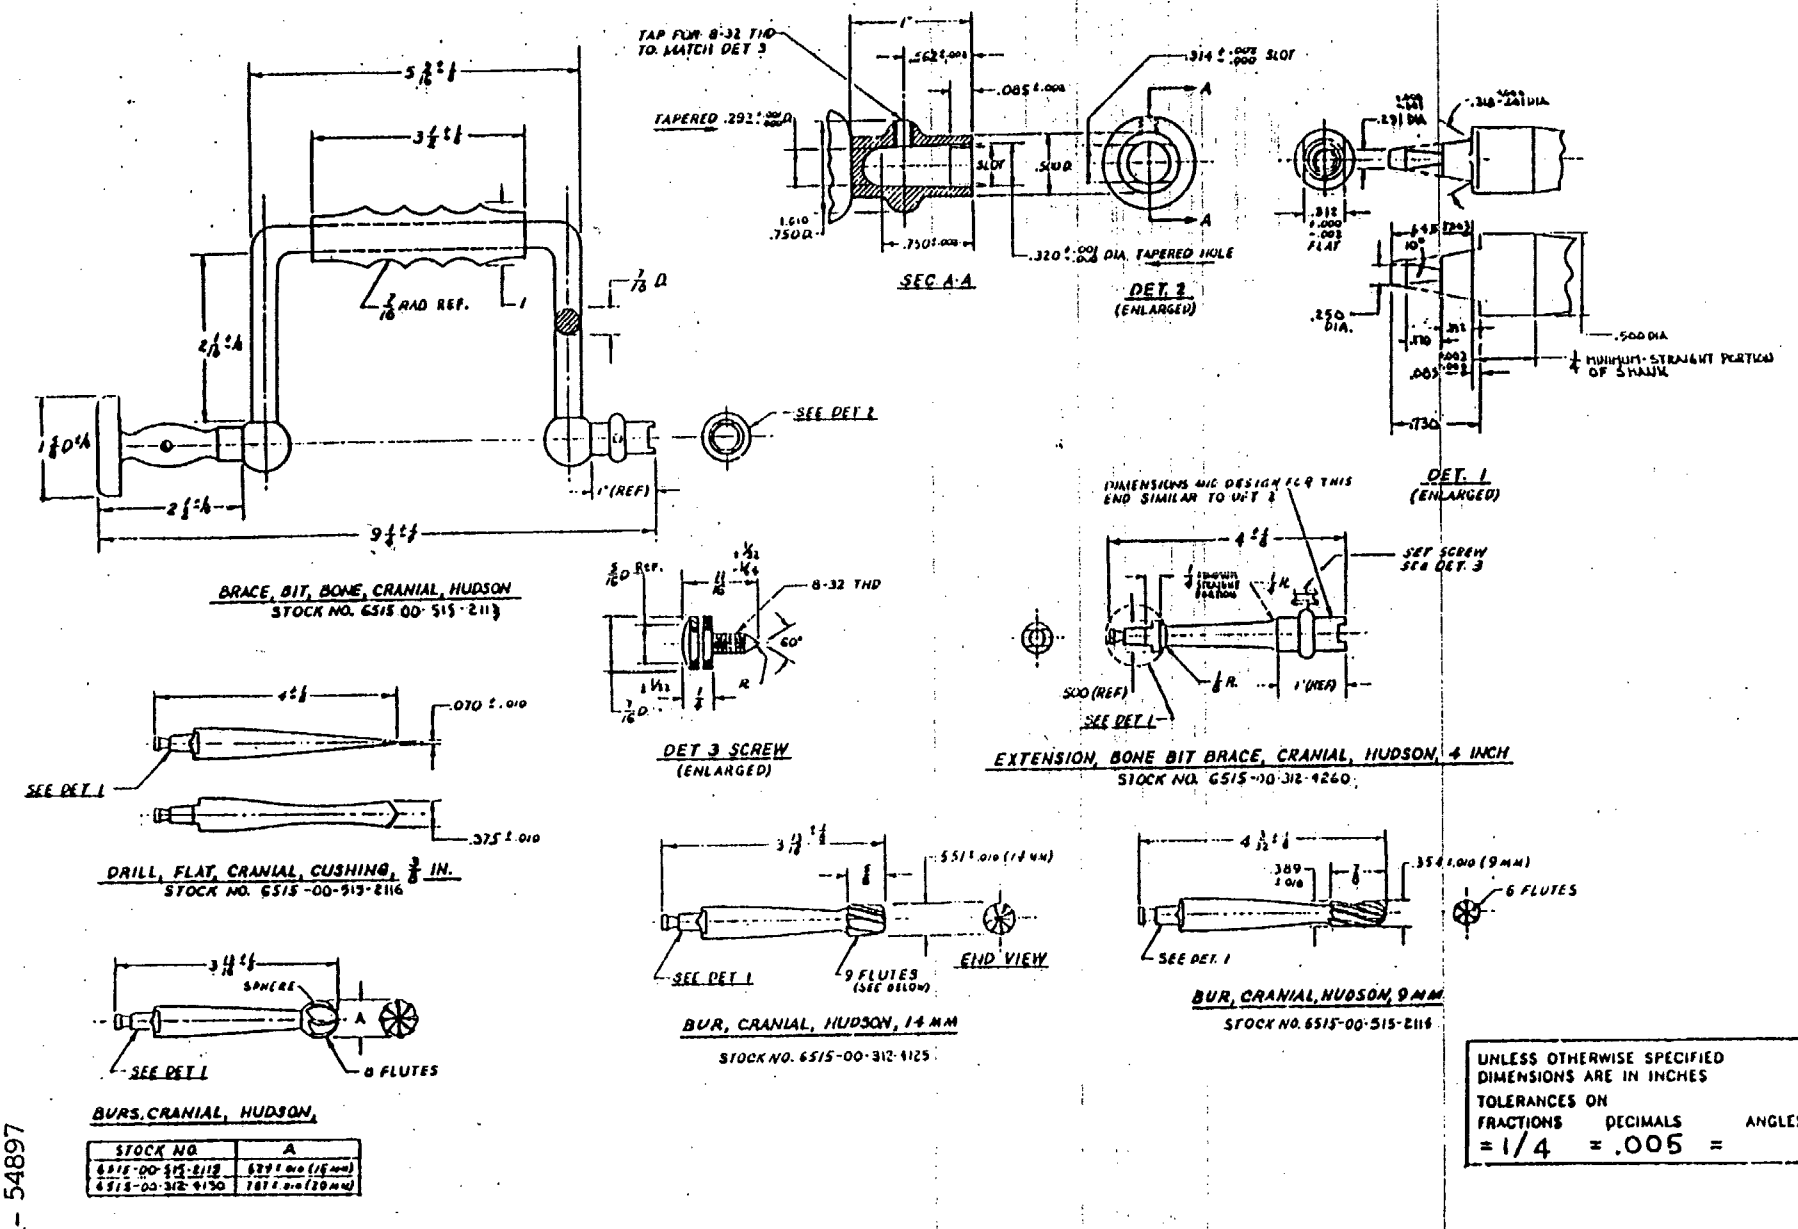

STOCK NO	A
6515-00-515-2118	.639 ± .010 (16 MM)
6515-00-312-4130	.787 ± .010 (20 MM)

A-A-54897

FIGURE 1 BRACE, BIT, BONE & COMPONENT PARTS

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8 In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1. DOCUMENT NUMBER	2. DOCUMENT DATE (YYMMDD)
	A-A-54897	930723

3. DOCUMENT TITLE

BRACE, BIT, BONE, CRANIAL, HUDSON, AND BURS, DRILL AND EXTENSION

4. NATURE OF CHANGE *(Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)*

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code)	
	(1) Commercial	(2) AUTOVON
Defense Personnel Support Center ATTN: DPSC-MSE	(215)7372870	444-2870
c. ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.