INCH-POUND

A-A-54982
30 September 1994

COMMERCIAL ITEM DESCRIPTION

SCISSORS, GENERAL SURGICAL
(Angular, Potts Smith)

The General Services Administration has authorized the use of this Commercial Item Description.

This Commercial Item Description covers the following scissors of the Potts Smith design for use in general and cardiovascular surgical procedures.

Salient characteristics:

Classification. The scissors shall be of the following types:

Type I	-	45 degree angular
Type II	-	60 degree angular
Type III	-	25 degree angular

General. The scissors shall be of the Potts Smith design, having angular cutting blades, as shown in Figure 1. Overall length shall be 7-1/2 inches and the cutting blade shall be 15/16 inch.

Material. The scissors shall be fabricated from class 4, martensitic stainless steel in accordance with ASTM Designation F899.

Style, design and dimensions. The scissors shall be in accordance with Figure 1 for style, design and dimensions. Blade tips shall match precisely in the closed position.

Hardness. After proper stress relieving, the Rockwell Hardness C Scale (HRC) of the scissors shall be 50 to 55. Conversion of hardness values shall be in accordance with ASTM Designation E140.

Finish. The scissors shall have a mirror finish.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:41Z
Check the source to verify that this is the current version before use.

Passivation. The scissors shall be properly passivated.

Corrosion resistance. The scissors shall show no signs of corrosion or plating of copper when tested for corrosion resistance in accordance with ASTM Designation F1089.

Performance. The scissors shall meet the performance requirements in accordance with ASTM Designation F1079.

Identification marking. Scissors shall be permanently marked with the contractor's name or registered trademark and the word "stainless". In addition, scissors of foreign manufacture shall bear the name of the country of manufacture.

Workmanship. The scissors shall meet the performance requirements in accordance with ASTM Designation F1079.

Unit. Each (EA). One scissors, as specified, constitutes one unit. Scissors shall be supplied in a suitable unit container.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:41Z
Check the source to verify that this is the current version before use.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified. Unit of product for examination purposes shall be one scissors as specified. Sampling shall be inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified. Unit of product for test purposes shall be one scissors. Sampling shall be inspection level S-2 with an AQL of 1.0.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:41Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

NOTE: The following National Stock Numbers, their respective Item Identifications and their respective Types are covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION	TYPE
6515-00-690-3222	SCISSORS, GENERAL SURGICAL, 45 degree Angular, Potts Smith, 7-1/2 inches long, 2.3 cm cut	I
6515-00-690-3223	SCISSORS, GENERAL SURGICAL, 60 degree Angular, Potts Smith, 7-1/2 inches long, 2.3 cm cut	II
6515-00-690-3224	SCISSORS, GENERAL SURGICAL, 25 degree Angular, Potts Smith, 7-1/2 inches long, 2.3 cm cut	III

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:41Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project Number: 6515-5728
Location: finals\mab

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:41Z
Check the source to verify that this is the current version before use.


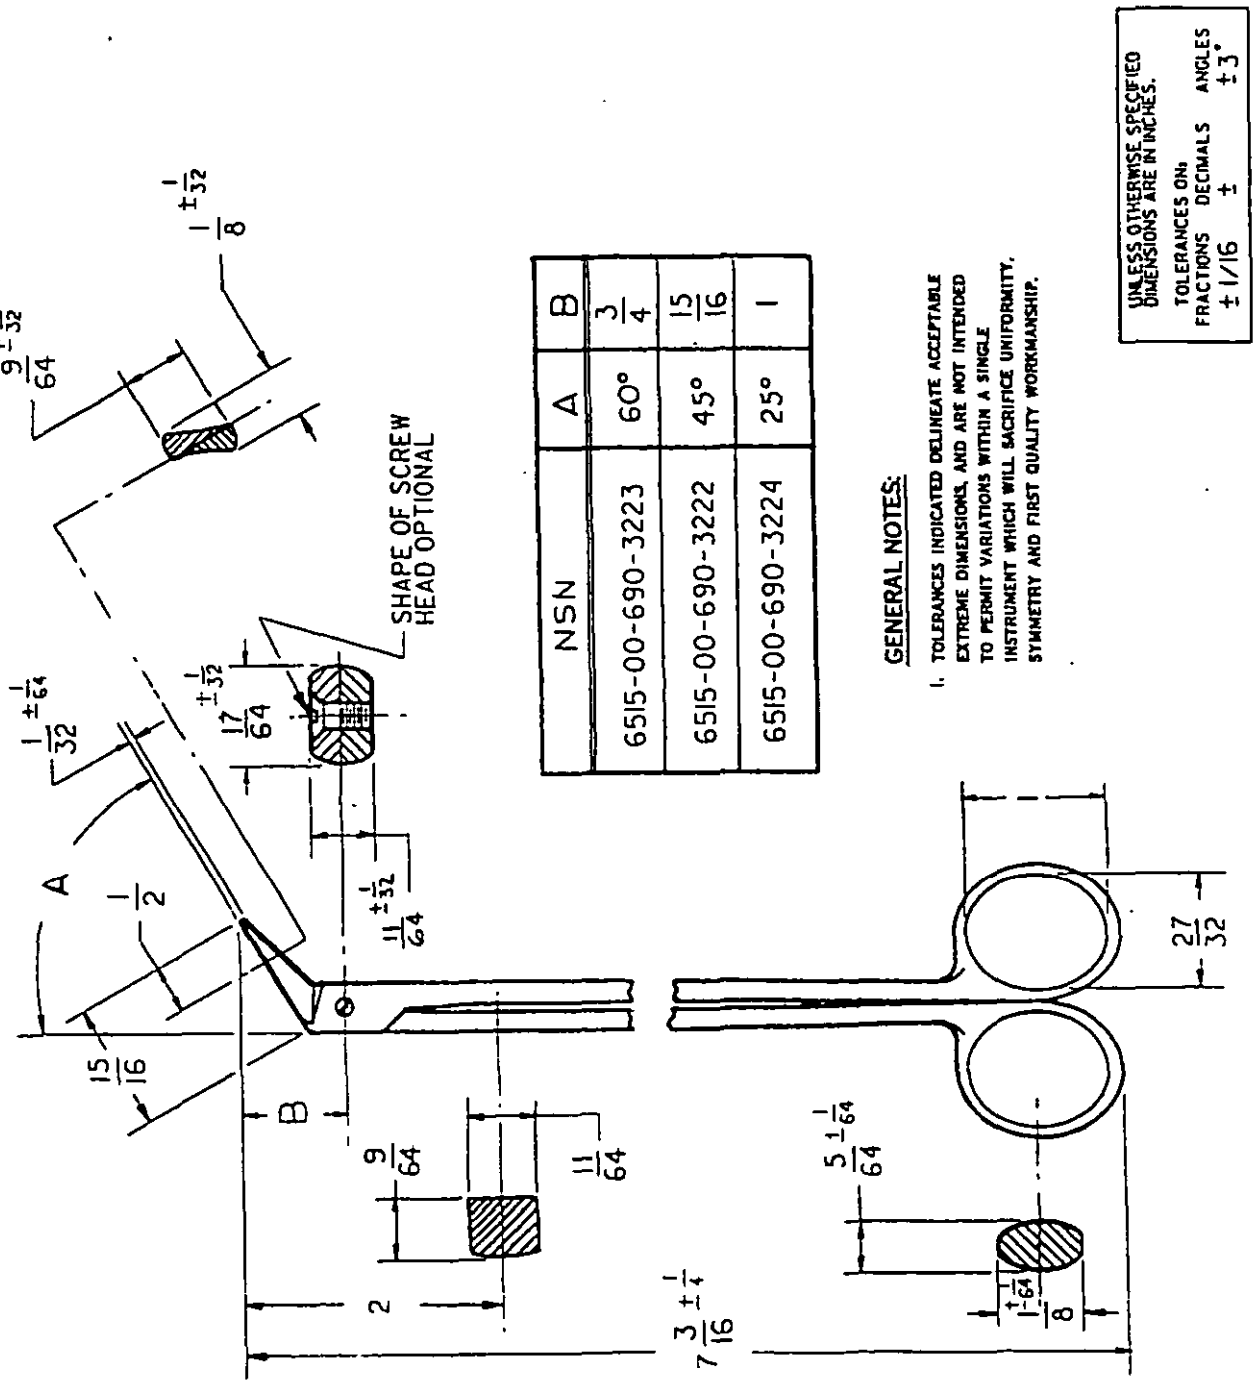


FIGURE 1 SCISSORS, GENERAL SURGICAL, POTTS SMITH

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:41Z
Check the source to verify that this is the current version before use.

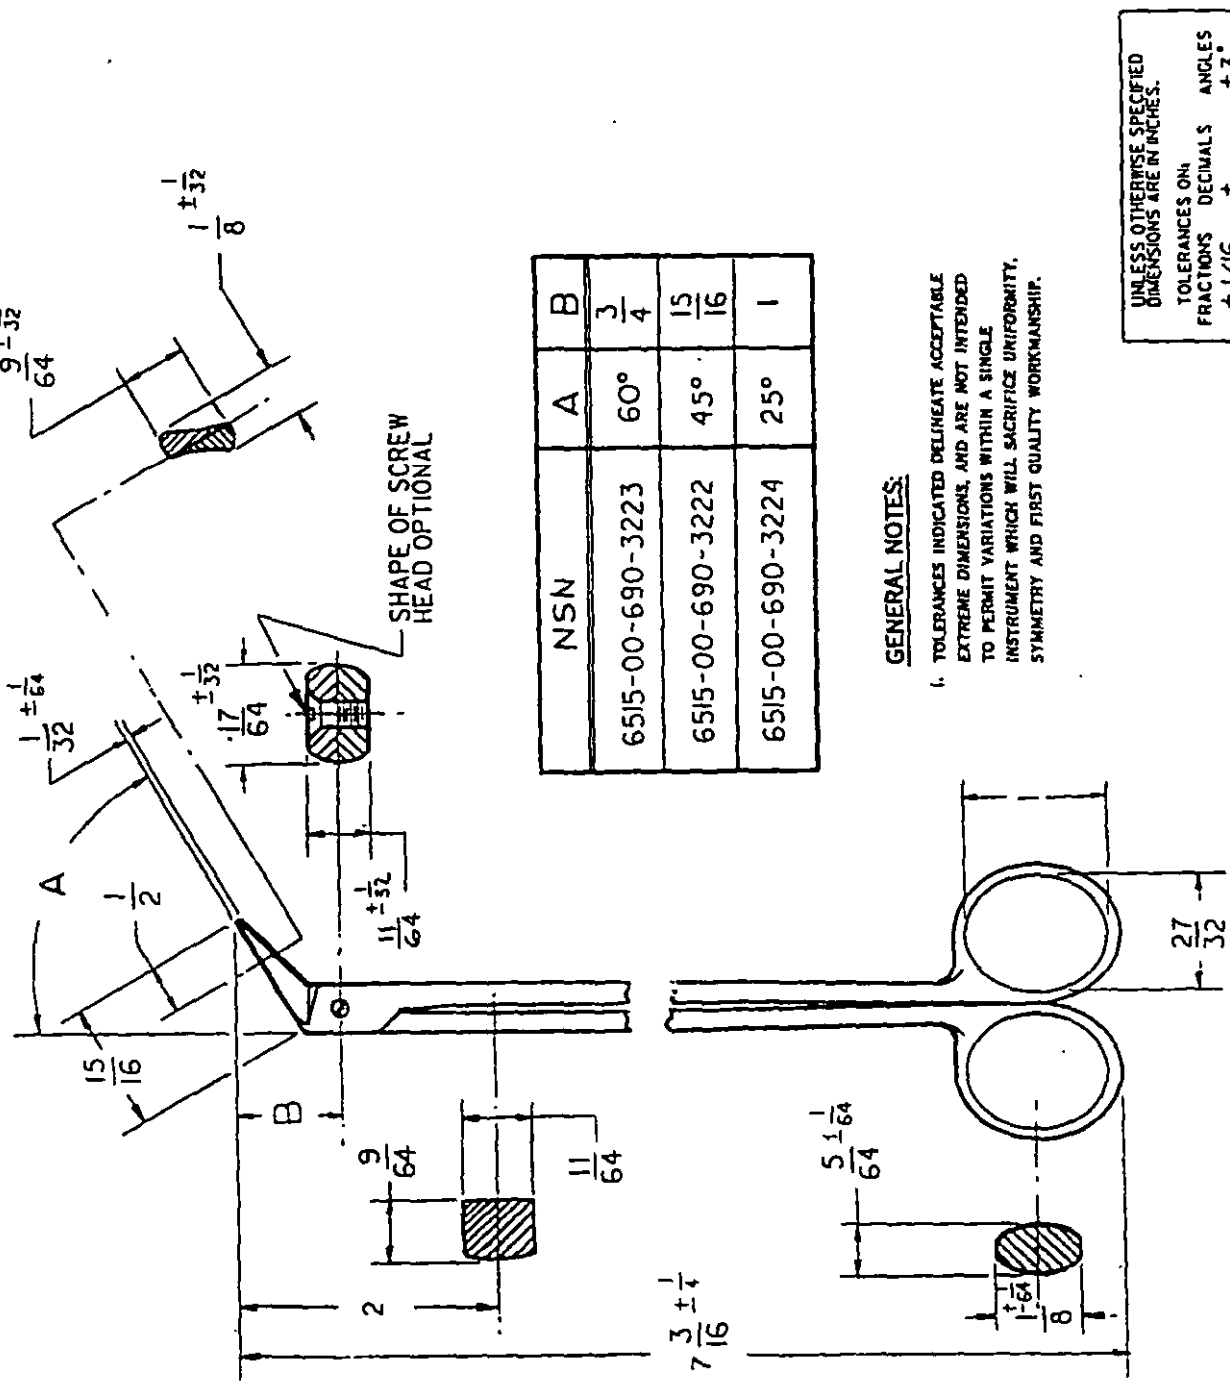

NSN	A	B
6515-00-690-3223	60°	3/4
6515-00-690-3222	45°	15/16
6515-00-690-3224	25°	1

GENERAL NOTES:

1. TOLERANCES INDICATED DELINEATE ACCEPTABLE EXTREME DIMENSIONS, AND ARE NOT INTENDED TO PERMIT VARIATIONS WITHIN A SINGLE INSTRUMENT WHICH WILL SACRIFICE UNIFORMITY, SYMMETRY AND FIRST QUALITY WORKMANSHIP.

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES.

TOLERANCES ON:	FRACTIONS	DECIMALS	ANGLES
	± 1/16	±	± 3°

FIGURE 1 SCISSORS, GENERAL SURGICAL, POTTS SMITH

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:41Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1. DOCUMENT NUMBER A-A-54982	2. DOCUMENT DATE (YYMMDD) 94/09/30

3. DOCUMENT TITLE
SCISSORS, GENERAL SURGICAL (Angular, Potts Smith)

4. NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code) (1) Commercial	(2) AUTOVON
Defense Personnel Support Center ATTN: DPSC- MAP	(215) 737-8431	444-8431
c. ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

DD Form 1426, OCT 89 — Previous editions are obsolete. — 198/290

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:41Z
Check the source to verify that this is the current version before use.