MIL-B-36444A
2 February 1977
SUPERSEDING
MIL-B-36444
6 October 1965

MILITARY SPECIFICATION

BAG, URINE COLLECTION, PEDIATRIC, PLASTIC, DISPOSABLE

This specification is approved for use by all Departments and and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers disposable plastic bags, suitable for collecting urine specimens from newborn infants and small children.

1.2 Classification. The disposable urine collection bags covered by this specification shall be of the following types and sizes as specified (see 6.2):

Type I. - Graduated, single chamber construction, no drain, 130 cubic centimetres (cc) capacity.

Type II. - Non-graduated, double chamber construction with a drain hole.

Size A - 100 cc capacity.
Size B - 200 cc capacity.

Type III. - Non-graduated, double chamber construction with a drain tube.

Size A - 100 cc capacity.
Size B - 200 cc capacity.

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: Headquarters, Defense Personnel Support Center, ATTN: Directorate of Medical Materiel, Code ATT, 2800 South 20th Street, Philadelphia, Pa. 19101, by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:36Z
Check the source to verify that this is the current version before use.

2. APPLICABLE DOCUMENTS

2.1 Issues of documents. The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein.

SPECIFICATIONS

FEDERAL

PPP-B-636 - Boxes, Shipping, Fiberboard.

STANDARDS

MILITARY

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of specifications, standards, drawings, and publications required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposals, shall apply.

AMERICAN SOCIETY FOR TESTING AND MATERIALS (ASTM).

D 882 - Test for Tensile Properties of Thin Plastic Sheeting.

D 1003 - Test for Haze and Luminous Transmittance of Transparent Plastics.

D 1709 - Test for Impact Resistance of Polyethylene Film by the Free Falling Dart Method.

D 1746 - Test for Transparency of Plastic Sheeting.

D 1894 - Test for Coefficients of Friction of Plastic Film and Sheeting.

(Application for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, Pennsylvania 19103.)

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:36Z
Check the source to verify that this is the current version before use.

PRESSURE SENSITIVE TAPE COUNCIL (PSTC).

PSTC-1 - Peel Adhesion for Single Coated Tapes 180° Angle.

(Applications for copies should be addressed to the Pressure Sensitive Tape Council, 1201 Waukegan Road, Glenview, Illinois 60025.)

3. REQUIREMENTS

3.1 First article. When specified in the procurement document, the contractor shall furnish sample unit(s) for first article inspection (see 4.1.2.1 and 6.2).

3.2 Material. The materials specified herein shall be of the highest quality throughout and suitable in all respects for the purposes intended.

3.2.1 Polyethylene film. The polyethylene film shall be non-toxic and non-irritating. The film shall have the following characteristics when tested as specified in table IV:

Tensile strength	6 pounds per inch of width, minimum.
Haze	15 percent, maximum.
Impact resistance	150 grams, minimum.
Transparency	50 percent, minimum.
Coefficient of friction	0.20 maximum.

3.2.2 Surgical adhesive. The surgical adhesive shall be a pressure-sensitive and hypo-allergenic adhesive of the acrylate family. The adhesive shall be non-toxic and non-irritating when tested as specified in 4.4.1. Upon removal of the bag from the patient, the adhesive shall not leave any residue on the surface of the skin, nor shall any abrasion or irritation of the skin result. The adhesive shall have a pull-factor of 20 to 25 ounces per inch of width when tested as specified in PSTC-1.

3.2.3 Release paper. The release paper shall be a protective cover for the adhesive. The paper shall adhere firmly to the adhesive, but shall not remove any of the adhesive when it is peeled away. The paper shall not modify the quality of the surgical adhesive.

3.3 Construction. All seams in the polyethylene film (3.2.1) shall be completely heat sealed. The urine collection bags shall be free of holes and tears and shall not leak. The urine collection bags covered by this specification are comprised of the following components:

a. Outer bag (3.3.1).
b. Inner bag-type II and type III only (3.3.2).
c. Opening (3.3.3).
d. Adhesive area (3.3.4).
e. Drainage tubing-type III only (3.3.5).

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:36Z
Check the source to verify that this is the current version before use.

3.3.1 Outer bag. All outer bags shall be fabricated from polyethylene film (3.2.1) a minimum of 0.002 inch thick. The dimensions given below for the outer bags are for reference only.

3.3.1.1 Type I, outer bag. The type I outer bags shall be indelibly graduated in 10 cc. increments from 10 cc. to 130 cc. to indicate liquid volume. The bags shall have a maximum capacity of at least 150 cc. and shall measure 7 inches by 2-3/4 inches.

3.3.1.2 Type II, outer bag. The type II outer bags shall have a 1/4 inch diameter drain hole near one bottom corner. The drain hole shall have a removable polyethylene film (3.2.1) cover which shall be heat sealed to the outer bag. The polyethylene film for the cover shall be at least 0.002 inch thick.

3.3.1.3 Type III, outer bag. The type III outer bags shall have a drainage tube (3.3.5) connected at one bottom corner.

3.3.1.4 Type II and Type III, (Size A and size B) outer bag.

3.3.1.4.1 Size A. Size A bags shall have a maximum capacity of at least 200 cc. with a practical capacity of 100 cc. The bags shall measure 6-1/2 by 3-3/8 inches.

3.3.1.4.2 Size B. Size B bags shall have a maximum capacity of at least 350 cc. with a practical capacity of 200 cc. The bags shall measure 8-5/8 by 3-1/2 inches.

3.3.2 Inner bag (Type II and Type III only). The inner bags shall be fabricated from polyethylene film (3.2.1) a minimum of 0.002 inch thick. The inner bag shall be at least 2-1/4 inches wide and 3-1/2 inches long with 2 slits in the polyethylene film near the bottom edge. The slits shall act as check valves, allowing the urine to pass from the inner bag to the outer bag and inhibiting the urine from re-entering the inner bag and splashing against the skin. The collection bag shall be tested for leakage into the inner bag in accordance with 4.4.2. Any evidence of leakage shall be cause for rejection.

3.3.3 Opening. Each outer bag (3.3.1) and each inner bag (3.3.2) shall have an opening. The opening shall be either round, oval, or tear-drop shaped (see figure 1) with dimensions as shown in table I. For all type II and type III collection bags, the inner bag and the outer bag shall have identical openings. The edges of the outer bag and the inner bag openings shall be completely heat sealed together.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:36Z
Check the source to verify that this is the currentversion before use.

TABLE I - Dimensions (inches) for openings (figure 1).

TYPE	SIZE	HOLE SHAPE				
		Round	Teardrop		Oval	
		Dia	L	W	L	W
I		1-1/4	1-9/16	1-1/4	1-1/4	1
II	A	1-1/4	1-9/16	1-1/4	1-1/4	1
	B	1-1/2	1-3/4	1-1/4	1-3/4	1-1/8
III	A	1-1/4	1-9/16	1-1/4	1-1/4	1
	B	1-1/2	1-3/4	1-1/4	1-3/4	1-1/8


3.3.4 Adhesive area. The adhesive area surrounding the opening (3.3.3) shall hold the urine collection bag in position on a male or female newborn infant or small child and shall prevent fecal contamination of the urine specimen. After a specimen has been taken, it shall be possible to fold the adhesive (3.2.2) area on itself to make a leakproof seal for transportation. The leakproof seal shall be tested for watertightness in accordance with 4.4.5. When the adhesive is not applied to the outer bag (3.3.1), it shall be applied to a gasket of polyethylene film (3.2.1) having a minimum thickness of 0.003 inch. The gasket shall have an opening which is identical to that of the outer bag (and the inner bag on all type II and type III collection bags). The edges of the opening in the gasket and the outer bag (and the inner bag on all type II and type III collection bags) shall be completely heat sealed together. The adhesive area shall be covered by release paper (3.2.3) and designed in accordance with figure 2.

3.3.4.1 Type I and Size A (Type II and Type III) collection bags. The top edge of the adhesive area shall be a maximum of 1/2 inch from the top edge of the outer bag.


3.3.4.2 Size B (Type II and Type III) collection bags. The top edge of the adhesive area shall be a maximum of 3/4 inch from the top edge of the outer bag.

3.3.5 Drainage tubing (Type III only). The drainage tubing shall consist of the tubing, the junction, and the cap. The tubing shall be clear, flexible vinyl tubing with a 3/16 inch (nominal) outside diameter and a 1/8 inch (nominal) inside diameter. One end of the tubing shall be heat sealed to a bottom corner of the outer bag (3.3.1). The junction shall be capable of joining two pieces of tubing and shall be stored on the free end of the tubing when not in use. The cap shall be capable of stopping both the free end of the tubing and the end of the junction. The drainage tubing shall be 60 $\pm$ 1 inches in length.


Source: https://assist.dla.mil -- Downloaded: 202610-21T08:36Z
Check the source to verify that this is the current version before use.



ROUND

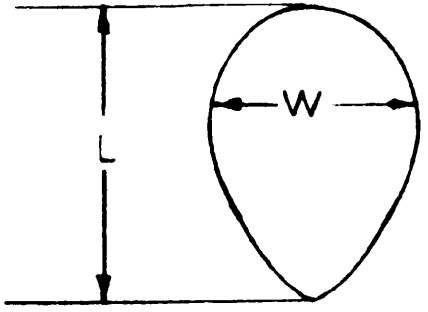

TEARDROP

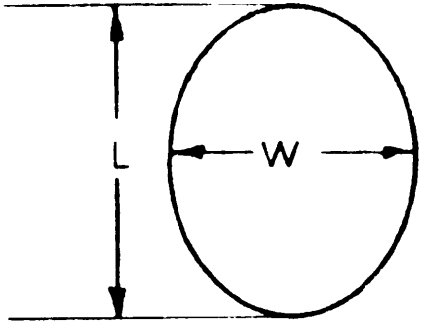


OVAL

NOTES


1. SEE TABLE I OF SPECIFICATION BODY FOR OPENING DIMENSIONS.
2. UNLESS OTHERWISE STATED, ALL TOLERANCES ARE $\pm \frac{1}{8}$ INCH.
3. "W" FOR TEARDROP SHAPED OPENING IS MEASURED AT THE WIDEST POINT.

FIGURE I. Opening Designs

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:36Z
Check the source to verify that this is the current version before use.

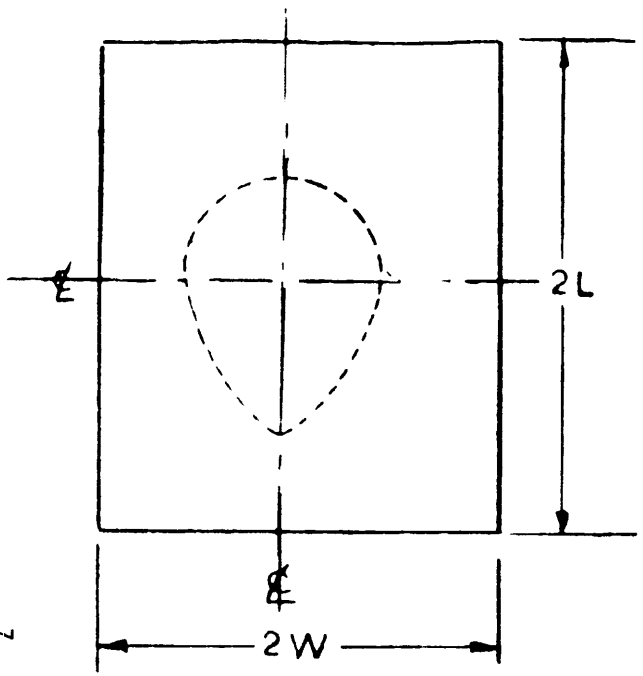

RECTANGULAR

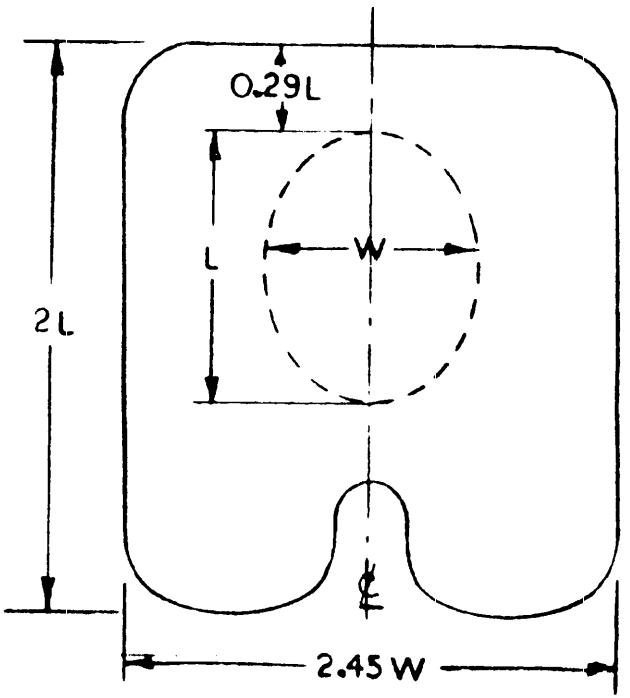

MODIFIED RECTANGULAR

NOTES

1. THE OPENINGS SHOWN ON THE ADHESIVE AREAS ARE FOR ILLUSTRATION, ANY OPENING DESIGN MAY BE USED WITH EITHER ADHESIVE AREA DESIGN.
2. SEE TABLE I OF SPECIFICATION BODY FOR OPENING DIMENSIONS.
3. UNLESS OTHERWISE STATED ALL TOLERANCES ARE $\pm \frac{1}{8}$ INCH.
4. ALL DIMENSIONS IN INCHES.

FIGURE 2. Adhesive Area Designs.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:36Z
Check the source to verify that this is the current version before use.

3.4 Directions for use. Each urine collection bag shall be supplied with a comprehensive instruction sheet for use. As an alternate the instructions for use shall be permanently and legibly marked on each bag.

3.5 Identification marking. Each urine collection bag shall be legibly and permanently marked with the manufacturer's name or registered trademark.

3.6 Workmanship. Workmanship shall be first class throughout. The bags shall be free from defects which detract from their appearance or may impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time. during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual, and auditory, investigation without the use of special laboratory appliances or procedures) and testing (determination) by technical means of physical and chemical properties) of the item.

4.1.2.1 Classification of inspection. The inspection requirements specified herein are classified as follows:

a. First article inspection.
b. Quality conformance inspection.

4.1.2.1.1 First article inspection. First article inspection shall be performed on the urine collection bags when a first article sample is required (see 3.1). This inspection shall include examination of 4.3 and tests of 4.4.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:36Z
Check the source to verify that this is the current version before use.

4.1.2.1.1 First article inspection. First article inspection shall be performed on the urine collection bags when a first article sample is required (see 3.1). This inspection shall include examination of 4.3 and tests of 4.4.

4.1.2.1.2 Quality conformance inspection. Quality conformance inspection shall include the examination of 4.3 and tests of 4.4.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the urine collection bags may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificates shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and table II.

TABLE II. Sampling for examination.

	Inspection level	AQL (defects per hundred units)
For visual examination		
Major defects	S-4	1.0
Total defects (Major and Minor combined)	S-4	4.0
For dimensional examination	S-1	2.5

4.2.2 For tests.

4.2.2.1 Urine collection bag. Sampling for tests of the urine collection bag shall be conducted in accordance with MIL-STD-105 and table III. The acceptance level shall be zero for all sample sizes.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:36Z
Check the source to verify that this is the current version before use.

TABLE III. Sampling of urine collection bag.

Characteristic	Requirement	Test method	Inspection level
Toxicity and irritation by adhesive	3.2.2	4.4.1	S-1
Pull factor of adhesive	3.2.2	PSTC-1	S-1
Leakage and Volumetric capacity	3.3	4.4.2	S-1
Indelibility	3.3.1.1	4.4.3	S-1
Leakage into inner bag	3.3.2	4.4.4	S-1
Watertightness of adhesive seal	3.3.4	4.4.5	S-1

4.2.2.2 Polyethylene film. Samples of the material used in the fabrication of the urine collection bag shall be selected for testing in accordance with table IV. Two samples, randomly selected, shall be tested from each lot of film used in the manufacture of the urine collection bag. The dimensions of each test sample shall be as specified in the test method. Acceptance level shall be zero for all sample sizes.

4.3 Examination. The bags shall be examined to determine compliance with all requirements contained in this specification.

TABLE IV. Sampling of polyethylene film.

Characteristic	Requirement	Test method
Tensile strength	3.2.1	ASTM-D882
Haze	3.2.1	ASTM-D1003
Impact resistance	3.2.1	ASTM-D1709
Transparency	3.2.1	ASTM-D-1746
Coefficient of friction	3.2.1	ASTM-D1894

4.3.1 Classification of defects. Examination shall be conducted in accordance with the classification of defects listed in table V. Examination shall not be restricted to the classified possible defects listed below.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:36Z
Check the source to verify that this is the currentversion before use.

TABLE V. Classification of defects.

Categories	Defects
Major:	
101	Bag not free of holes or tears.
102	Heat seals not complete.
103	Adhesive area not complete.
104	Adhesive peels away upon removal of paper cover.
105	Unit not complete with all components.
Minor:	
201	Marking missing or incomplete or otherwise not in accordance with specification.

4.3.2 Dimensional examination. The urine bags shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted, to determine compliance with specification requirements.

4.4.1 Toxicity and irritation. A certificate for each lot of urine collection bags shall be forwarded to the procuring activity by the contractor to the effect that the urine collection bags are nontoxic and nonirritating as specified in 3.2.1 and 3.2.2. The adhesive-covered areas shall be applied to ten human subjects for a period of six hours under the supervision of a doctor of medicine or osteopathy who shall certify the tests. In addition, a copy of each certificate shall be furnished to the cognizant Government inspector. The certificates shall conform to 4.1.3.

4.4.2 Leakage and volumetric capacity. The urine collection bags shall be filled with measured amounts of tap water as indicated in table V. The graduation marks on the bag shall be checked. The bags shall then be suspended on a suitable support for 24 hours. At the end of this period each bag shall be examined for evidence of leakage.

TABLE VI. Volumetric capacity.

Type	Size	Volume (+ 5 cc)
I		150
II	A	200
	B	350
III	A	200
	B	350

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:36Z
Check the source to verify that this is the current version before use.

4.4.3 Indelibility. Markings shall not fade or disappear when rubbed 10 complete cycles (forward and back) with a water moistened cotton cloth. The rubbing pressure shall be 5 pounds.

4.4.4 Leakage to inner bag. The type II and type III urine collection bags shall be filled with 60 ± 5 milliliters (ml) of tap water. Hold the bag in the vertical position to permit all of the water to flow into the outer bag. Lay the filled bag on a horizontal surface and observe for a period of five minutes changing position every minute so that both valves are checked. During the five minute period check visually and record any evidence of leakage.

4.4.5 Watertightness of adhesive seal. The urine collection bag shall be filled with 60 ± 5 ml of tap water. Remove backing from the adhesive area and press adhesive to a piece of glass which has previously been cleaned with alcohol. Remove bag from glass and fold adhesive area over on itself to form a watertight seal. Suspend bag in the inverted position (seal downward), observe for a period of 5 minutes and record any evidence of leakage.

4.5 Packaging inspection. The inspection of the unit, intermediate package, packing and marking for shipment and storage shall be in accordance with quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

5. PACKAGING

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Unit of issue. One box containing fifty type I bags or one package containing fifty type III size A or type III size B bags or one package containing one hundred type II size A or type II, size B bags, as specified, constitutes one unit of issue.

5.1.2 Level A.

5.1.2.1 Unit package.

5.1.2.1.1 Type I and type II, sizes A and B. Fifty type I or one hundred type II size A or size B bags shall be packaged in a snug fitting paperboard, dispenser type box of an appropriate design. Closure shall be adequate to prevent accidental opening.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:36Z
Check the source to verify that this is the current version before use.

5.1.2.1.2 Type III, size A and size B. Each bag with tubing neatly coiled shall be sealed in a clear plastic envelope of an appropriate size and design. Fifty individually packaged bags of one size only shall be further packaged in a snug fitting paperboard, dispenser type box of an appropriate design. Closure shall be adequate to prevent accidental opening.

5.1.3 Level C. Fifty type I, one hundred type II size A or B or fifty individually packaged type III, size A or B shall be packaged in a dispenser type box that will afford adequate protection against deterioration and physical damage during shipment from the supply source to the first receiving activity.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.2).

5.2.1 Level A. Ten unit packages containing type I or type II, size B or eighteen unit packages containing type III, size A or size B or seventy unit packages containing type II size A shall be packaged in an exterior container conforming to PPP-B-636, class weather-resistant. Closure, strapping and waterproofing shall be as specified in the appendix of the box specification.

5.2.2 Level B. Units shall be packed as specified in 5.2.1 except that the exterior container shall conform to PPP-B-636, class domestic. Strapping and waterproofing shall not be required.

5.2.3 Level C. The packaged bags shall be packed in shipping containers in a manner that will afford adequate protection against damage during direct shipment from the supply source to the first receiving activity. These packs shall conform to the applicable carrier rules and regulations.

5.3 Marking.

5.3.1 Unit packages. Each unit package shall be marked in accordance with MIL-STD-129. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The disposable, plastic urine collection bags covered by this specification are intended for collection of urine specimens from pediatric patients as specified below.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:36Z
Check the source to verify that this is the current version before use.

Type I - Collection of urine specimens from newborn infants or small children.

Type II

Size A - Collection of urine specimens from newborn infants.
Size B - Collection of urine specimens from newborn infants or small children.

Type III

Size A - Collection of 24 hour urine specimens from newborn infants.
Size B - Collection of 24 hour urine specimens from newborn infants or small children.

6.2 Ordering data. Procurement documents should specify the following:

a. Title, number and date of this specification.
b. Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
c. When a first article is required (see 3.1, 4.1.2.1 and 6.3).
d. Type, size and National Stock Number (NSN) of desired item (see 1.2 and 6.4).

6.3 First article. When a first article is required, it shall be tested under the appropriate provisions of the Armed Services Procurement Regulation. The contract or purchase order specifies the quantity, procedure for delivery and other specific instructions for inspection of the first article.

6.4 This specification covers the following items appearing in the Federal Supply Catalog.

NSN	Item Identification	Type & Size
6530-00-080-0982	Bag, Urine Collection, Pediatric, Plastic, Disposable, 130cc, 50's	Type 1
6530-00-181-8099	Bag, Urine Collection, Pediatric, Plastic, Disposable, 100cc, 50's	Type III Size A
6530-00-495-7143	Bag, Urine Collection, Pediatric, Plastic, Disposable, 100cc, 100's	Type II Size A

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:36Z
Check the source to verify that this is the current version before use.

NSN	Item Identification	Type & Size
6530-00-495-7144	Bag, Urine Collection, Pediatric, Plastic, Disposalbe, 200cc, 50's	Type III Size B
6530-00-935-4120	Bag, Urine Collection, Pediatric, Plastic, Disposable, 200cc, 100's	Type II Size B

6.5 Changes from previous issue. Asterisks are not used in this revision to identify changes with respect to the previous issue, due to the extensiveness of the changes.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
DLA-DM

Project Number 6530-1176

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:36Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:36Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE
MIL-B-36444A Bag, Urine Collection, Pediatric, Plastic, Disposable

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A
☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?
   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:36Z
·Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:36Z
Check the source to verify that this is the current version before use.