MIL-R-36433B
18 April 1972
SUPERSEDING
MIL-R-36433A
29 October 1968

MILITARY SPECIFICATION

* RESIN, ACRYLIC, DENTAL, IMPRESSION TRAY MATERIAL

This specification is mandatory for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers a self-curing acrylic resin (see 6.1).

2. APPLICABLE DOCUMENTS

2.1 Specifications and standards. The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of the specification to the extent specified herein:

SPECIFICATIONS

Federal

RR-S-366	Sieve, Standard For Testing Purposes.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Setup.
PPP-C-186	Containers, Packaging and Packing For Drugs, Chemicals, and Pharmaceuticals.

FSC 6520

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:35Z
Check the source to verify that this is the current version before use.

Military

MIL-L-10547 Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

STANDARDS

Military

MIL-STD-105 Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material. The acrylic resin shall consist of a liquid and a powder which when mixed in the proper proportion and manner (according to manufacturer's directions) shall produce a self-cured resin for forming dental trays and base-plates.

3.1.1 Liquid. The liquid shall be essentially an acrylic monomer. The liquid shall be clear, colorless, and substantially free from undissolved or particulate matter when examined without accessory magnification. This examination shall be made against a black background and against a white background each illuminated by a light providing an intensity of illumination which is no less than 100 foot-candles nor more than 350 foot-candles at a point 10 inches from its source.

3.1.2 Powder. The powder shall be essentially an acrylic polymer free from extraneous material such as dirt and lint. The powder may contain a maximum of 50 percent of a suitable inert filler provided the resin complies with the physical properties specified herein.

3.1.3 Toxicity. The manufacturer shall submit a statement that the mixing, the forming and use of the resulting dental tray shall have no toxic effect on a normal healthy person.

3.2 Color. The cured resin shall have an opaque blue color produced by incorporation of inorganic pigment only in the powder in manufacture, or produced by the user adding a Food and Drug Administration certified blue dye which shall be supplied in a capsule with the resin. Color shall be uniformly distributed.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:35Z
Check the source to verify that this is the current version before use.

3.3 Unit size. The amount of powder and liquid supplied as a unit, when mixed as directed, shall be sufficient to make a minimum of 22 mixes of at least 20 cubic centimeters each of cured resin, when tested as specified in 4.4.5.

3.4 Manufacturer's instructions. Instructions for storing and processing the resin shall accompany each package. Adequate and accurate instructions for using the resin in forming dental impression trays and baseplates, and in stabilizing baseplates shall also accompany each package. Two copies of instructions shall be forwarded to the contracting officer for information purposes. The instructions shall include the following minimum details:

a. Proper powder liquid ratio.
b. Method mixing, including time and temperature required.
c. Effect of temperature on mixing, working time, and procedures.
d. Method of forming impression trays, baseplates, and stabilizing baseplates.
e. Length of working time and setting time.
f. Method of trimming the cured resin to shape.

3.5 Particle size. The particle size shall be such that a minimum of 97.5 percent of the powder shall pass through a No. 80 U.S. Standard Sieve when tested as specified in 4.4.1.

3.6 Working qualities of uncured resin. The uncured resin shall be plastic and workable for forming either an impression tray or a baseplate for a minimum of 5 minutes from start of mix, when tested as specified in 4.4.2.2.

3.7 Working qualities of cured resin. When processed according to the instructions furnished by the manufacturer (3.4), the cured resin shall yield a satisfactory dental impression tray or baseplate, when tested as specified in 4.4.2.2. The cured resin shall lie inert or "dead" when applied to a cast without a spring back.

3.8 Hardening time of uncured resin. The uncured resin shall harden and set within 12 minutes from start of mix, when tested as specified in 4.4.2.3.

3.9 Transverse deflection. The deflection of at least three of the five specimens prepared as outlined in 4.4.3, shall meet the requirements specified in table I when tested in water of 37 ± 2 degrees Centigrade (°C.) (98.6 ± 3.6 degrees Fahrenheit [°F.]).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:35Z
Check the source to verify that this is the current version before use.

Table I. Deflection Limits of Specimens in Transverse Deflection Test

	DEFLECTION For loads (1) 1,500 grams (gm.) (3.31 pounds [lb.]) to		
Load	2,500 gm. (5.51 lb.)	3,500 gm. (7.72 lb.)	
	Maximum millimeters (mm.)	Minimum mm.	Maximum mm.
Deflection	1.5 (0.059 inch [in.])	1.0 (0.039 in.)	3.5 (0.138 in.)

(1) Deflections shall be measured from an initial load of 1500 gm. (3.31 lb.) to the load indicated.

3.10 Stability. The resin shall comply with the specification for at least two years from date of shipment when stored at 59° F. to 86° F.. No reference to shelf life or expiration date shall be included in the instructions or other accompanying data.

3.11 Delivery schedule. Not more than two months shall have elapsed from the date of manufacture of the resin to the date of delivery to the Government.

3.12 Lot or control number. Each unit of issue shall be marked with the lot or control number. Each lot or control number shall consist of a maximum of 4000 unit packages of the acrylic resin.

3.13 Accessories. A suitable powder scoop and liquid measure shall be included in each unit of issue. In addition, if the resin is formulated for pouring consistency, a tray former shall be supplied.

3.14 Workmanship. Workmanship shall be first class throughout. The acrylic resin and its containers shall be free from defects which either detract from their appearance or may impair their serviceability.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:35Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

* 4.1.2 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

* 4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the component material, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the FSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Quality conformance inspection. The examinations and tests required to assure compliance with specification requirements are classified as specified in tables II and IV (see 4.2.1 and 4.3), table III (see 4.2.2), and 4.2.3.

4.2.1 Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels (AQL's) shall be as indicated in table II. Unit of product for examination purposes shall be one unit of issue of acrylic resin (see 5.1.1).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:35Z
Check the source to verify that this is the current version before use.

Table II. Sampling for Examination

Type defect	Inspection level	AQL (percent defective)
Major	II	1.5
Minor	II	4.0

4.2.2 Sampling for tests (except leakage test). Sampling for tests (except leakage test) shall be conducted as specified in table III. Acceptance number shall be zero.

Table III. Tests

Characteristic	Requirement	Test procedure	Number of determinations per lot or batch number	Unit of product
Particle size	3.5	4.4.1	1	1 container of powder
Working qualities:				
of uncured resin	3.6	4.4.2.2	1	1 unit package
of cured resin	3.7	4.4.2.2	1	1 unit package
hardening time	3.8	4.4.2.3	1	1 unit package
Transverse deflection	3.9	4.4.3	1 (1)	1 container of liquid
Unit size	3.3	4.4.5	2 (2)	1 unit package

(1) Each determination shall be the average of 5 specimens.

(2) Two units of product to be tested per lot or batch number; a lot shall be rejected if any determination fails the test requirement.

4.2.3 Sampling for leakage test. Sampling for leakage test shall be in accordance with MIL-STD-105, inspection level S-4. Acceptance number shall be zero. Unit of product for leakage test shall be one bottle of liquid.

4.3 Examination. Acrylic resin shall be examined for defects including, but not limited to those listed in table IV.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:35Z
Check the source to verify that this is the current version before use.

Table IV. Classification of Defects

Categories	Defects
Major	
101	Color not as specified.
102	Unit package not complete with powder and liquid.
103	Dirt or lint present in powder.
104	Liquid not free from undissolved or particulate matter.
Minor	
201	Manufacturer's instructions not present in unit package; not complete (see 3.4).
202	Closure for bottles of powder not as specified.
203	Closure for bottles of liquid not as specified.
204	Powder scoop and liquid measure not present in unit package.
205	Packaging, packing, and marking not as specified.

4.4 Tests.

4.4.1 Particle size. Particle size of the powder shall be determined by taking ten to twelve grams of the resin powder and placing it on a number 80 sieve conforming to RR-S-366. The top and bottom shall be replaced, and the assembly shall be vibrated mechanically in a Ro-tap for 2 minutes. On completion of the test, the sieve shall be carefully examined for residue remaining on the upper surface of the wire or occluding the sieve openings.

4.4.2 Mixing and packing characteristics.

4.4.2.1 Mixing. Resin shall be mixed as directed by instructions accompanying the package, except the mixing temperature shall be 23.0° C. ± 2.0° C. (73.4° F. ± 3.6° F.).

4.4.2.2 Working qualities test. A mix, prepared in accordance with 4.4.2.1, shall be used to make a dental impression tray on an endentulous plaster or stone model in accordance with normal dental prosthetic technic. The resin shall be tested for the working qualities specified in 3.6 and 3.7.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:35Z
Check the source to verify that this is the current version before use.

4.4.2.3 Hardening time. A mix, prepared in accordance with 4.4.2.1, shall be placed immediately in a stainless steel ring, 60 ± 3 mm. inside diameter, 67 ± 3 mm. outside diameter and 2 ± 0.1 mm. high. The ring shall rest on a flat, dry glass plate, approximately 10 X 8 X 0.60 centimeters (cm.) covered with a thin polyethylene sheet. Any excess mix shall be removed. The hot junction of a thermocouple made from 30 gauge wire shall be placed within 2 mm. of the center of the specimen with the leads of the thermocouple passing through two grooves cut in one side of the ring. The glass plate shall be marked so that the hot junction of the thermocouple can be centered. A sheet of polyethylene and a second glass plate as the bottom plate shall be placed on top of the ring containing the mix. Potentiometer readings shall be made at 30 second intervals between two minutes from start of mix and terminating a minute after the maximum temperature has been reached. The time at which peak temperature is reached, measured from start of mix, shall be considered the hardening time.

4.4.3 Transverse deflection test. A mix of sufficient size to yield five specimens and prepared in accordance with 4.4.2.1 shall be made. A plate of resin shall be processed in a gypsum mold lined with tinfoil (figure 1). Specimens for the transverse test shall be machined from this plate to the dimensions shown in figure 2. The plate (figure 1) shall be sawed lengthwise into five equal strips with a band saw operated at a speed of approximately 100 meters per minute (328 feet per minute). The plate shall be at least 2 days old prior to sawing. The strips may then be sanded slightly on the molded surfaces, if necessary, to remove imperfections. All subsequent milling operations shall be with a 50 mm. (2 in.) diameter flycutter, operating at a spindle speed of approximately 1,800 revolutions per minute and at a table feed of about 15 cm. per minute (6 in. per minute). Rough cuts shall be approximately 0.08 mm. (0.003 in.) deep, and finish cuts shall be 0.03 mm. (0.001 in.) deep. The strips shall be mounted side by side in a vise and the edges machined parallel in order to remove all band saw marks. The strips at this point shall be oversize in width. One or more strips shall be mounted in a vise and the faces milled to the required thickness (2.50 ± 0.03 mm. [0.0984 ± 0.0012 in.]). All five strips shall then be clamped face to face in a vise and the edges milled to the required width (10.00 ± 0.02 mm. [0.393 ± 0.0012 in.]). The specimens shall be stored in distilled water at 37° ± 1° C. (98.6° ± 1.8° F.) for 2 days immediately before testing. The specimen shall be mounted in an appropriate instrument, such as is shown in figure 2. An initial load, consisting of the free-moving parts of the apparatus (figure 2) plus sufficient lead shot to make a load of 1500 gm. (3.3 pounds), shall be placed on the specimen. Each 500-gm. increment of shot shall be added at a uniform rate during the last 30 seconds of each minute. The schedule indicated in table V shall be used in applying the loads and in making the observations.

Source: https://assist.dla.mil -- Downloaded: 202640-21T08:35Z
Check the source to verify that this is the currentversion before use.

TRANSVERSE TESTING MACHINE



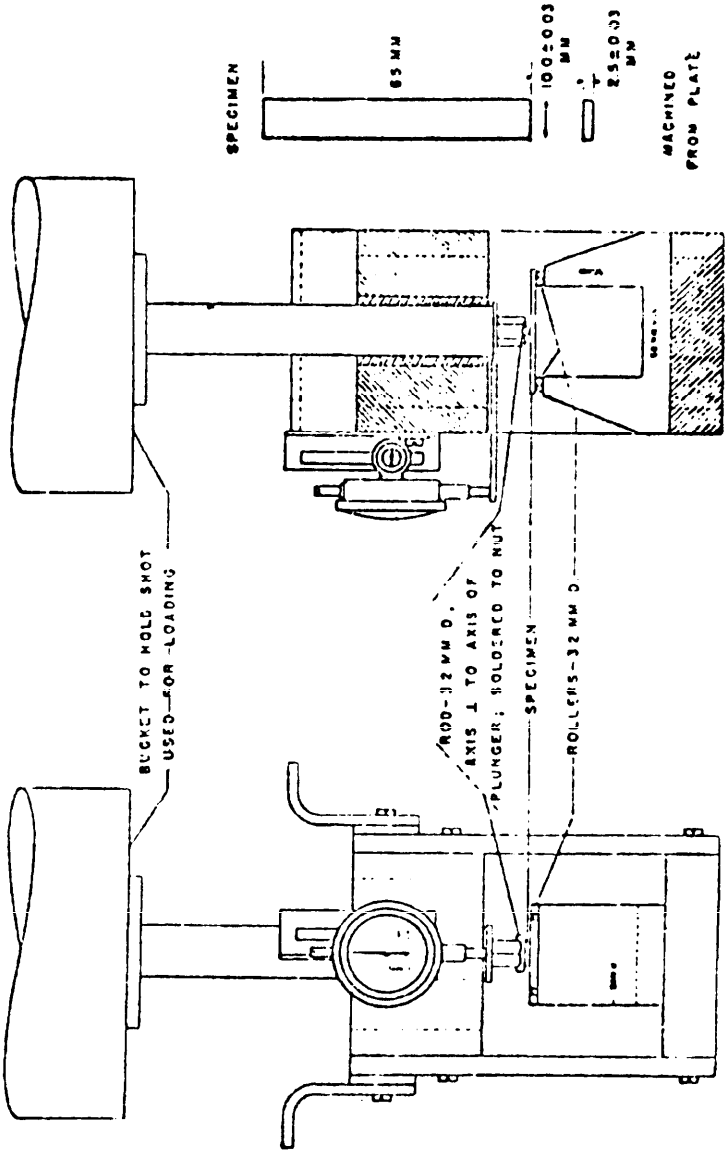


Figure 1

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:35Z
Check the source to verify that this is the current version before use.

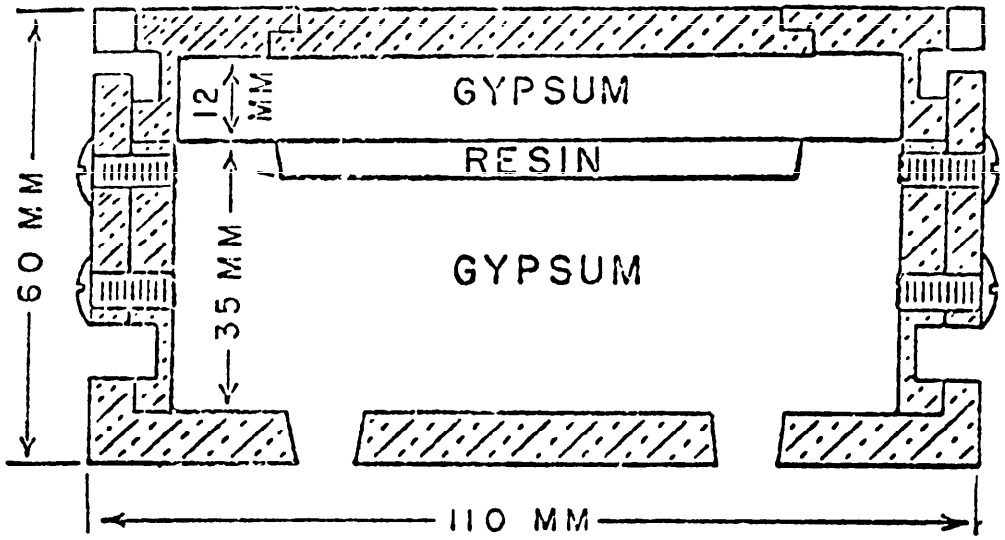

DENTURE FLASK

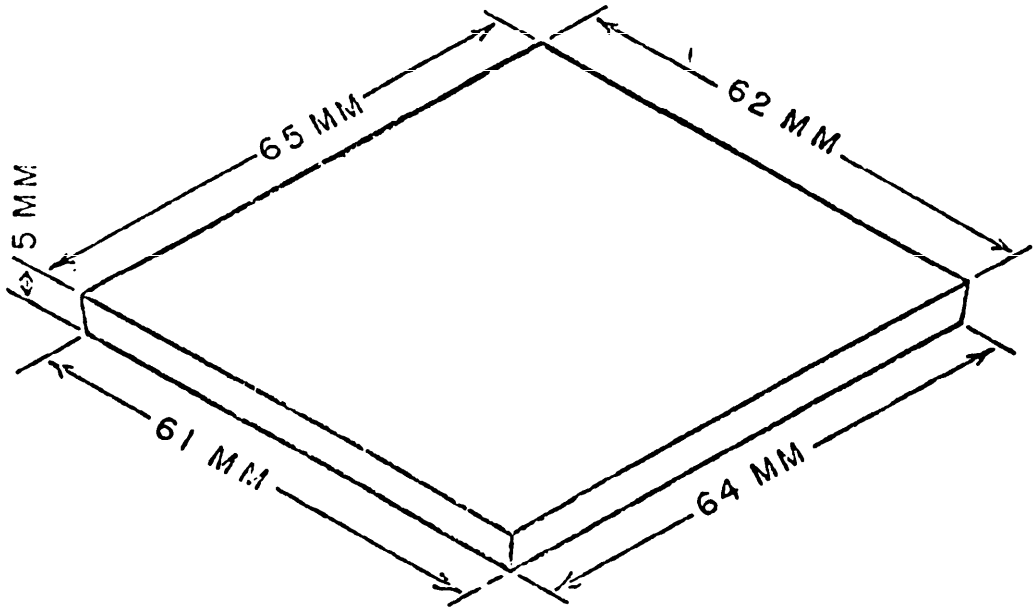

SPECIMEN PLATE

Figure 2

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:35Z
Check the source to verify that this is the current version before use.

Table V. Schedule of Loading and Reading

Time		Load	Dial Reading (1)
min.	sec.	gm.	mm.
0	00	1,500	
0	30	1,500- - -	- - - A
1	00	2,000	
1	30	2,000	
2	00	2,500	
2	30	2,500- - -	- - - B
3	00	3,000	
3	30	3,000	
4	00	3,500	
4	30	3,500- - -	- - - C

Deflection at 2,500 gm. = B minus A
Deflection at 3,500 gm. = C minus A
(1) Readings shall be made to the nearest 0.01 mm.

The difference between the deflections at the initial load and at specified loads shall be taken as the deflections of the specimen. The recorded deflections shall be reported to the nearest 0.1 mm.. When the determined number falls midway between two numbers, the even number shall be recorded.

4.4.4 Leakage test. The bottles of liquid with closures and seals in place shall be subjected to the leakage test as specified in PPP-C-186 for immediate containers holding liquids, except that sampling for this test shall be as specified herein in 4.2.3.

4.4.5 Unit size. A portion of powder and liquid shall be mixed according to manufacturer's instructions, and the volume shall be calculated to the nearest cubic centimeter. Calculate the number of mixes (20 cubic centimeters minimum each) obtainable from unit package.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One package, consisting of one container of powder having a minimum net weight of 1 pound and one container of liquid containing 8 fluid ounces (minimum), constitute one unit of issue. The liquid shall be at least 10 percent in excess of the amount required for the powder. A suitable powder scoop and liquid measure shall be included. In addition, if the resin is formulated for pouring consistency, a tray former shall be supplied.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:35Z
Check the source to verify that this is the current version before use.

5.1.2 Packaging quantities. The number of units of issue indicated in table VI shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table VI. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	Not required	12 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Immediate container. Powders shall be packaged in wide-mouth glass bottles of suitable size and design. Liquids shall be packaged in narrow-mouth, light-resistant glass bottles of suitable size and design.

5.1.3.1.1 Closure for bottles of powder. Bottles containing powder shall be closed by means of a metal, continuous-thread screwcap treated inside and outside to resist corrosion. Cap shall have a tight-fitting, impervious, resilient liner which must remain in cap when cap is removed from bottle. Liner shall be vinylite or aluminum faced. As an alternate, paraffin faced liner is permitted. Cap shall be tightened to prevent leakage. Bottle shall be further sealed by an inner seal which shall cover and adhere to mouth of bottle, capable of preventing loss of contents should the cap become loosened. A suitable outer seal, when furnished, shall be acceptable.

5.1.3.1.2 Closure for bottles of liquid. Bottles containing liquid shall be closed by means of a continuous-thread screwcap, fabricated of 1.25 hot-dipped tinplate or 0.50 electrolytic tinplate. Screwcap shall be treated inside and outside with a clear lacquer to resist corrosion. Cap shall have a tight-fitting, impervious, resilient liner which must remain in cap when cap is removed from bottle. Liner shall be aluminum faced. Cap shall be tightened to prevent leakage. Bottle shall be further sealed by an inner seal which shall cover and adhere to mouth of bottle, capable of preventing loss of contents should the cap become loosened. The bottles of liquid with closures and seals in place shall not leak when tested as specified in 4.4.4.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:35Z
Check the source to verify that this is the current version before use.

5.1.3.1.3 Compatibility of container. The container, closure, and liner shall not interact physically or chemically with the substance contained so as to be altered or to alter the strength, quality, or purity of the container contents.

* 5.1.3.2 Unit package. Each unit of issue shall be packaged in a box constructed in accordance with PPP-B-636, type CF, class domestic; or PPP-B-676. Bottles shall be protected by flexible corrugated fiberboard sleeves or by suitable interior fittings in such a manner as to secure the bottles in a vertical position and to insure against shifting or damage. Commercial colors are acceptable on unit packages and the closure shall be adequate to prevent spilling of contents under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A.

* 5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant. Closure and strapping shall be as specified in the appendix of the applicable box specification. Special requirements of Table II of PPP-B-636 shall apply for fiberboard boxes.

* 5.2.1.2 Case liner. Each Level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Each fiberboard box shall be waterproofed in accordance with 30.4 of PPP-B-636.

5.2.2 Level B.

* 5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Fiberboard boxes shall be closed by method II of PPP-B-636. Special requirements of Table I in PPP-B-636 shall apply for fiberboard boxes.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:35Z
Check the source to verify that this is the current version before use.

5.3 Marking.

* 5.3.1 Interior packages. Each bottle shall be commercially identified and shall show the lot (control) number. Each bottle of liquid shall also be marked with the word "Flammable". Each unit box shall be marked with stock number, item identification, lot (control) number, contract or purchase order number, type of resin (e.g., if the powder is a mixture of methyl and ethyl methacrylate it shall be stated), date of manufacture (month, year), unit, quantity, name of contractor, and the legend: "Store in a cool, dark place."

* 5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129. Lot (control) number and date of manufacture shall be shown. Date packed shall not be required. Marking shall include the legend:

"STORE AT CONTROLLED ROOM TEMPERATURE (59°-86° F.)".

6. NOTES

6.1 Intended use. The acrylic resin shall be suitable for fabricating dental impression trays and baseplates (see 1.1).

6.2 Ordering data. Procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

* 6.3 Federal Stock Number (FSN) coverage. This specification covers the following item appearing in the Federal Supply Catalog: 6520-889-9566, RESIN, ACRYLIC, DENTAL, Impression Tray Material, 1 lb.

6.4 Specification changes. The margins of this specification are marked with an asterisk to indicate where changes (additions, modifications, corrections, or deletions) from the previous issue were made. The marking was done as a convenience only, and the Government assumes no liability whatsoever for any inaccuracies in these notations. Bidders and contractors are cautioned to evaluate the requirements of this document based on the entire content, irrespective of the marginal notations and relationship to the previous issue.

Source: https://assist.dla.mil -- Downloaded: 2026-02-21T08:05Z
Check the source to verify that this is the current version before use.

6.5 Limitations. This specification does not cover all types, classes, grades, styles, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover those items which are normally procured to meet Military requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6520-1312

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:35Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:35Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

MIL-R-36433B

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:35Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE INFORMATION SUBMITTED ON THIS FORM SINCE ANY CHANGES OR DELETIONS IN THE SPECIFICATIONS MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CANNOT BE CONSIDERED FOR AWARD.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, Pa. 19101

Defense Supply Agency

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:35Z
Check the source to verify that this is the current version before use.