COMMERCIAL ITEM DESCRIPTION

ADAPTER, SYRINGE TO TUBING

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers one type of syringe to tubing adapter.

Salient characteristics:

Style and design. Shall be a syringe-to-tubing adapter conforming to Figure 1. The adapter shall contain a finger-grip, hose-end and Female Luer-Lock. The design of the Female Luer-Lock shall be in accordance with ANSI/HIMA MD70.1 when tested in accordance with the dimensional test specified therein.

Performance. The adapter shall effect a leak-tight connection between a Luer-Lock syringe and 1/8 inch I.D. Rubber tubing. When rubber tubing is connected, the tubing-to-adapter connection shall not separate under a 2 lb. tensile load. The adapter shall pass the test specified in ANSI/HIMA MD70.1. Prior to testing, rubber tubing shall be secured to the adapter's hose-end and closed with a suitable pinch-clamp.

Material. The adapter shall be fabricated from properly tempered Type 260, 270, or 360 brass conforming to GG-I-526.

Corrosion-resistance. The adapter shall pass the boil and salt-spray tests specified in GG-I-526.

Finish. The adapter shall be plated as specified in GG-I-526 for Type 260 brass. As an alternate, the adapter may be nickel-plated. Nickel plating shall conform to QQ-N-290. The plated adapter shall have a smooth, uniform finish.

Workmanship. The adapter shall be free from nicks, dents, burrs sharp edges, slivers, and any other defects that detract from its appearance or impair its serviceability. The adapter shall be supplied clean.

Unit. Each (EA). One adapter as specified, constitutes one unit.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 202610-26T08:55Z
Check the source to verify that this is the current version before use.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105. Inspection shall be conducted at Level II, AQL (Acceptable Quality Level) 1.0 percent. The unit of product for test purposes shall be one adapter.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:55Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-00-300-0720	ADAPTER, SYRINGE TO TUBING, Brass

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

Source: https://assist.dla.mil -- Downloaded: 202610-26T08:55Z
Check the source to verify that this is the current version before use.

CIVIL COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-3583

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:55Z
Check the source to verify that this is the current version before use.

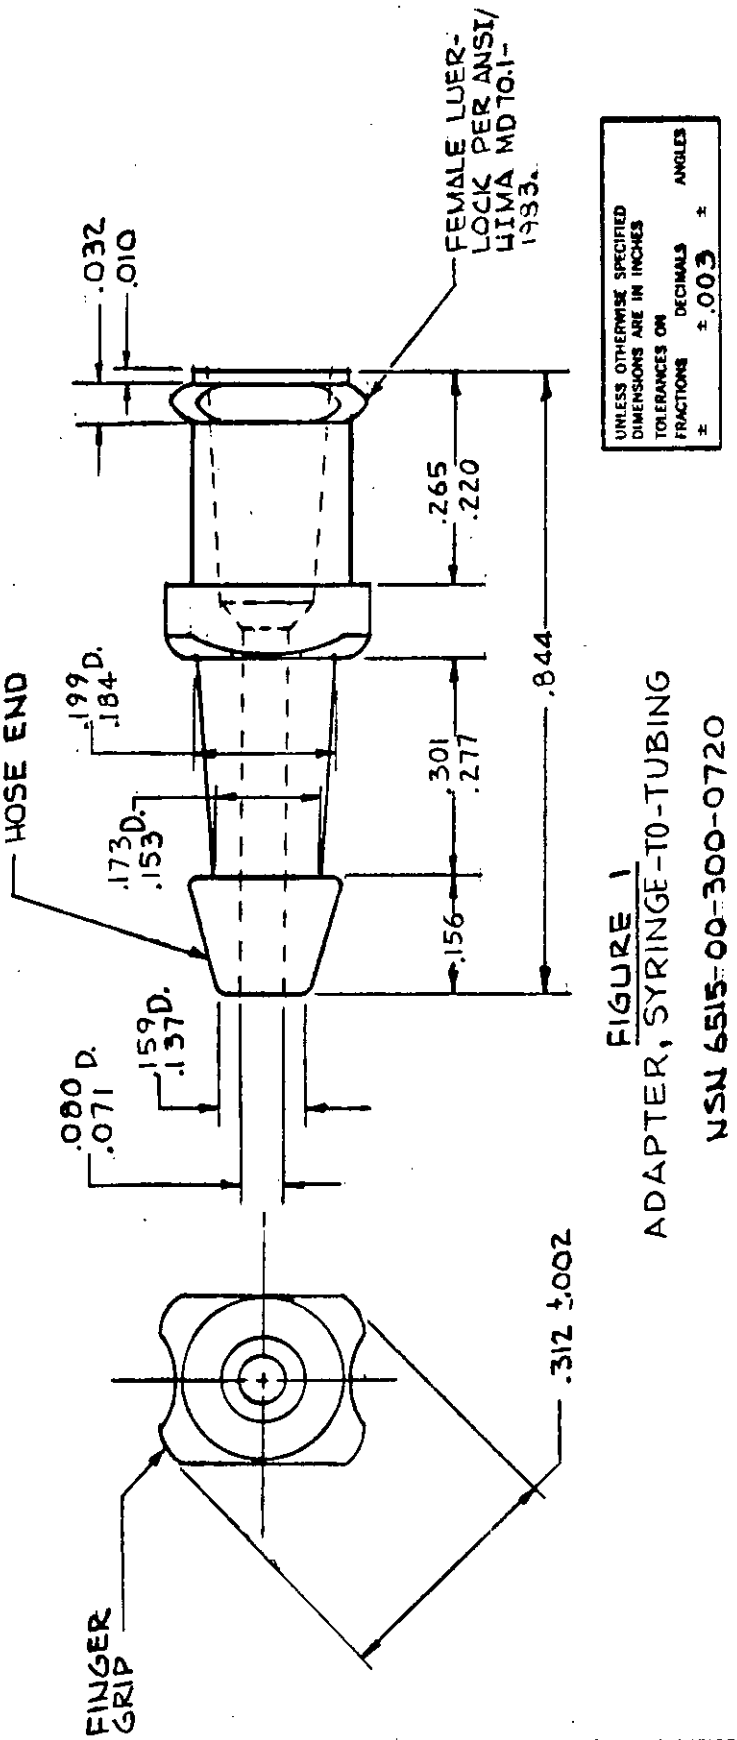


FIGURE 1
ADAPTER, SYRINGE-TO-TUBING
NSN 6515-00-300-0720

☆U.S. GOVERNMENT PRINTING OFFICE: 1986 — 605-036/45213

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:55Z
Check the source to verify that this is the current version before use.