A-A-51430
20 May 1986

COMMERCIAL ITEM DESCRIPTION

SPLINT, SET, ARCH WIRE, DENTAL AND
BAND, LIGATURE, DENTAL

The General Services Administration has authorized the use of this commercial item description in preference to Interim Federal Specification GG-S-00627b (DSA-DM).

This commercial item description covers an arch wire splint set and replacement ligature bands suitable for the fixation of fractures of the jaw.

Salient characteristics:

The arch wire splint set shall be suitable for the fixation of fracture of the jaw. The set shall be of the Winter design and shall consist of 2 splints, 10 ligature wires with dental floss, and 24 rubber bands. The replacement ligature bands shall consist of 48 rubber bands.

The splint shall consist of a base arch wire to which attachment pins shall be soldered. Each pin shall have a body and a round head. There shall be not less than 5 pins for each 1-inch length of base wire. The splint shall be made of copper alloy composition 752, dead-soft annealed temper, and shall be plated with rhodium. The splint shall conform to Figure 1 in style, design and dimensions.

The ligature wire shall be 0.018 ± 0.001 inch in diameter and 8.5 ± 0.05 inches long. The wire shall be bent over itself in the center, and shall have 9 ± 1/2 inch piece of dental floss inserted at the bend. The wire shall be gold or rhodium plated brass, or soft AISI 304 stainless steel with a tensile strength of 80,000 to 120,000 pounds per square inch (psi). The dental floss shall be composed of waxed nylon continuous filaments. The floss shall be at least 960 denier with a tensile strength of at least 13.0 pounds.

AMSC N/A FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:55Z
Check the source to verify that this is the current version before use.

The rubber bands shall be made from live Para rubber or pale crepe rubber. The outside diameter shall be 1/4 ± 1/32 inch, thickness shall be 0.031 ± 0.005 inch and width shall be 0.062 ± 0.005 inch. Dimensions shall be determined by conventional measuring devices (toolmaker's microscope, suitable scales). The rubber bands shall have a minimum tensile strength of 1300 psi and a minimum ultimate elongation of 700 percent (%). After accelerated aging, the bands shall show no more than 20% loss in tensile strength and no more than a 10% loss in ultimate elongation from the original values. Testing shall be conducted in accordance with American Society for Testing and Materials (ASTM) standards: ASTM D412-83 Rubber Properties in Tension, 26 August 83, and ASTM D572-81, Rubber, Deterioration by Heat and Oxygen, 27 March 81, or the latest edition thereof.

Workmanship. The splint set and bands shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Set (SE) or Package (PG). One arch wire splint set or one package containing 48 dental ligature bands, as specified, constitutes one unit.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:55Z
Check the source to verify that this is the current version before use.

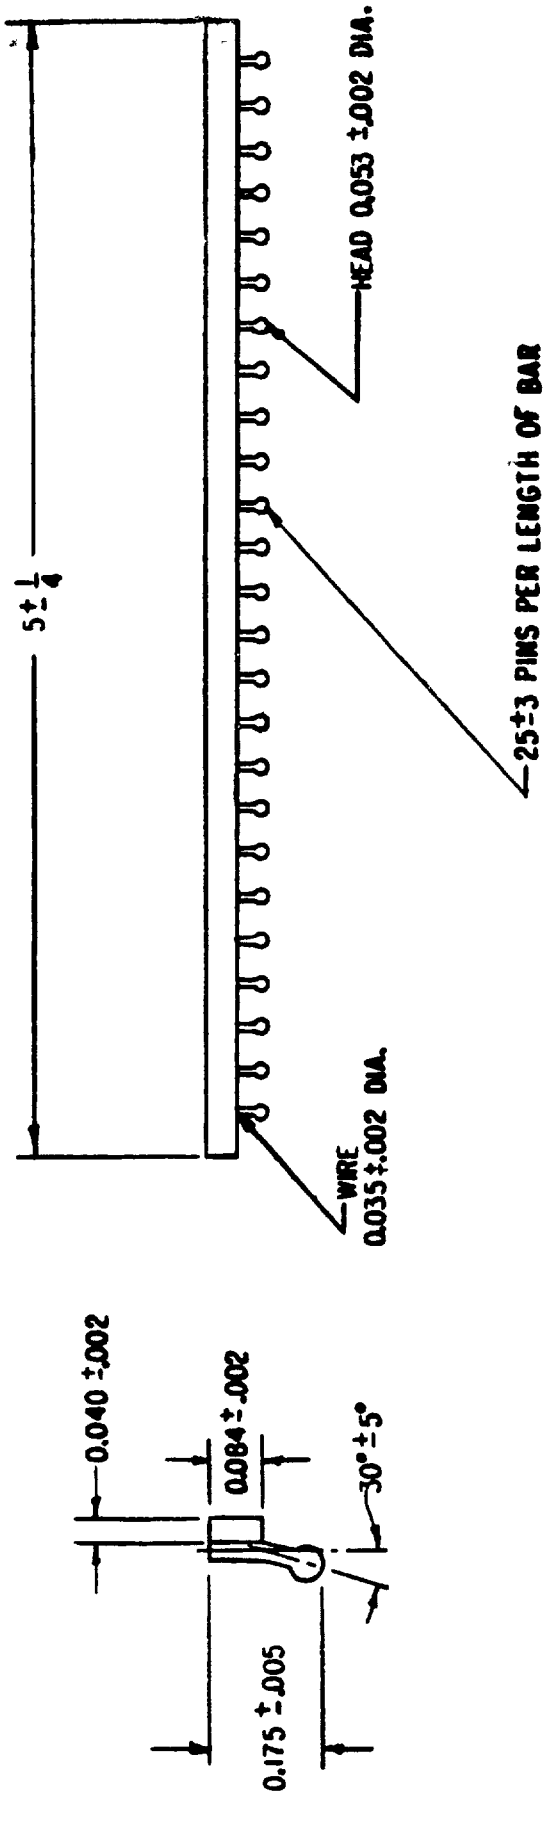


FIGURE I SPLINT SET

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T
Check the source to verify that this is the current version be

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more inspection characteristics. The unit of product inspection purposes shall be one splint set or one replacement band. Unless otherwise specified, sampling for examination shall be conducted at inspection level II, AQL 2.5, and sampling for tests (when applicable) shall be conducted at inspection level S-1, AQL 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:55Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

Stock Number	Item Identification
6520-00-299-8284	SPLINT SET, ARCH WIRE, DENTAL
6520-01-094-1970	BAND, LIGATURE, DENTAL, Rubber, Assorted, 48s.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:

DLA - DM

CIVIL AGENCY COORDINATING ACTIVITY

VA-OSS

Project No. 6520-1927

47600
49069

Location: NCR

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:55Z
Check the source to verify that this is the current version before use.