FEDERAL SPECIFICATION

CABINETS, COMPARTMENTED, METAL; DENTAL, FOR PORCELAIN TEETH

This specification was approved on the above date by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. CLASSIFICATION

1.1 Type and grade.—Cabinets for porcelain teeth covered by this specification shall be of one type and grade.

2. APPLICABLE SPECIFICATIONS AND OTHER PUBLICATIONS

2.1 The following Federal Specifications, of the issues in effect on date of invitation for bids, form a part of this specification:

QQ-A-561—Aluminum (AL-2); Plate and Sheet.

QQ-S-636—Steel; Carbon (Low-Carbon), Sheets and Strips.

TT-E-491—Enamel; Gloss, Synthetic (for Metal and Wood Hospital Furniture).

TT-P-659—Primer-Surfacer; Synthetic, Tints and White (for Metal and Wood Hospital Furniture).

(Copies of Federal specifications and the Federal Specifications Index may be obtained upon application, accompanied by postal note, money order, coupon, or cash, to the Superintendent of Documents, Government Printing Office, Washington 25, D. C. Prices may be obtained from the Superintendent of Documents.)

2.2 Specifications and other publications applicable only to individual departments are listed in section 7.

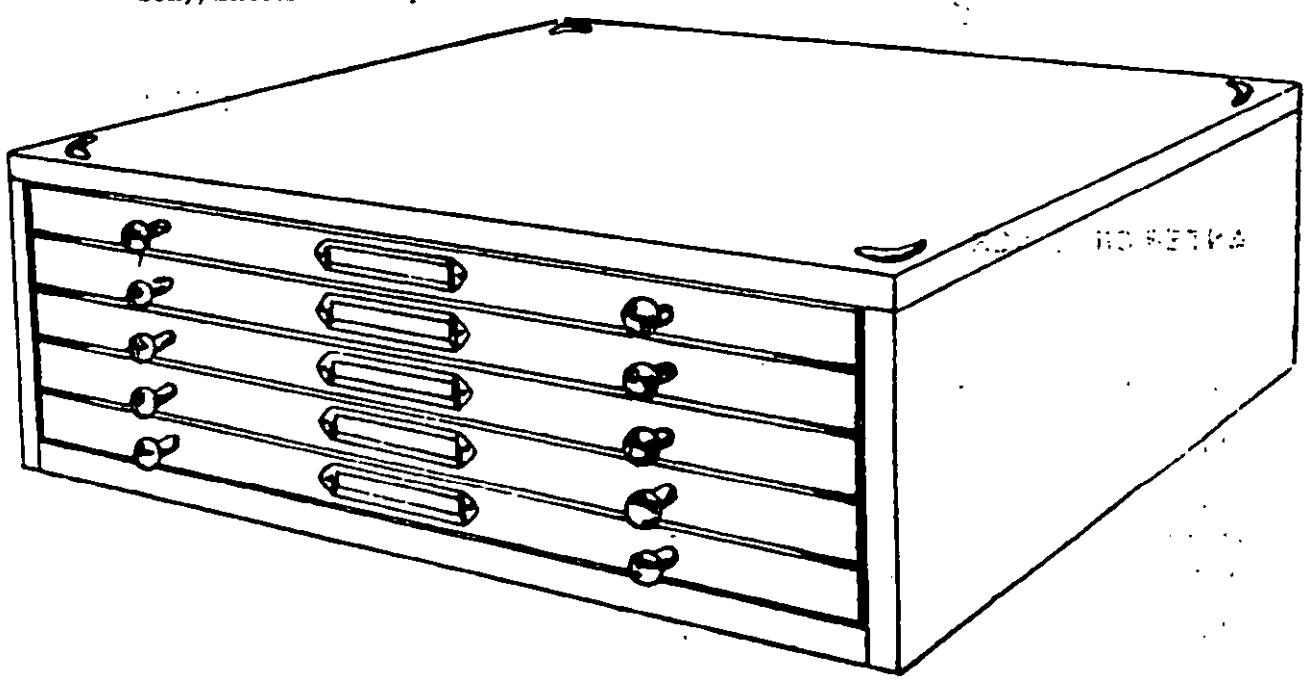


FIGURE 1.—Cabinet, compartmented, metal; dental, for porcelain teeth.

501682—50—(401)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

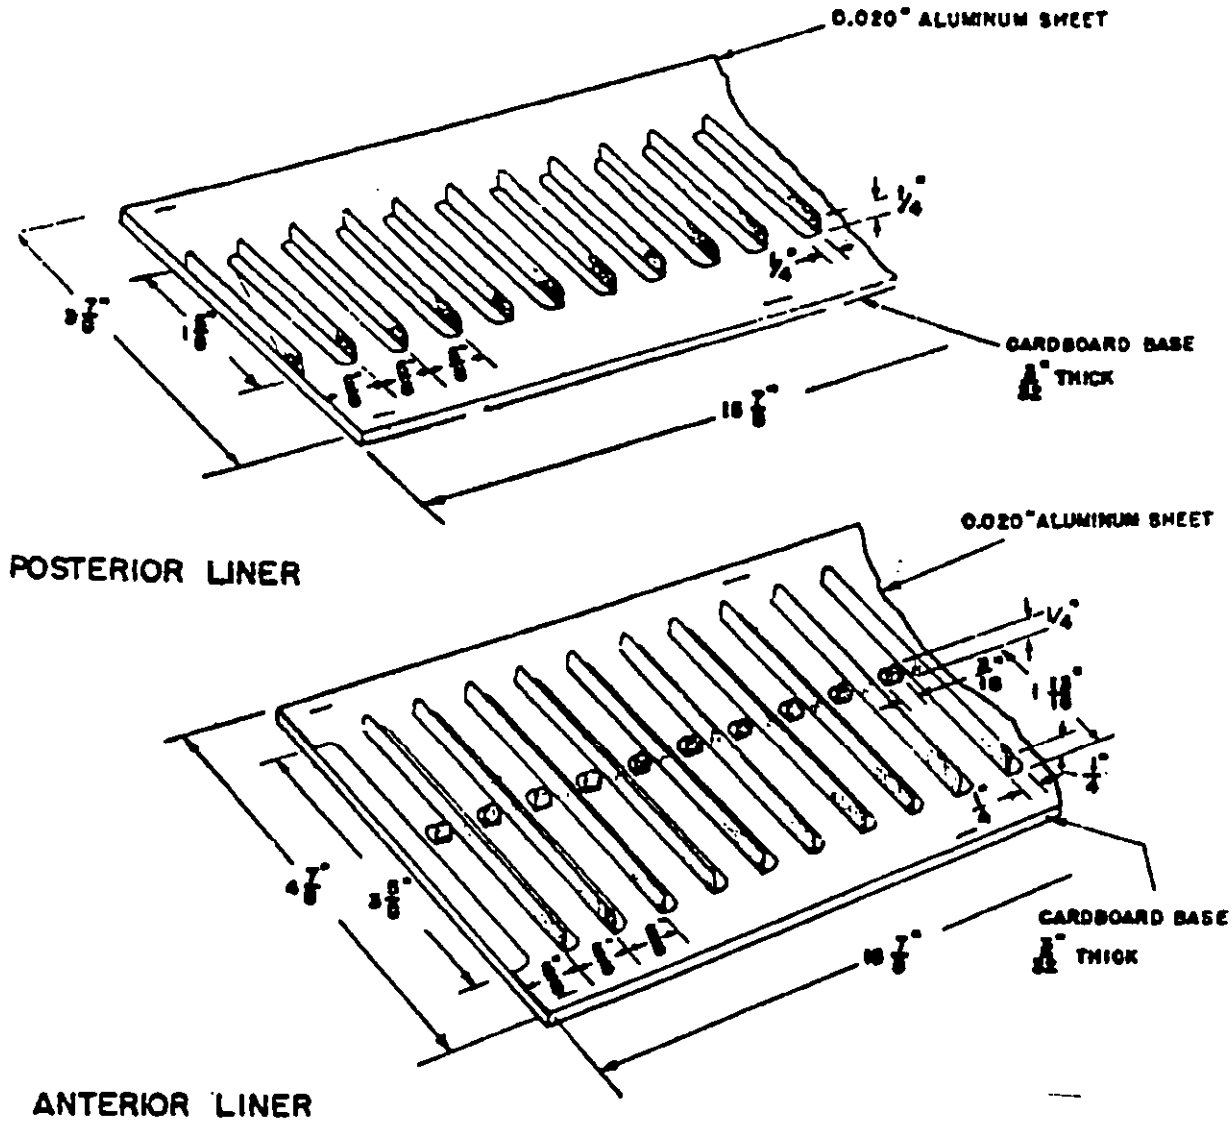


FIGURE 2.—Drawer liners for dental compartmented cabinet.

3. REQUIREMENTS

3.1 Material.

3.1.1 *Aluminum.* — The aluminum shall conform to the requirements of Federal Specification QQ–A–561 for condition A.

3.1.2 *Steel.*—The steel shall conform to the requirements of Federal Specification QQ–S–636 for cold-rolled steel.

3.1.3 *Gloss enamel.* — The gloss enamel shall conform to the requirements of Federal Specification TT–E–491 for class B.

3.1.4 *Primer.*—The primer shall conform to the requirements of Federal Specification TT–P–659.

3.1.5 *Other material.*—All other material shall be of high commercial quality throughout and shall be suitable in every respect for the purpose intended.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

3.2 Cabinet.—The cabinet shall be constructed of aluminum or steel and shall be of the general design shown in figure 1. The steel shall be not less than 0.032 inch in thickness. The cabinet shall be of welded construction throughout. The cabinet shall be approximately 17½ inches wide, approximately 16⅝ inches deep, and approximately 5⅞ inches high. A raised crescent made of steel not less than 3/32 inch in thickness shall be welded to each corner as shown in figure 1. Each corner of the bottom shall have a semicircular indentation that will fit the corresponding raised crescent on the top when two or more cabinets are stacked. The cabinet shall have five drawers complete with liners as specified in 3.3 and 3.4.

3.3 Drawers.—The drawers shall be approximately 16 7/16 inches wide, approximately 16½ inches deep, and the sides approximately 2 7/32 inch high. The drawers shall slide on metal strips not less than ½ inch wide. The inside of the drawers shall be not less than 16 3/32 inches wide and shall be suitable for holding the drawer liners. Each drawer front shall be fitted with two chromium-plated knobs and a chromium-plated label holder as shown in figure 1. All knobs and label holders shall be of matched design.

3.4 Drawer liners.—Each drawer shall be furnished with aluminum drawer liners, constructed to form dividers, to segregate and file anterior and posterior teeth. The liners shall be of the general design shown in figure 2 and shall be designed to prevent sliding over one another. The liners shall be made from bright aluminum sheet not less than 0.020 inch in thickness. The aluminum sheet shall be punched at intervals of approximately ⅝ inch and bent to form dividers. Unless otherwise specified, the liners shall have a cardboard base.

3.4.1 *Anterior liners.*—The anterior liners shall be approximately 15⅞ inches long and approximately 4⅞ inches wide. The liners shall be punched to form dividers approximately 3⅝ inches long by approximately ¼ inch wide. The recesses thus formed shall be punched in the center approximately 3/16 inch long by approximately ¼ inch wide to provide two rows for filing 25 sets of anterior teeth in each row.

3.4.2 *Posterior liners.*—The posterior liners shall be approximately 15⅞ inches long and approximately 3⅞ inches wide. The posterior liners shall be punched to form dividers approximately 1⅝ inches long by ¼ inch wide to provide one row of recesses for filing 25 sets of posterior teeth.

3.4.3 *Distribution.* — Unless otherwise specified, the cabinet drawers shall contain the following distribution of anterior and posterior liners:

First drawer—three anterior liners.
Second drawer—two anterior liners and one posterior liner.
Third drawer—four posterior liners.
Fourth drawer—four posterior liners.
Fifth drawer—four posterior liners.

If necessary to provide a snug fit, fillers between the liners shall be provided.

3.5 Finish.—The inside and outside surfaces of the cabinet shall be finished with a coat of primer surfacer of neutral tint conforming to the requirements of Federal Specification TT–P–659 followed by two coats of enamel of the specified color (see 6.2), conforming to the requirements of Federal Specification TT–E–491.

3.6 *Identification marking.*—Each cabinet shall be permanently and legibly marked with the name or registered trade-mark of the manufacturer.

3.7 Workmanship. — The workmanship shall be first class throughout. The cabinets shall be free from any imperfections which detract from their appearance or which may impair their serviceability.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Sampling.

4.1.1 *Cabinets.* — Unless otherwise specified, two cabinets shall be taken at random from each lot of 100, or fraction thereof, delivered.

4.1.2 *Enamel and primer.*—Unless otherwise specified, the manufacturer shall furnish 1 quart each of enamel and primer from the same lots as those used in the manufacture of the cabinets.

4.2 Inspection.—Each sample cabinet shall be inspected for material, design, dimensions, presence of parts, construction, finish, workmanship, packaging, packing, and marking.

4.3 Tests.

4.3.1 *Material.* — Tests for material shall be conducted as described in the applicable specifications listed in 2.1.

5. PREPARATION FOR DELIVERY

5.1 Packaging. — Unless otherwise specified, each cabinet shall be packaged in accordance with accepted commercial practice.

5.2 Packing.—The cabinets shall be prepared for shipment to permit acceptance by carrier for transportation at the lowest applicable rate, and to afford maximum protection from normal hazards of transportation.

5.3 Marking.

5.3.1 *Packages.*—Unless otherwise specified, each package shall be marked with the name of the commodity, the stock number, the quantity contained therein, and the names of the contractor and manufacturer.

5.3.2 *Shipping containers.*—Unless otherwise specified, shipping containers shall be marked with the name of the commodity as defined by the contract or order under which the shipment is made, the quantity contained therein, the name of the contractor, the number of the contract or order, the name and address of the consignee, and the gross weight.

6. NOTES

6.1 Intended use.—The cabinets covered by this specification are intended for use in dental prosthetic laboratories for segregating and filing porcelain teeth.

6.2 The enamel specified for finishing the cabinets covered by this specification may be obtained in white or tints. The desired color should be specified in the invitation for bids, contract, or purchase order. To obtain a match for a particular color, the seller and testing laboratory should be supplied with wet samples or color chips of the color desired. In general, white enamel may be purchased without reference to a standard.

6.3 Ordering data.—Purchasers should exercise any desired options offered herein. (See 3.4, 3.4.3, 4.1, 5.1, 5.3, and 7.2.6.)

6.4 This specification covers the following stock number listed in the Armed Services Catalog of Medical Materiel.

5–110–010 — Cabinet, Compartmented, Porcelain Teeth.

6.5 It is believed that this specification adequately describes the characteristics necessary to secure the desired material, and that normally no samples will be necessary prior to award to determine compliance with this specification. If, for any particular purpose, samples with bids are necessary, they should be specifically asked for in the invitation for bids, and the particular purpose to be served by the bid sample should be definitely stated, the specification to apply in all other respects.

6.6. This specification does not include all types, classes, grades, sizes, etc., of the com-

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

modity indicated by the title of the specification, or which are commercialy available, but is intended to cover the types, etc., which are normally procured for Federal Government requirements.

Patent notice.—When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

7. DEPARTMENTAL REQUIREMENTS

7.1 The following specifications and other publications, of the issues in effect on date of invitation for bids, and special requirements, form a part of this specification for purchases made under this specification by the respective departments.

7.2 Army, Navy, and Air Force.

7.2.1 *Applicable specifications and other publications.*

Federal Specifications:

NN-B-601 —Boxes; Wood-Cleated-Plywood, for Domestic Shipment.

NN-B-621 —Boxes; Wood, Nailed and Lock-Corner.

NN-B-631 —Boxes; Wood, Wirebound, for Domestic Shipment.

LLL-B-631 —Boxes, Fiber, Corrugated (for Domestic Shipment).

LLL-B-636 —Boxes, Fiber, Solid (for Domestic Shipment).

Military Specifications:

JAN-P-105 —Packaging and Packing for Overseas Shipment — Boxes, Wood, Cleated, Plywood.

JAN-P-106 —Packaging and Packing for Overseas Shipment — Boxes; Wood, Nailed.

JAN-B-107 —Boxes, Wood, Wirebound (Overseas Type).

JAN-P-125 —Packaging and Packing for Overseas Shipment — Barrier-Materials, Waterproof, Flexible.

JAN-P-140 —Packaging and Packing for Overseas Shipment — Adhesives, Water-Resistant, Case-Liner.

MIL-M-3157—Marking of Domestic Shipments by Contractors for Supplies and Equipment Consigned to the Medical Departments of the Armed Services.

U. S. Army Specification:

3-1—Paint and Related Materials, General Specifications for Inspection and Tests.

Navy Department Specification:

General Specifications for Inspection of Material.

(Copies of specifications required for Army purchases may be obtained upon application to the procuring agency. Both the title and identifying symbol or number should be stipulated when requesting copies.

(Copies of Federal and Military specifications required for Navy purchases and Navy Department specifications may be obtained without cost upon application to the Bureau of Supplies and Accounts, Department of the Navy, Washington 25, D. C., except that Naval activities should make application to Supply Officer in Command, Naval Supply Center, Norfolk 11, Virginia. Both the title and identifying symbol or number should be stipulated when requesting copies of specifications.

(Copies of specifications required for Air Force purchases may be obtained upon application to the Commanding General, Air Matériel Command, Wright-Patterson Air Force Base, Dayton, Ohio. Both the title and identifying symbol or number should be stipulated when requesting copies.)

7.2.2 *Finish.*—Unless otherwise specified, the inside and outside surfaces of the cabinet shall be finished in a neutral coat of primer followed by two coats of medium gray metal-

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:48Z
Check the source to verify that this is the currentversion before use.

lic wrinkle enamel conforming to No. 123 in the Color Card Supplement to Department of the Army Specification 3–1.

7.2.3 *Packaging.*—One cabinet constitutes one unit. Each cabinet shall be packaged in a box of appropriate size conforming to the requirements of Federal Specification LLL–B–631 or LLL–B–636. Each box shall be adequately secured to prevent accidental opening. Each box shall contain sufficient cushioning material (Kimpak, cellulose, excelsior, die-cut pads, cells, etc.) to insure against shifting or breakage.

7.2.4 *Packing.*

7.2.4.1 *Domestic.* — Each unit shall be packed in a shipping container conforming to the requirements of Federal Specification NN–B–601, NN–B–621, or NN–B–631.

7.2.4.2 *Overseas.* — Each unit shall be packed in a shipping container designed for type 2 load and conforming to the requirements of Military Specification JAN–P–105, JAN–P–106, or JAN–B–107. Closure and strapping shall conform to the requirements of the appendix to the applicable box specification. Each shipping container shall be lined with a sealed waterproof bag, or its equivalent, made from material conforming to the requirements of Military Specification JAN–P–125, for case-liners; seams and closures shall be sealed with a continuous seam at least ¾ inch wide of water-resistant adhesive conforming to the requirements of Military Specification JAN–P–140.

7.2.5 *Marking.*

7.2.5.1 *Packages.*—Each package shall be marked with the stock number, nomenclature, unit, quantity, and the name of the contractor. When the contractor is not the manufacturer, the name of the manufacturer shall also appear as the manufacturer.

7.2.5.2 *Shipping containers.* — Each shipping container shall be marked in accordance with Military Specification MIL–M–3157.

7.2.6 *Ordering data.* — Requests, requisitions, schedules, and contracts or orders should specify domestic or overseas packing and marking of shipping containers (see 7.2.4 and 7.2.5.2).

NAVY: MS

This specification is a part of Section IV, Part 5, of the Federal Standard Stock Catalog.

For sale by the Superintendent of Documents, Washington 25, D. C. Price 5 cents.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.