GG-H-0080a (DSA-DM)
AMENDMENT-1
9 September 1970

AMENDMENT

TO

INTERIM FEDERAL SPECIFICATION

HANDLE AND BLADE SET, SURGICAL KNIFE, DETACHABLE BLADE

This amendment was developed by the Department of Defense, Defense Supply Agency, Defense Personnel Support Center, Directorate of Medical Materiel, Philadelphia, Pennsylvania 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above.

The General Services Administration has authorized the use of this amendment as a valid exception to Interim Federal Specification GG-H-0080a, dated 27 December 1967.

1.2.1 Sizes and types. Delete heading and substitute:

"1.2.1 Sizes, types, and styles. "Line 3, delete "and" and insert ",". Line 3, after types add ", and styles". Add to end of paragraph: "Styles a and b are both intended for existing handle."

1.2.3 Blades. Under "Size 1" add the following:

"Style a - regular dimensions
"Style b - additional dimensions"

Under "Size 2" add the following:

"Style a - regular dimensions
"Style b - additional dimensions"

FSC 6515, 6520

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

3.1.1.2.2 Grade B. Second and third lines delete "B122-60, alloy 3" and substitute "B122, alloys No. 740 and 745". Fifth line delete "68.5" and substitute "73.5". Seventh line delete "19" and substitute "14".

3.1.2.1 Composition A. Last line, after "83" add "(45N 64 to 73)".

3.6.1 Design. Second sentence, delete period and add ", except that figure 4C' shall apply instead of figure 4C". After second sentence, insert "However, for the Type EE blade shown in figure 5e delete "6°/9°" and substitute "5-1/2° to 8-1/2°". Before last sentence insert "Type EE blades, however, shall be thicker along back edge for the purpose of reinforcement."

3.6.2 Tang. Line 4 after "6" add "and figure 10". Last line delete "the" and add "6" after "figure". Add the following to the end of the paragraph: "Dimensions of blades shall be checked by Go and No-Go gages (figure 8) as described in 4.4.1. Blades not passing Go and No-Go gages shall then be subjected to examination by means of a comparator as stated in 4.4.1.1. Blades not passing the dimensional examination on the comparator shall be rejected.

"Style b represents an additional set of dimensions which in no way indicates or implies a change in handle dimensions whether for Size 1 or Size 2 blades. Style a dimensions remain as they are stated in GG-H-0080a. Blades may be submitted under either style, but shall not be accepted when complying partially with Style a dimensions and partially with Style b dimensions."

3.6.3.1 Sharpness and cutting edge angle. Line 3 delete "36" and substitute "38". Line 4 delete "± 5" and substitute "+7,-5".

Figure 6. Design of Tang of Blade. Insert "Style a" under "BLADES". Add this additional set of dimensions as follows:

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

	Size	A	B	C	D	E	F	G	H	I
Blades Style b	1	.240 to .265	59 to 61	.126 to .159	.702 to .709	.095 to .099	.0462 to .051	.055 to .071	.360 to .410	.060 to .090
	2	.275 to .375	54 to 56	.224 to .250	.9536 to .957	.145 to .151	.076 to .081	.090 to .110	.420 to .500	.105 to .140

3.6.6 Assembly. After first sentence insert "However, for Type EE blades, the requirements for sterility, freedom from pyrogens, and safety shall not apply."

3.8.3 Certificate of safety. First sentence, delete "A" and substitute "Unless otherwise specified, a".

4. QUALITY ASSURANCE PROVISIONS

Delete paragraphs 4.1, 4.1.1, and 4.1.2 in their entirety and substitute the following:

"4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

"4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

"4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item."

Add the following:

"4.4.1.1 Comparator examination. Blades not passing the Go and No-Go examination, shall be subjected to examination by means of the Jones and Lamson comparator, or equal, at 25 to 35 X magnification."

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

5.1.3.2.2 Blade: composition B (stainless steel). Delete entirely and substitute:

"5.1.3.2.2 Blade: composition B (stainless steel). Each blade shall be packaged in the same manner as specified in 5.1.3.2.1 except that the anticorrosive paper will not be required. The complete package shall be closed by heat sealing. The complete package shall be such as to maintain sterility until package is opened."

Delete paragraphs 5.1.3.2.3 and 5.1.3.3 entirely and substitute the following paragraphs:

"5.1.3.3 Unit package.

"5.1.3.3.1 Blades. Unit package shall be a box of appropriate size and constructed in accordance with PPP-B-566 or PPP-B-676, except commercial colors will be acceptable. As an alternate, each unit may be packaged in an envelope of suitable size and design.

"5.1.3.3.2 Handles. Each unit shall be packaged in accordance with MIL-P-116, method IA-8."

5.2.1.1 Exterior container. Line 3, following PPP-B-585, delete remainder of paragraph and substitute: "class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, grade V3c."

5.2.2.1 Exterior container. Delete and substitute:

"5.2.2.1 Exterior container. Exterior container shall be designed for a type II load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification."

Custodians:
Army - MD
Navy - MS
Air Force - 03


Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1517

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:48Z
Check the source to verify that this is the current version before use.

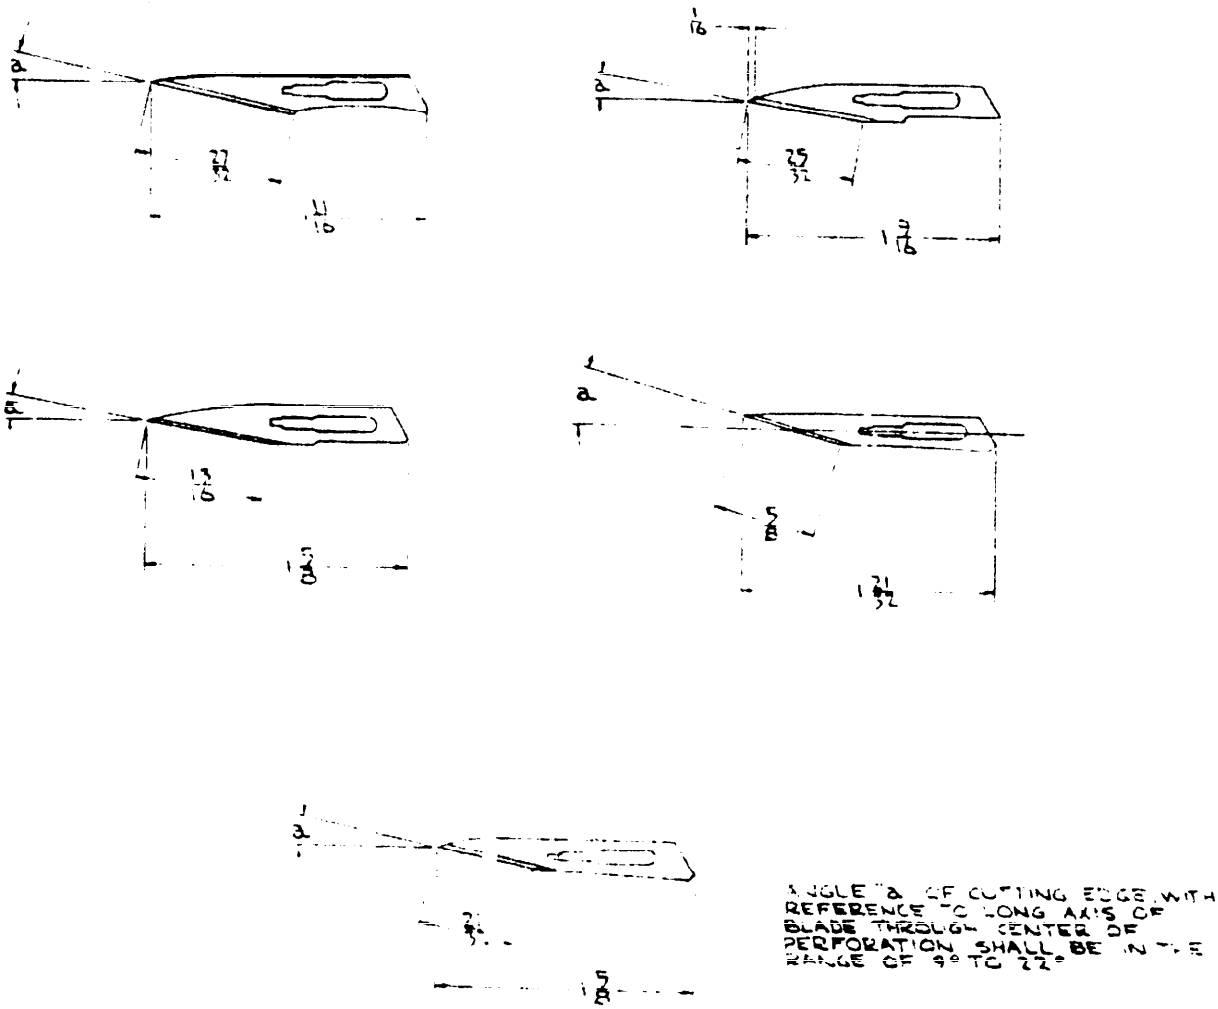

ANGLE "a" OF CUTTING EDGE WITH REFERENCE TO LONG AXIS OF BLADE THROUGH CENTER OF PERFORATION SHALL BE IN THE RANGE OF 9° TO 22°.

FIGURE 4[illegible].-

SIZE 1 BLADE SMALL TANG
TYPE CC BISTOURY STRAIGHT
ALTERNATE TIP DESIGNS

Source: https://assist.dla.mil -- Downloaded: 2026[illegible]-26T11:48Z
Check the source to verify that this is the current version before use.

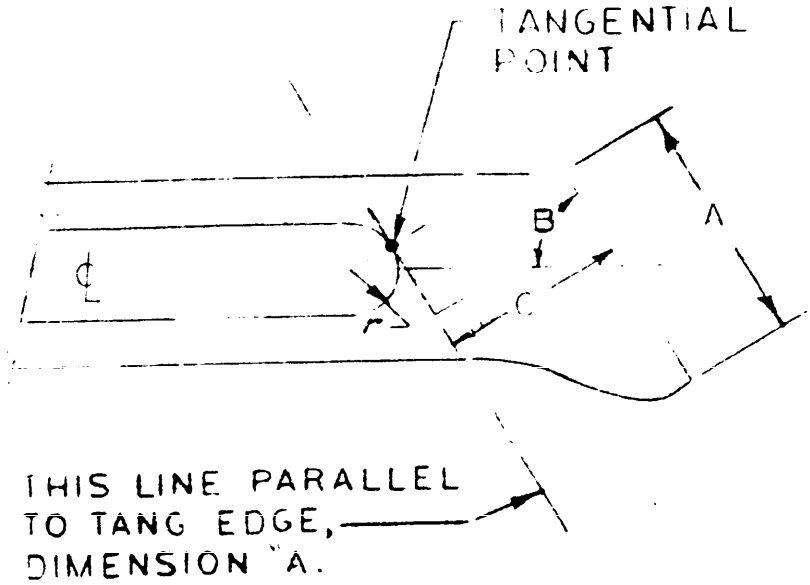


FIGURE 10.- ENLARGED VIEW OF DIMENSION "C" (OF FIGURES 3 AND 6) AND EQUIVALENT DIMENSION "C" IN FIGURE 8

☆ U. S. GOVERNMENT PRINTING OFFICE: 1970-433-691/2153

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.