FEDERAL SPECIFICATION

RACK, DRYING, RADIOGRAPHIC FILM

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 **Scope.**—This specification covers wall racks for holding radiographic-film hangers while drying X-ray film.

1.2 **Classification.**—The drying racks shall be of one type, size, grade, and two styles as specified:

Style A.— 90° Bend.

Style B.—145° Bend.

2. APPLICABLE SPECIFICATIONS

2.1 The following Federal Specifications, of the issues in effect on date of invitation for bids, form a part of this specification:

GG–H–109—Hangers, X-Ray Film Developing and Drying.

GG–H–111—Hangers, X-Ray Film (Dental); Developing and Drying.

QQ–S–766—Steel, Corrosion-Resisting, Plates, Sheets, Strips, and Structural Shapes.

(Copies of Federal specifications and the Federal Specifications Index may be obtained upon application, accompanied by check, money order, cash, or Government Printing Office coupons, to the General Services Administration, Business Service Center, Region 3, Seventh and D Streets, S. W., Washington 25, D. C. This office will also honor deposit account numbers issued by the Government Printing Office. Single copies of product specifications required for bidding purposes are available without charge at the GSA Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C. Prices of additional copies may be obtained from the GSA Regional Offices.)

2.2 Specifications and standard applicable only to individual departments are listed in section 7.

3. REQUIREMENTS

3.1 **Material.**—The radiographic-film drying rack shall be fabricated from corrosion-resistant steel sheet conforming to the requirements for class 7 finish of Federal Specification QQ–S–766. The rack shall be passivated after fabrication.

3.2 **Design style A.**—The rack shall be manufactured approximately as shown in figure 1 and shall be formed from a single piece of corrosion-resistant steel, 3 inches wide, 20 inches long, and 0.045 inch thick. The finished rack shall have approximately equal sides formed over a radius of not less than $\frac{1}{16}$ inch to approximately a 90° angle. The sides shall be not less than $1\frac{1}{4}$ inches long. The rack shall be designed to support by either end of the top hanger bar type I or type II radiographic-film hangers, constructed in accordance with Federal Specification GG–H–109. One side of the rack shall be punched or formed to support the hangers so that the top hanger bar is at an angle of 10° to 30° above horizontal. The rack shall be designed to permit easy insertion of the hanger into the rack. The rack shall support twelve hangers equally spaced $1\frac{5}{8}$ inches

203438-53-(257)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

apart. The hangers shall be supported firmly so that the breeze from a common 10-inch fan directed at loaded hangers from any angle at a distance of 48 inches will not cause adjacent hangers or films to touch. The other side of the rack shall have three holes of approximately $\frac{3}{16}$-inch diameter, located approximately as shown in figure 1, to permit mounting. The rack shall accommodate three dental film hangers in accordance with the requirements of type I Federal Specification GG–H–111.

3.3 Design style B.—The racks shall be as specified in 3.2, except the angle between the sides shall be approximately 145°, and the racks shall support hangers at an angle of approximately 8° above horizontal.

3.4 Identification marking.—Each hanger shall be permanently marked with the manufacturer's name or registered trade-mark.

3.5 Workmanship.—Workmanship shall be first class throughout. Radiographic-film hanger racks shall be free from defects which detract from their appearance or may impair their serviceability.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Sampling for lot acceptance.

4.1.1 *Inspection lot.* — For purposes of sampling, a lot shall consist of all racks offered for delivery at one time.

4.1.2 *Sampling for inspection.*—A random sample of racks shall be selected from each lot in accordance with table I to verify compliance with all stipulations of the specification regarding visual and dimensional characteristics, marking, and other requirements not involving tests.

4.1.3 *Sampling for tests.* — Unless otherwise specified, one rack shall be taken at random from each lot for testing.

TABLE I.—*Sampling for inspection*

Number of racks in lot	Number of racks in sample	Number of defectives allowed for acceptance	Number of defectives for rejection
15 and under	7	0	1
16 to 40	10	0	1
41 to 110	15	0	1
111 to 800	25	1	2
801 to 500	35	1	2
501 to 800	50	2	3
801 to 1,300	75	3	4
1,301 and over	110	4	5

4.2 Inspection.


4.2.1 *Visual and dimensional inspection.*—Each of the sample racks, selected in accordance with table I, shall be visually and dimensionally inspected by the Government inspector to verify compliance with the requirements of this specification for finish, design, marking, and workmanship. Any rack in the sample containing one or more visual or dimensional defects shall be rejected, and if the number of defective racks in any sample exceeds the acceptance number for that sample, the lot represented by the sample shall be rejected.

4.2.2 *Rejected lots.*—Rejected lots may be offered again for Government inspection provided the contractor has repaired or removed all nonconforming racks. The Government inspector shall again select and examine samples from such resubmitted lots to verify compliance with the specification.

4.3 Test procedures.

4.3.1 *Fan test.*—The drying rack shall be mounted on an appropriate support for the purpose of this test. Twelve type I, size F (14 by 17) radiographic-film hangers shall be loaded with film and inserted into the drying rack. A common 10-inch fan shall be placed 48 inches from the hangers and at about a

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

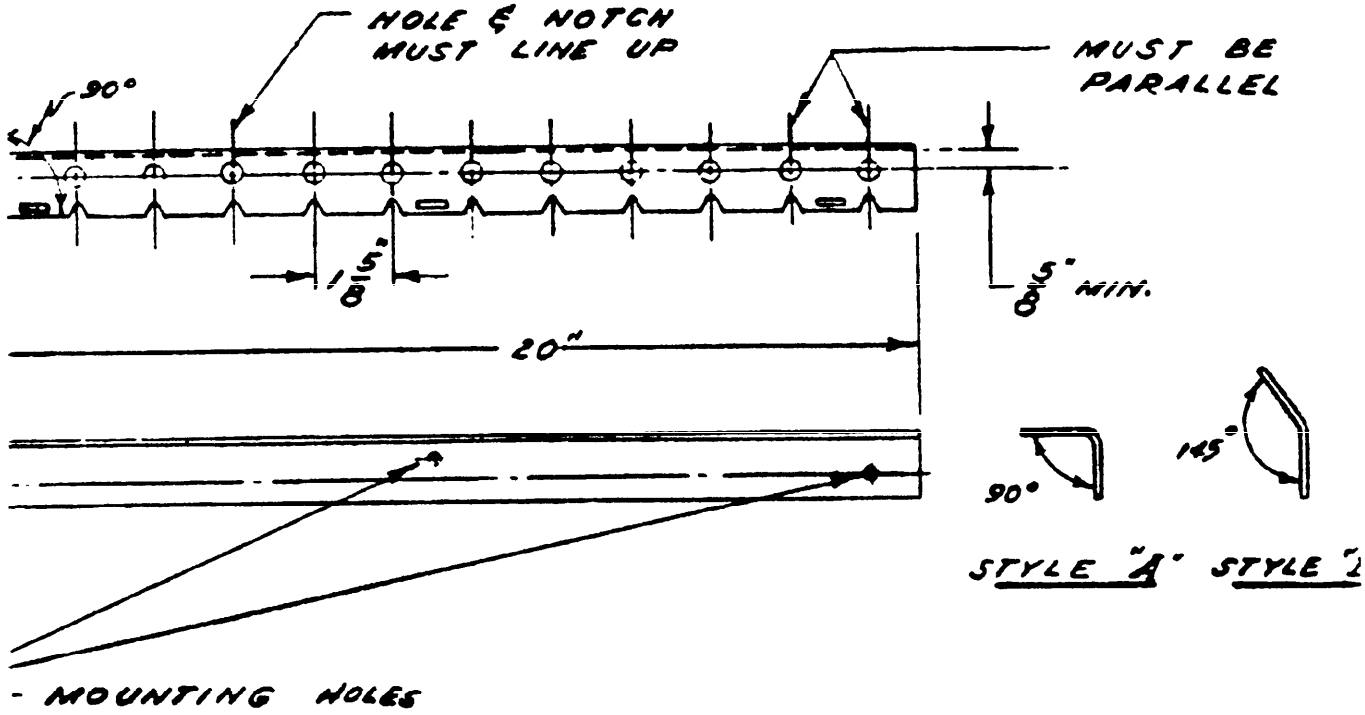

NOTE
STYLE "A" & STYLE "B" IDENTICAL EXCEPT FOR ANGLE DIFFERENCE

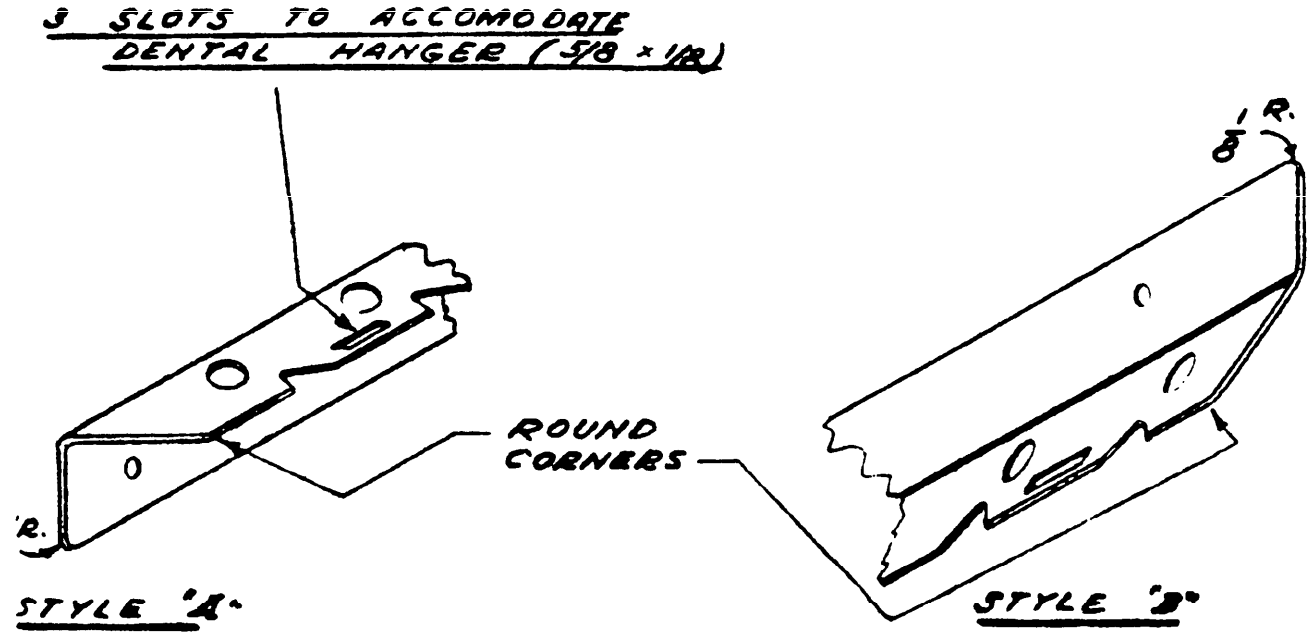


FIG. 1.
RACK, DRYING, RADIOGRAPHIC FILM

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

60° angle to the hangers. The fan shall be turned on and the hangers checked for any contact with each other or with the film. Also check for ease of inserting the hangers into the drying rack.

4.3.2 Other tests shall be conducted as necessary to determine compliance with the requirements of this specification.

4.4 **Rejection.**—When samples from a lot are tested and fail to meet the requirements of this specification, the entire lot from which the samples were taken shall be rejected.

5. PREPARATION FOR DELIVERY

5.1 **Packaging.** — Unless otherwise specified, racks shall be packaged in accordance with accepted commercial practice.

5.2 **Packing.** — Unless otherwise specified, commercial packing will be acceptable. The subject commodity shall be prepared for shipment to permit acceptance by carrier for transportation at the lowest applicable rate, and to afford maximum protection from normal hazards of transportation.

5.3 **Marking.**

5.3.1 *Packages.* — Unless otherwise specified, packages shall be marked with the name of the commodity, the quantity contained therein, and the names of the manufacturer and contractor.

5.3.2 *Shipping containers.*—Unless otherwise specified, shipping containers shall be marked with the name of the commodity as defined by the contract or order under which the shipment is made, the quantity contained therein, the name and address of the consignee, and the gross weight.

6. NOTES

6.1 **Ordering data.** — Purchasers should specify the style required and exercise any desired options offered herein. (See 1.2, 4.1.3, 5.1, 5.2, 5.3.1, 5.3.2, 6.3, 7.2.4.1, and 7.2.4.2.)

6.2 This specification covers the following item appearing in the Armed Services Catalog of Medical Matériel:

6–124–700—Rack, Hanger, X-Ray Film.

6.3 **Bid samples.**—It is believed that this specification adequately describes the characteristics necessary to secure the desired material, and that normally no samples will be necessary prior to award. If, for any particular purpose, samples with bids are necessary, they should be specifically requested in the invitation for bids, and the particular purpose to be served by the bid sample should be definitely stated, the specification to apply in all other respects.

6.4 Federal specifications do not include all types, classes, grades, sizes, etc., of the commodities indicated by the title of the specification, or which are commercially available, but are intended to cover the types, etc., which are suitable for Federal Government requirements.

6.5 **Transportation description.** — Transportation description applicable to these items is:

Sheet steel ware, not otherwise indexed by name.

(State whether nested or not nested.)

6.6 Table I in section 4 was taken from Military Standard MIL–STD–105. Acceptable Quality Level (normal inspection) approximately equals 1.5 percent defective.

Patent notice.—When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

any patented invention that may in any way be related thereto.

7. DEPARTMENTAL REQUIREMENTS

7.1 The following specifications and standard, of the issues in effect on date of invitation for bids, and special requirements, form a part of this specification for purchases made under this specification by the respective departments.

7.2 Army, Navy, and Air Force.

7.2.1 *Applicable Specifications and standard.*

Federal Specifications:

NN-B-601—Boxes, Wood-Cleated-Plywood, for Domestic Shipment.
NN-B-621—Boxes, Wood, Nailed and Lock-Corner.
NN-B-631—Boxes, Wood, Wirebound (for Domestic Shipment).
LLL-B-631—Boxes; Fiber, Corrugated (for Domestic Shipment).
LLL-B-636—Boxes; Fiber, Solid (for Domestic Shipment).

Military Specifications:

JAN-P-105—Packaging and Packing for Overseas Shipment—Boxes, Wood, Cleated, Plywood.
JAN-P-106—Packaging and Packing for Overseas Shipment—Boxes, Wood, Nailed.
MIL-B-107—Boxes, Wood, Wirebound (Overseas Type).
MIL-L-10547—Liners, Case, Waterproof.

Navy Department Specification:

General Specifications for Inspection of Material.[1]

Military Standard:

MIL-STD-129—Marking of Shipments.

(Copies of specifications, standards, and drawings required by the contractor in connection with specific procurement functions should be obtained from the procuring agency or as directed by the contracting officer.)

[1] Applicable only to Navy purchases.

7.2.2 *Inspection procedures (Navy only).* —The general inspection procedures shall be in accordance with General Specifications for Inspection of Material.

7.2.3 *Packaging for domestic or overseas shipment.* — One rack constitutes one unit. Each unit shall be packaged in a solid fiberboard or double-faced corrugated fiberboard carton of appropriate size and design, constructed in accordance with the requirements of Federal Specification LLL-B-631 or LLL-B-636. Each carton shall be adequately secured to prevent accidental opening.

7.2.4 *Packing.*

7.2.4.1 *For domestic shipment.*—Twenty-four unit cartons (24 units) shall be overpacked in an exterior container constructed in accordance with the requirements of Federal Specification NN-B-601, or in an exterior container designed for type 2 load, and constructed in accordance with the requirements of Federal Specification NN-B-621 or NN-B-631. Boxes shall be strapped when required by appendix of applicable specification.

7.2.4.2 *For overseas shipment.*—Twenty-four unit cartons (24 units) shall be overpacked in an exterior container designed for type 2 load, and constructed in accordance with the requirements of Military Specification JAN-P-105, JAN-P-106, or MIL-B-107. Closure and strapping shall comply with appendix of applicable specification.

7.2.4.2.1 *Case liner.* — Each box shall be lined with a waterproof case liner conforming to the requirements of Military Specification MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto.

7.2.4.3 *Packing variation permitted.* — If the number of units in any shipment is not

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

the exact multiple of the number of units specified to be contained in each shipping container, the units not constituting the nearest such multiple shall be packed in an exterior container of suitable size and design and so constructed as to insure safe delivery to specified destination.

7.2.5 **Marking.**—Each unit carton and each shipping container shall be marked in accordance with the requirements of Military Standard MIL-STD-129.

NAVY INTEREST: Md Sh S

ARMY INTEREST: M

This specification is a part of Section IV, Part 5, of the Federal Standard Stock Catalog.

Copies of this specification can be purchased for 5 cents each from the General Services Administration, Business Service Center, Region 3, Seventh and D Streets, S. W., Washington 25, D. C. Single copies required for bidding purposes are available without charge at the nearest GSA Regional Office.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.