DDD-C-570C
February 28, 1980
SUPERSEDING
Int. Fed. Spec. DDD-C-00570B(VAMI)
June 30, 1961 and
Fed. Spec. DDD-C-570A
April 2, 1958

FEDERAL SPECIFICATION

COMPRESS, GAUZE; AND, COMPRESS AND SKULLCAP, HEAD DRESSING, CAMOUFLAGED

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers sterile gauze compresses used for surgical dressings, and sterile, adjustable head dressing of the skull cap type.

1.2 Classification. The gauze compresses shall be of the following types and sizes as specified (see 6.2):

Type I - Compress, gauze

Size 1 - 2 X 2 inches
Size 2 - 4 X 4 inches

Type II - Compress and skullcap

2. APPLICABLE DOCUMENTS

2.1 The following documents, of the issue in effect on date of invitation for bid or request for proposal, form a part of this specification to the extent specified herein.

Federal Specifications:

V-T-276	- Thread, Cotton.
FF-P-416	- Pin, Safety.
CCC-C-446	- Cloth, Muslin, Cotton.
DDD-T-86	- Tape, Textile, Cotton, General Purpose, Unbleached, Bleached or Dyed.
PPP-B-636	- Boxes, Fiberboard, Shipping.

FSC 6510

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.

Federal Standards:

Fed. Test Method Std. No. 191 - Textile Test Methods.
Fed. Std. No. 595 - Colors.

(Activities outside the Federal Government may obtain copies of Federal specifications, standards and commercial item descriptions, as outlined under General Information in the Index of Federal Specification, Standards, and Commercial Item Descriptions. The Index, which includes cumulative bimonthl supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, DC 20402.

(Single copies of this specification, other Federal specifications and commercial item descriptions required by activities outside the Federal Government for bidding purposes are available without charge from General Services Administration Business Service Centers in Boston; New York; Philadelphia; Washington, DC; Atlanta; Chicago; Kansas City, MO; Fort Worth; Houston; Denver; Los Angeles; San Francisco; and Seattle, WA.

(Federal Government activities may obtain copies of Federal specifications, standards, commercial item description and the Index of Federal Specification, Standards and Commercial Item Description from established distribution points in their agencies.)

Military Specifications:

MIL-S-36586 - Sterilization Test Strip Set, Bacterial spore.

Military Standards:

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of military specifications and standards required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

Laws and Regulations:

U.S. Department of Health, Education, and Welfare, Food and Drug Administration

21 CFR 1 - Regulations for the Enforcement of the Federal Food, Drug, and Cosmetic Act.

(Application for copies should be addressed to the Food and Drug Administration, 5600 Fisher Lane, Rockville, MD 20857.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bid or request for proposal shall apply.

U.S. Pharmacopeial Convention, Inc.:

The Unite States Pharmacopeia (USP).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.

(Application for copies should be addressed to the Mack Publishing Company, Easton, PA 18042.)

National Motor Freight Traffic Association, Inc., Agent:

National Motor Freight Classification

(Application for copies should be addressed to the American Trucking Association, Inc., Traffic Department, 1616 P Street, NW, Washington, DC 20036.)

Uniform Classification Committee, Agent:

Uniform Freight Classification

(Application for copies should be addressed to the Uniform Classification Committee, Room 1106, 222 South Riverside Plaza, Chicago, IL 60606.)

3. REQUIREMENTS

3.1. Material.

3.1.1 Muslin. Muslin cloth shall conform to type VI, class 2, bleached in accordance with CCC-C-446.

3.1.2 Gauze. Gauze shall be absorbent gauze in accordance with the USP for the types specified hereinafter, except that sterility shall not apply.

3.1.3 Cotton. Cotton shall be purified cotton in accordance with the USP, except that sterility and fiber length shall not apply.

3.1.4 Thread. Thread shall conform to type IA2, 3-ply, ticket no. 60, in accordance with V-T-276.

3.1.5 Tape. Tape shall be 1/2 inch wide in accordance with DDD-T-86.

3.1.6 Safety pin. Safety pins shall be in accordance with FF-P-146 for size 2 (medium).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.

3.2 Design and construction.

3.2.1 Type I, size 1. The compress and bandage shall consist of a sterile compress pad in white, and a sterile gauze bandage in camouflaged color, suitable for use as a first-aid field dressing.

3.2.1.1 Bandage. The bandage shall be fabricated of type I, USP absorbent gauze. The bandage shall have a width of 2-1/4 ± 1/4 inches and a length of 49 ± 1 inches. The cut edges shall be crushed, rolled or so processed as to preclude fraying or raveling.

3.2.1.2 Compress. The compress pad shall be 2 by 2 inches, with a tolerance of +1/4 inch, -0 inch in each direction. The pad shall consist of 16 plies of gauze meeting the requirements for USP type III absorbent gauze, or a combination of 4 plies of USP type VII absorbent gauze lined with a minimum of 4 grains (avoirdupois) USP purified cotton. The compress pad shall be affixed within 1-1/2 inch of the lengthwise center of the bandage, by sewing, and so constructed that it can be opened to form a pad 4 inches long by 2 inches wide. The sewing shall consist of two rows of stitching. One row at the approximate lengthwise center of the pad and one row within 1/4 inch of one of the narrow sides. The compress pad shall be so constructed that no raw edges are exposed.

3.2.2 Type I, size 2. The compress and bandage shall consist of a sterile compress pad in white, and a sterile gauze bandage in camouflaged color, suitable for use as a first-aid field dressing.

3.2.2.1 Bandage. The bandage shall be fabricated of type I, USP absorbent gauze. The bandage shall have a width of 4-1/4 ± 1/4 inches and a length of 85 ± 1 inches. The cut edges shall be crushed, rolled, or so processed as to preclude fraying or raveling.

3.2.2.2 Compress. The compress pad shall be 4 by 4 inches, with a tolerance of + 1/4 inch, -0 inch in each direction. The pad shall consist of 16 plies of gauze meeting the requirements for USP type III absorbent gauze, or a combination of 4 plies of USP type VII absorbent gauze lined with a minimum of 20 grains (avoirdupois) USP purified cotton. The compress pad shall be affixed within 1-1/2 inches of the lengthwise center of the bandage, by sewing, and so constructed that it can be opened to form a pad 8 inches long by 4 inches wide. The sewing shall consist of 2 rows of stitching. One row at the approximate lengthwise center of the pad and one row within 1/4 inch of one of the narrow sides. The compress pad shall be so constructed that no raw edges are exposed. An overlap of approximately 1/2 inch by 16 thicknesses of gauze is permitted on the back side of the compress, next to the bandage.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.

3.2.3 Type II. The compress and bandage, and skullcap shall consist of a sterile compress pad in white, a sterile bandage in camouflaged color, a sterile skullcap with the strip for securing to patient's head, in camouflaged color, and a safety pin in accordance with FF-P-416, size 2.

3.2.3.1 Bandage. The bandage shall be fabricated of type I, USP absorbent gauze. The bandage shall have a width of 2-3/4 + 1/4 inches and a length of 37 + 1 inches. The cut edges shall be crushed, rolled, or so processed as to preclude fraying or raveling.

3.2.3.2 Compress. The compress pad shall be 2-1/2 by 4 inches, with a tolerance of + 1/4 inch, -0 inch in each direction. The pad shall consist of 16 plies of gauze meeting the requirements for USP type III absorbent gauze. The compress pad shall be affixed within 1-1/2 inches of the lengthwise center of the bandage by sewing. The sewing shall consist of one row of stitching within 1/4 inch of one of the narrow sides. The compress pad shall be so constructed that no raw edges are exposed. An overlap of approximately 1/2 inch by 16 thicknesses of gauze is permitted on the back side of the compress, next to the bandage.

3.2.3.3 Skullcap. The skullcap shall be fabricated of muslin in accordance with 3.1.1. The skullcap shall have an integral tie strip having a length of 25 + 1 inches. The crown portion of the cap shall be cut to form a conventional type crown adjustable to fit most adult heads. Any seams on the crown shall be suitably taped (3.1.5). All edges shall be hemmed. Construction shall be as shown in figure 1.

3.2.4 Stitching, stitches, and seams. The crown of the skullcap shall be fabricated by folding the tape (3.1.5) in half and placing the cut edges of the cap material within the fold, seam type BSa-1. The tape shall be attached using stitch type 301. The remaining cut edges of the skullcap shall be hemmed with stitching type EFb-1, and stitch type 301. The width of the hem shall be 1/4 + 1/16 inch. The stitching shall be 1/16 to 1/8 inch from the side of the tape and from the turned edge of the hem. As an alternate, in lieu of the tape, the crown cut edges may be butted and joined together with seam type FSa-1 and stitch type 606.

3.3 Folding and wrapping.

3.3.1 Type I, size 1 and 2. Each compress and bandage shall be folded with free ends of bandage folded, or rolled, in such a position that when the dressing is opened it can be applied directly to the wound without contamination by the applier. Each folded compress and bandage shall be wrapped and sealed in a suitable paper that will maintain sterility of the contents until manually opened.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.

3.3.2 Type II. The folded compress, and the safety pin shall be placed inside the skullcap and the unit then folded and compressed to a maximum size of 3-1/2 inches long by 2 inches wide by 5/8 inches thick. The compressed unit shall be wrapped and sealed in a suitable paper that will maintain sterility of the contents until manually opened.

3.4 Camouflaged color. The color of the dyed bandages and skullcap shall closely approximate color no. 30324 or color no. 30219 of Fed. Std. No. 595 (see 6.5) when tested as specified in 4.4.1.

3.5 Dye. The dye used in the dyeing of the bandages and skullcap shall contain no known toxic or skin irritating substances.

3.5.1 Colorfastness. The dyed fabric used for the manufacture of the bandage and skullcap shall have at least good colorfastness to laundering when tested as specified in 4.4.3.

3.6 Thread color. The thread used in the fabrication of the bandage and skullcap shall be dyed to the approximate colors specified in 3.4, shall be natural, or shall be bleached.

3.7 Instructions. The unit package of the type I gauze compresses shall be marked in ink with instructions for use as shown in figure 2 or figure 3.

3.8 Ink. The ink used in the printing of the paper identification slip shall exhibit no flowing or bleeding of the print on the surface of the individual bandage wrappers when tested as specified in 4.4.2.

3.9 Sterility. The compress bandages and compress bandage and skullcap shall be sterile when tested with a biological indicator as specified in 4.4.3.

3.9.1 Certificate of sterility. A certificate of sterility, stating that samples from each sterilizer lot have been tested and found to be sterile, shall be submitted to the procuring activity. The certificate of sterility shall include.

a. Item identification.
b. National stock number.
c. Contract or purchase order number.
d. Sterility lot or control number.
e. Date of sterilization.
f. Quantity of product in sterilizer lot.
g. Type of sterilization (gas, radiation, heat, steam, etc.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.

h. Form of biological indicator (i.e., inoculated paper spore strip or carrier or inoculated product.)
i. Test organism(s) and population density used.
j. Test medium, incubation temperature, incubation time, and dates of tests.
k. Number of test units.
l. Statement that samples comply with sterility tests.
m. Signature of head of a laboratory or a designated qualified alternate.

When the contract provides for acceptance at destination, the certificate of sterility shall be submitted by the contractor to the procuring activity and a copy forwarded with each shipment to the consignee. When the contract provides for acceptance to be made at source, certificate of sterility shall be furnished to the cognizant Government Quality Assurance Representative for submission to the procuring activity.

3.9.2 Sterility lot. A sterility lot is that single quantity of product subjected to the same manufacturing operation and simultaneously sterilized in the same sterilizer chamber. Each unit package shall be clearly marked with a sterility lot (control) number and date of sterilization as specified in 5.3.2. Each sterility lot shall be traceable to the pertinent manufacturing lot(s).

3.10 Workmanship. Workmanship shall be first class throughout. The compress bandages and skullcaps shall be free from loose ends, ravelings, or other defects which affect their appearance or which impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.

4.1.3 Certificates.

4.1.3.1 Of quality. Certificates of quality, supplied by the manufacturer of the materials may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government, and provided also that the test methods and the results obtained comply with those described in this specification. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.1.3.2 Of non-toxicity and non-irritability. Certificates of non-toxicity and non-irritability supplied by the manufacturer of the dyed bandages and skullcaps shall state that the product offered to the Government meets the requirements of the Food and Drug Administration for dyed bandages. The certificate shall include the name of the manufacturer, the contract number, the lot number and the NSN of the item(s) offered.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and table I. The unit of product for sampling purposes shall be one gauze compress, or one compress and skullcap.

TABLE I. Sampling for examination.

Type defect	Inspection level	AQL (percent defective)
Major defects	II	1.0
Minor defects	II	2.5
Dimensional	S-2	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and table II. Where feasible, the same sample unit shall be used for the determination of two or more characteristics. The unit of product for test purposes shall be one gauze compress or one compress and skull cap.

TABLE II. Sampling for tests

Unit of product	Characteristic	Requirement	Test procedure	Inspection level	AQL (percent defective)
Gauze compress or compress and skullcap	Color	3.4	4.4.1	S-1	2.5
	Sterility	3.9	4.4.4	S-3	1.0
Ink	Permanency	3.8	4.4.2	S-1	2.5
Bandage/Skullcap	Colorfastness	3.5.1	4.4.3	S-1	2.5

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.

4.3 Examination.

4.3.1 Gauze compress and compress and skullcap. The gauze compress and compress and skullcap shall be examined to determine compliance with all requirements contained in this specification. Examination shall be conducted as specified in table III. Examination however, shall not be restricted to the defects listed in table III.

TABLE III. Classification of defects

Categories	Defects
Major:	
101	Bandage not specified width.
102	Bandage not specified length.
103	Compress pad not specified size.
104	Compress pad not sewn to bandage as specified.
105	Compress pad has exposed raw edges.
106	Cut edges of bandage not crushed, rolled or treated to prevent raveling or fraying.
107	Bandage and compress not free of loose thread or lint.
108	Compress and bandage not folded as specified.
109	Skullcap not fabricated as specified.
110	Missing item from skullcap and compress ensemble.
111	Bandages and skullcap not dyed.
112	Compress pad dyed.
113	Instructions for use not as specified.
114	Compress pad not folded as specified.
Minor:	
201	Pleats of folded bandage not as specified.
202	Bandage not free of cuts and tears.
203	Thread ends up to 1/4 inch present.
204	Instructions for use not legible.
205	Labeling not legible.
206	Unit package not as specified.

4.3.2 Examination of preparation for delivery. An examination shall be made to determine compliance with the packaging, packing and marking requirements of section 5. Defects shall be scored as specified in table IV. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 with an AQL of 4 expressed in terms of percent defective.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.

TABLE IV. Examination of preparation for delivery

Examine	Defect
Contents	Not as specified.
Container	Not as specified.
Marking	Omitted; incorrect; illegible; improper size, location, sequence, or method of application.
Packaging and packing material	Component missing or damaged.
Workmanship	Bulging or distortion of containers.

4.3.2.1 Examination of closure, waterproofing and banding of container. When the container is required to comply with PPP-B-636, the examination for defects in closure, waterproofing or banding shall be in accordance with the appendix of the appropriate box specification.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Color. The dyed material shall be visually examined under artificial daylight having a color temperature of 7500° Kelvin (K).

4.4.2 Ink permanency. The packaged item, unit of issue, for type I gauze compresses, shall be autoclaved at 250°F for a period of 20 minutes. After autoclaving the package shall be permitted to cool to room temperature and examined.

4.4.3 Colorfastness. The compress gauze shall be subjected to 3 cycles of laundering in accordance with Method 5610 of Fed. Test Method Std. No. 191.

4.4.4 Sterility test. The gauze compresses and gauze compress and skullcap shall be tested for sterility in accordance with the method specified in the U.S.P. for purified cotton, gauze, surgical dressing, and related material using inoculated product, or paper spore strip (carrier). Product containing a biological indicator shall be marked or labeled so that it clearly differentiates from product intended for distribution. The incubation medium and minimum time in each case shall be soyben casein digest for 7 days for inoculated product, or paper spore strip (carrier). The incubation temperature shall be as indicated in 4.4.4.1. The minimum number of test units, regardless of lot size, shall be 10, except for inoculated carrier which shall be 20 for type I sterilization and 30 for type II sterilization including inoculated carrier and product test units. The inspection level shall be as indicated in table II.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.

4.4.4.1 Inoculated product. For each type of sterilization, the organism used shall be as listed below:

Type of Sterilization	Orgranism	Incubation Temperature
Steam	B. stearothermophilus	55° - 65°C
Dry Heat	B. stearothermophilus or	55° - 65°C
	B. subtilis var. niger (or globigii)	30° - 35°C
Gas	B. subtilis var. niger (or globigii)	30° - 35°C
Radiation	B. pumilus	30° - 35°C

The number of viable cells shall be sufficient to provide assurance that the product has been sterilized.

4.4.4.2 Inoculated carrier. Inoculated carriers (paper spore strips) if used, shall be in accordance with MIL-S-36586. Other paper carriers shall be inoculated to be of equivalent resistance. The method of incubation and number of test units shall be as indicated in 4.4.4 and 4.4.4.1. The method of sterilization will control the organism in the spore strip to be tested for as shown in 4.3.1. NOTE: When an inoculated carrier is chosen, product samples must also be tested as required by the U.S.P.

4.4.4.3 Alternate method. Suppliers conducting sterility tests or designating lots in a manner other than that indicated herein shall submit proof that the alternate method provides equal assurance concerning the sterility of the product. However, all sterility tests shall be conducted using biological indicators. Requests for approval of any alternate method of testing for sterility shall be made to the Contracting Officer, and approval obtained before employment of the alternate method on a government contract.

4.4.4.4 Product testing. Testing for sterility of the product after receipt by the government shall be without a biological indicator and in accordance with the U.S.P.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C, as specified (see 6.2).

5.1.1 Level A.

5.1.1.1 Unit packaging.

5.1.1.1.1 Type I, size 1 and 2. Bandages shall be wrapped as specified in 3.3.1. Four size 1 bandages or one size 2 bandage shall be packaged in a close fitting polyethylene bag having a minimum wall thickness of 0.0040 inch.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.

Excess air shall be evacuated from the bag and the closure effected by heat sealing. The overall dimension of the sealed bag shall not exceed 4 inches in length by 2-1/8 inches in width by 5/8 inches in depth.

5.1.1.1.2 Type II. Each type II head dressing wrapped as specified in 3.3.2 shall be packaged in a close fitting polyethylene bag having a minimum wall thickness of 0.0040 inch. Excess air shall be evacuated from the bag and the closure effected by heat sealing.

5.1.1.2 Intermediate package. Ten unit packages containing type I bandages of one size only or twelve unit packages containing type II head dressings shall be packaged in a close fitting fiberboard box. Closure shall be adequate to prevent accidental opening during shipment and handling.

5.1.2 Level C (commercial). Type I and type II compresses packaged as specified in 5.1.1.1.1 and 5.1.1.1.2 shall be further packaged in a manner that will afford adequate protection against deterioration and physical damage during shipment from the supply source to the first receiving activity.

5.2 Packing. Packing shall be level A, B or C, as specified (see 6.2).

5.2.1 Level A. Forty-eight intermediate packages containing compresses of one type and size only shall be packed in a shipping container designed for a type 2 load and conforming to PPP-B-636, class weather-resistant. Closure, banding and waterproofing shall be as specified in the appendix of the box specification.

5.2.2 Level B. Forty-eight intermediate packages containing compresses of one type and size only shall be packed in a shipping container designed for a type 2 load and conforming to PPP-B-636, class domestic. Closure shall be as specified in the appendix of the box specification.

5.2.3 Level C. Compresses of one type and size shall be packed in shipping containers in a manner that will afford adequate protection against damage during shipment from the supply source to the first receiving activity. These packs shall conform to the carrier's rules and regulations.

5.3 Marking.

5.3.1 Civil agencies. Marking shall be as specified in the contract or purchase order.

5.3.2 Military activities.

5.3.2.1 Wrapper. Each wrapper shall be marked with the legend or similar statement: "STERILITY GUARANTEED UNLESS WRAPPER IS DAMAGED OR OPENED".

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.

5.3.2.2 Unit package. Each unit package shall be marked in accordance with the requirements of the Federal Food, Drug and Cosmetic Act and as specified in MIL-STD-129. The sterility lot or control number, contract or purchase order number, name of contractor and the legend "STERILE" shall be shown. The method of sterilization (G-Gas, R-Radiation, S-Steam, C-Cold, D-Dry heat) shall be shown following the level of packaging and date of packaging. Example: "A 10/78-G". Final sterilization shall be on or after indicated packaging date. The instructions for use as specified in 3.7 applicable to type I compresses shall be printed on the back face of the unit package. All marking may be printed on the bag or on inserts placed within the bag in such a manner to permit ready identification.

5.3.2.3 Intermediate package. Each intermediate package shall be marked as specified in MIL-STD-129. The sterility lot or control number, contract or purchase order number, name of contractor and the method of sterilization as specified in 5.3.2.2 shall be shown.

5.3.2.4 Shipping container. Shipping containers shall be marked as specified in MIL-STD-129. The sterility lot or control number and method of sterilization as specified in 5.3.2.2 shall be shown.

6. NOTES

6.1 Intended use. The items covered by this specification are intended for use as first-aid field dressing.

6.2 Ordering data. Purchasers should select the preferred options permitted herein and include the following information in the procurement documents:

a. Type required (See 1.2).
b. Title, number and date of this specification.
c. National Stock Number (NSN).
d. Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.3 This specification covers the following items listed in the Federal Supply Catalog:

National Stock Number	Item Identification
6510-00-200-3075	COMPRESS AND BANDAGE, Camouflaged, 2 by 2 inches, 4s
6510-00-200-3080	COMPRESS AND BANDAGE, Camouflaged, 4 by 4 inches
6510-00-201-7680	COMPRESS AND SKULLCAP, Head Dressing

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.

6.4 For military procurements originating from the Defense Personnel Support Center, Philadelphia, PA, certificates of sterility are to be forwarded to the Directorate of Medical Material, Attn: DPSC-ATQ, Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, PA 19101. For procurements originating from other agencies, the certificates of sterility shall be forwarded as indicated by the contracting officer (see 3.7.1).

6.5 Color chips may be obtained from the General Services Administration, Specification Consumer Information Distribution Center, Navy Yard Annex, First and N Streets, SE, Room 301, Washington, DC 20407.

6.6 Supersession data. This specification includes the requirements of MIL-C-982B, dated 18 May 1961 for Compress and Skullcap, Head Dressing.

MILITARY CUSTODIANS:
Army - MD
Navy - MS
Air Force - 03

Review activity:
DOD-MB

Preparing activity
DLA - DM

Civil Agency Coordinating Activities:
HEW-FDA
GSA-FSS

Project No. 6510-0631

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.


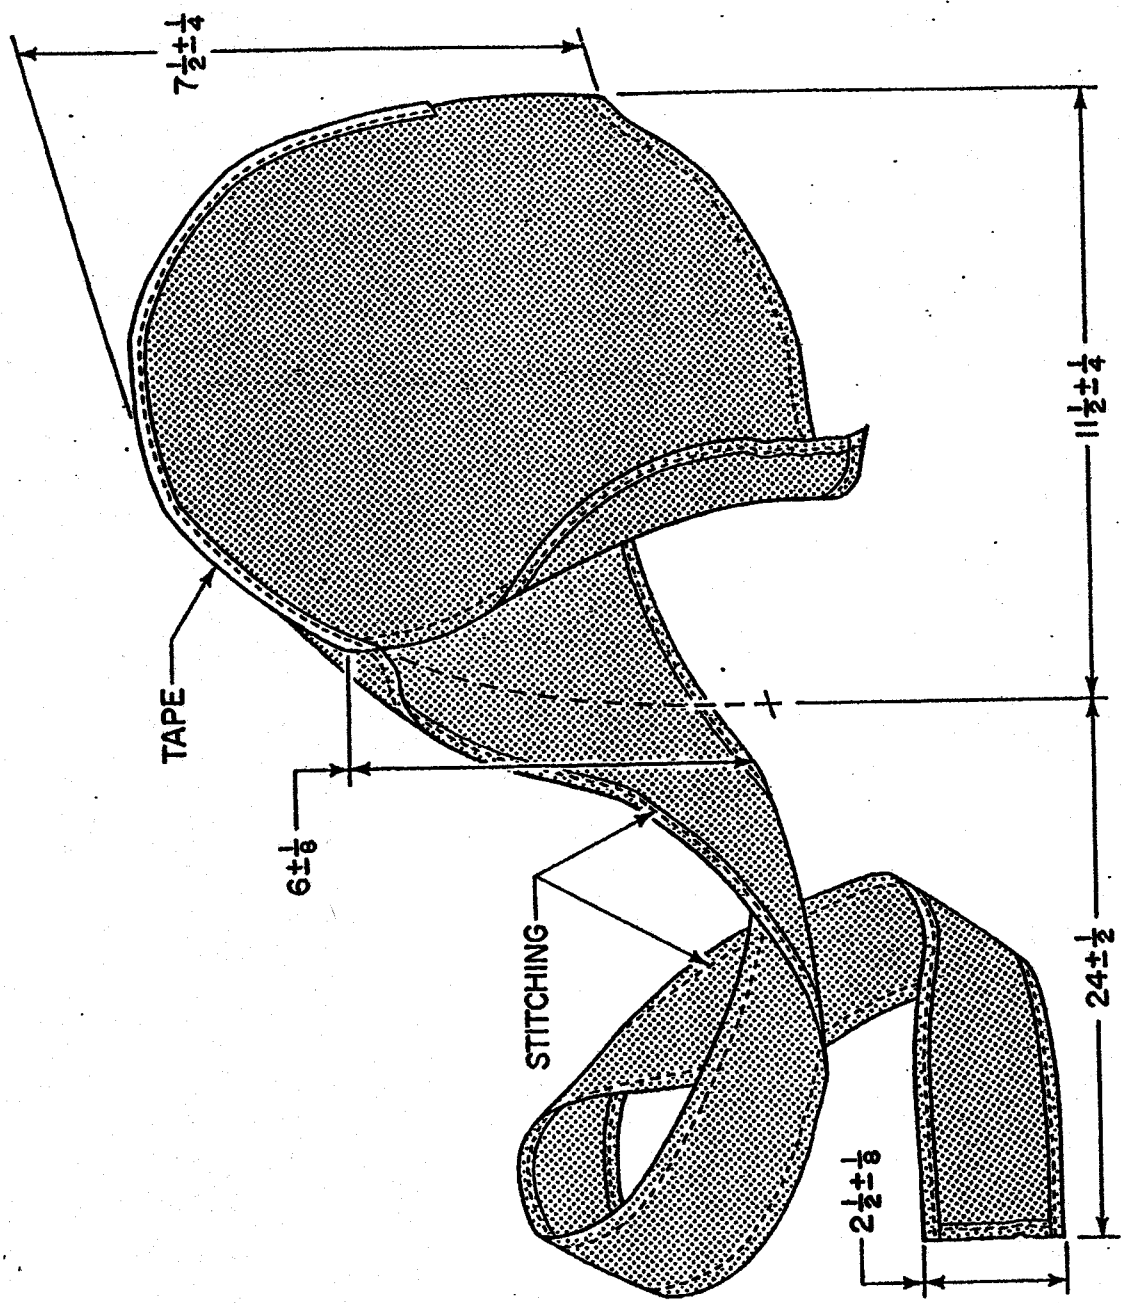


FIGURE 1. Skullcap head dressing.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.

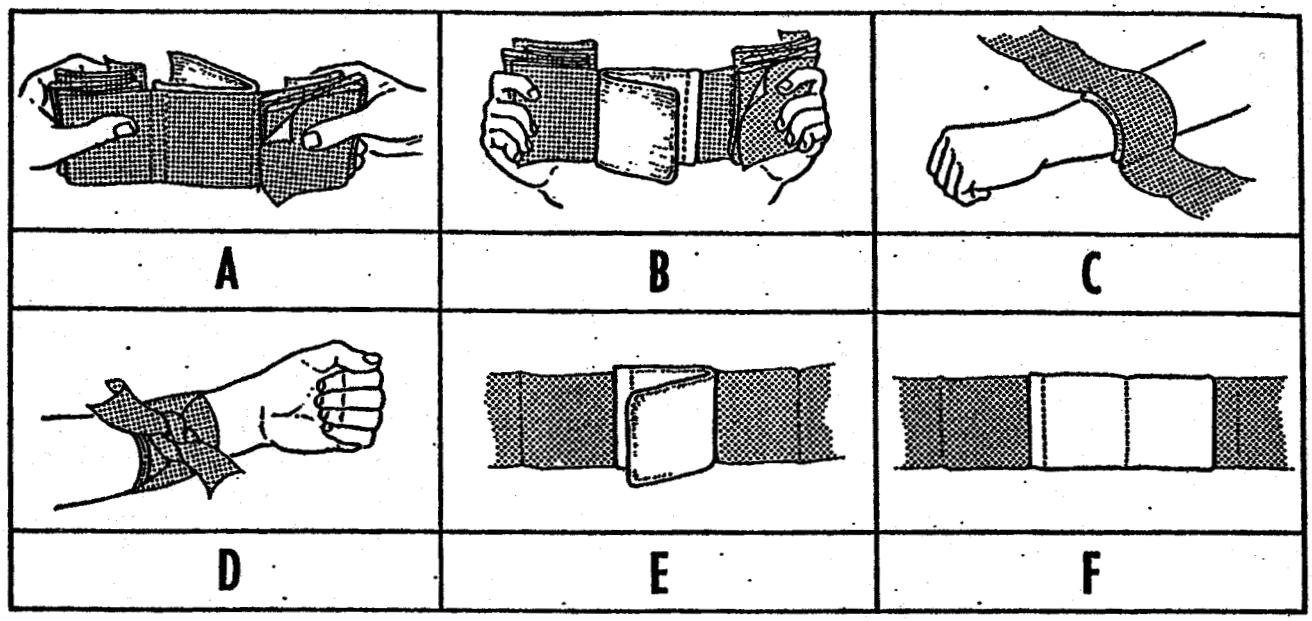

A Take hold of tails and pull out.

B Do not touch side of compress which goes on the wound.

C Place compress directly over wound. Wrap tails around arm or leg

D Make tails secure by tying square knot.

E If larger compress is necessary, open compress.

F Spread compress but do not touch surface which goes on wound.

FIGURE 2. Instructions for Use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.

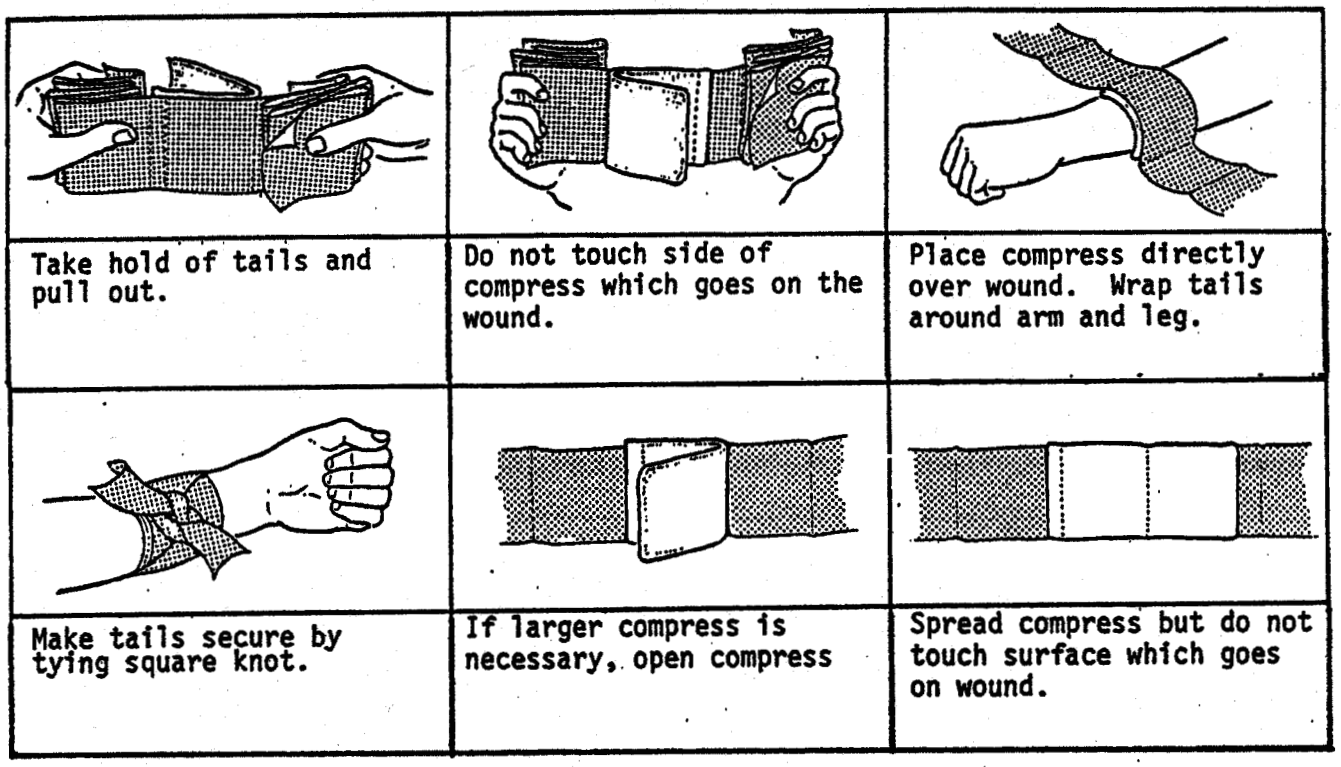


FIGURE 3. Instructions for use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.