DDD-D-626a
APRIL 28, 1959
SUPERSEDING
Fed. Spec. DDD-D-626
May 24, 1949

FEDERAL SPECIFICATION

DRAPE, SURGICAL

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 **Scope.**—This specification covers surgical drapes for use in general surgery.

1.2 **Classification.**

1.2.1 *Types and sizes.*—Surgical drapes shall be of the following types and sizes, as specified (see 6.1):

Type I.—With leggings.

Type II.—Plain.

Size 1.—24 inches by 24 inches.
Size 2.—34 inches by 66 inches.
Size 3.—72 inches by 94 inches.
Size 4.—94 inches by 108 inches.

2. APPLICABLE SPECIFICATIONS, STANDARDS, AND OTHER PUBLICATIONS

2.1 **Specifications and standards.**—The following specifications and standards, of the issues in effect on date of invitation for bids, form a part of this specification:

Federal Specifications:

V-T-276—Thread, Cotton.
TT-I-542 — Ink; Marking, Indelible, Black, for Fabrics.
CCC-C-430—Cloth, Cotton, Sheeting.
CCC-T-191—Textile Test Methods.
DDD-S-751 — Stitches; Seams; and Stitching.
PPP-B-636—Boxes, Fiber.
PPP-T-76 — Tape, Pressure-Sensitive Adhesive, Paper, Water Resistant.

Federal Standards:

Fed. Std. No. 102—Preservation, Packaging, and Packing Levels.
Fed. Std. No. 123—Marking for Domestic Shipment (Civilian Agencies).

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications, Standards, and Handbooks and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D. C.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.


(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications, Standards, and Handbooks from established distribution points in their agencies.)

Military Standards:

MIL-STD-105 — Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129—Marking for Shipment and Storage.


(Copies of Military Specifications and Standards required by contractors in connection with specific procurement functions should be obtained from the

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:35Z
Check the source to verify that this is the currentversion before use.

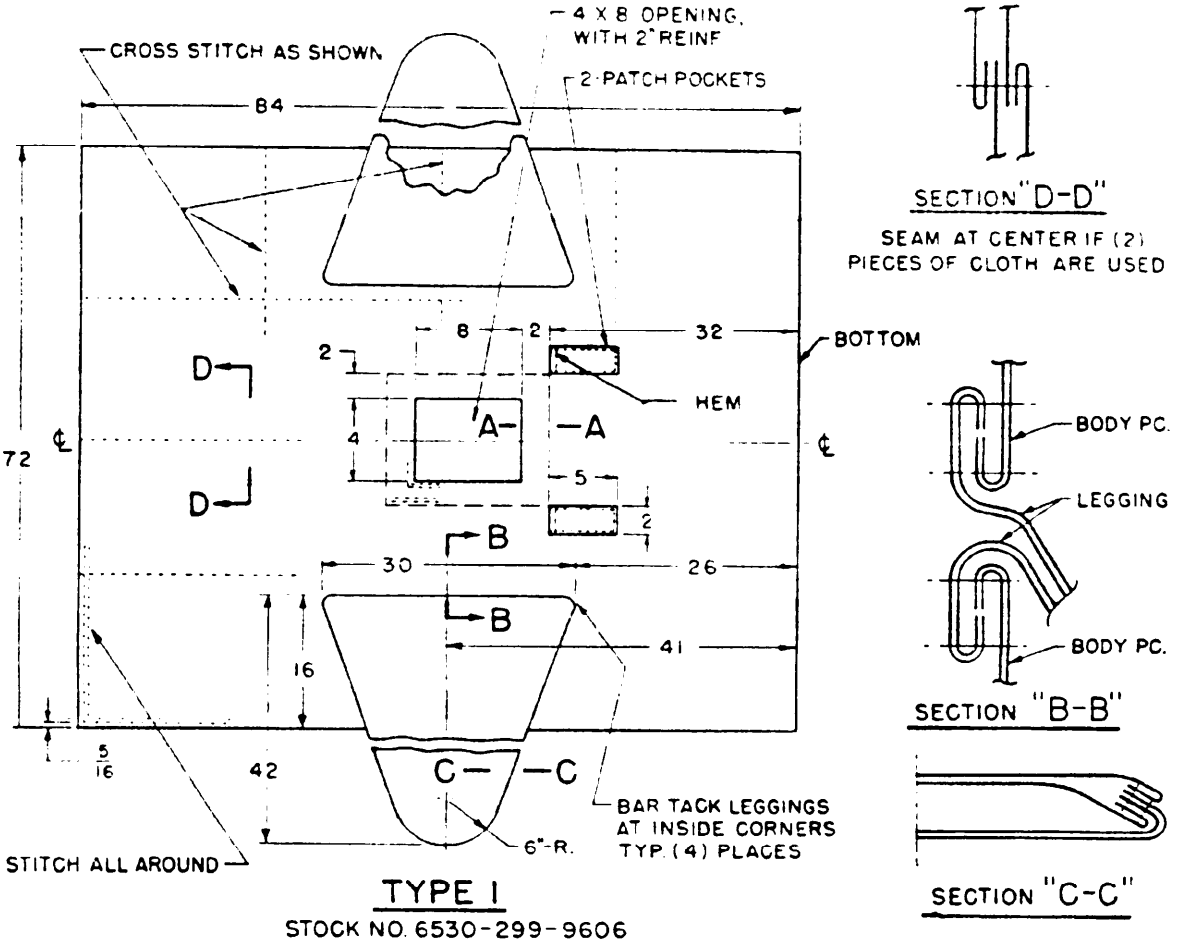

TYPE I

STOCK NO. 6530-299-9606

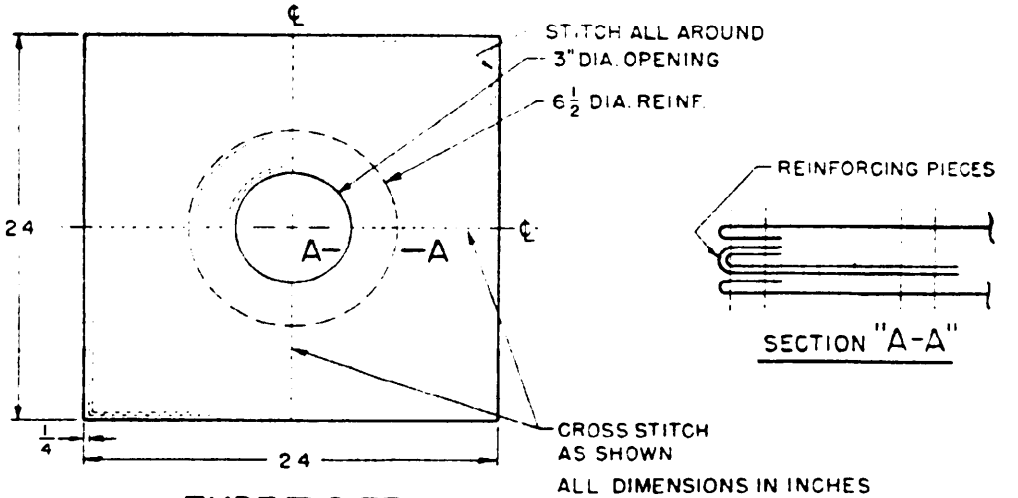

TYPE II, SIZE I

STOCK NO. 6530-299-9608

ALL DIMENSIONS IN INCHES


TOLERANCES:

15" AND UNDER • ± ¼"

OVER 15" • ± 1"

FIGURE 1.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:35Z
Check the source to verify that this is the currentversion before use.

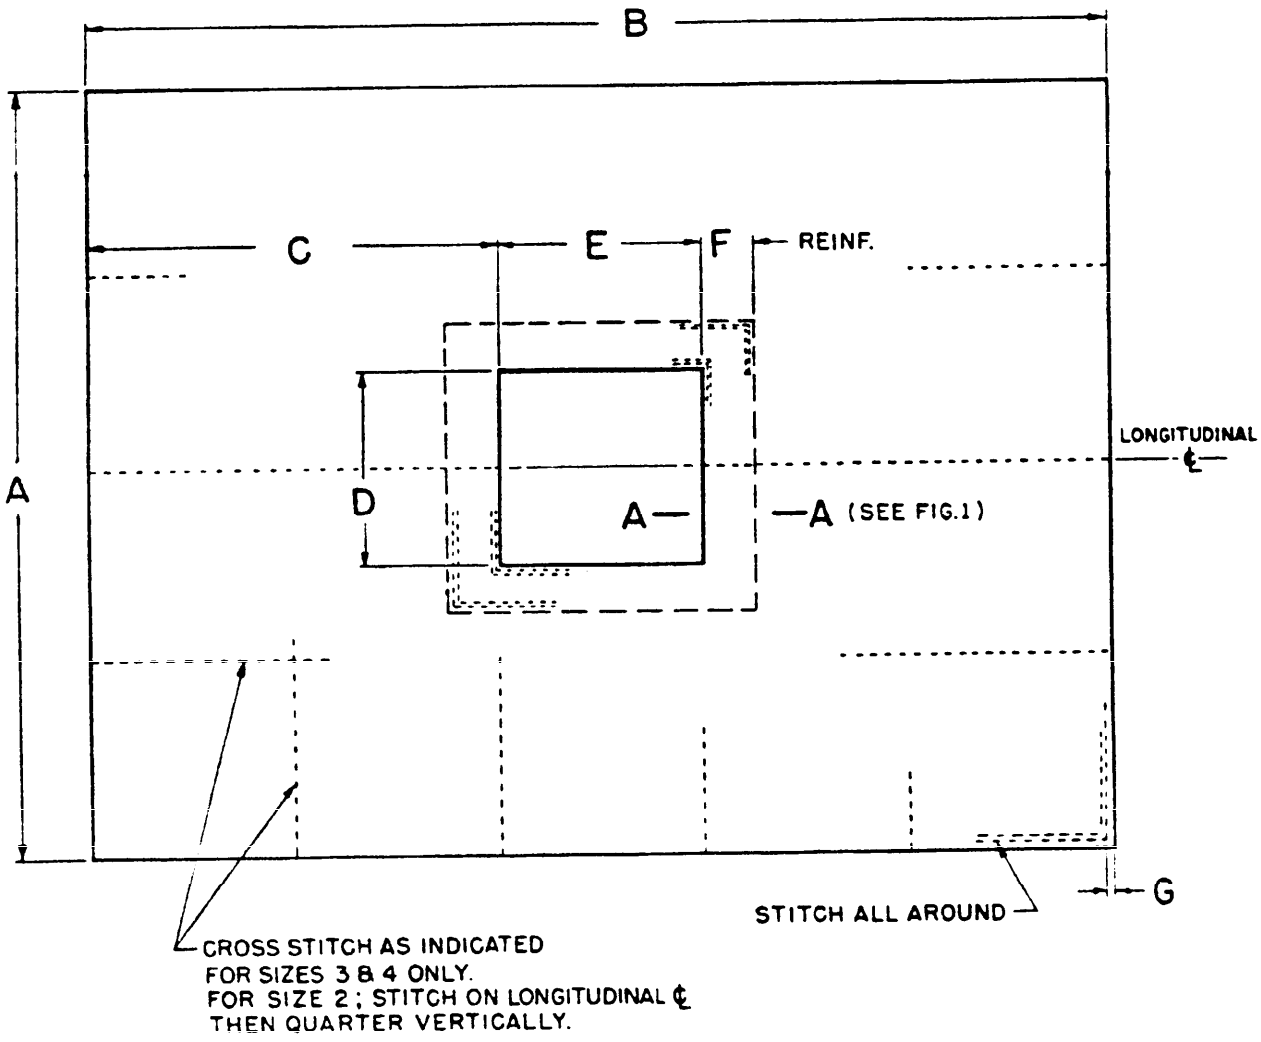

TYPE II

STOCK NO.	SIZE	DIMENSIONS						
		A	B	C	D	E	F	G
6530-299-9607	2	34	66	27	2	12	1 3/4	1/4
6530-299-9605	3	72	94	46	5	10	5	5/16
6530-299-9604	4	94	108	46	15	10	5	5/16

ALL DIMENSIONS IN INCHES

TOLERANCES:

15" AND UNDER = ± 1/4"

OVER 15" = ± 1"

FIGURE 2.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.

procuring activity or as directed by the contracting officer.)

2.2 **Other publications.**—The following publication forms a part of this specification. Unless otherwise indicated, the issue in effect on date of invitation for bids shall apply.

Munsell Color Company Color Book.

(Application for copies should be addressed to the Munsell Color Company, 10 East Franklin Street, Baltimore, Md.)

3. REQUIREMENTS

3.1 Material.

3.1.1 *Sheeting.*—The basic sheeting used in the fabrication of the drapes shall be type I, class 1, style A, as specified in table I of Federal Specification CCC-C-430.

3.1.1.1 *Color.*—Unless otherwise specified (see 6.1), the color of the sheeting employed in the fabrication of the drapes shall be vat dyed to a uniform grayish-green shade identified in the Munsell Color Company Color Book as follows:

Hue	8BG to 2B
Value	5.0 to 6.0
Chroma	1.5 to 2.5

The color shall be approximately identified as 10BG 5.6/2.0, although its hue, value, and chroma may fall within the range listed above. The color of the fabric shall show good fastness to light after 60 standard fading hours, to crocking, to chlorine bleaching, and to 15 launderings, when tested as specified in 4.4.

3.1.2 *Thread.*—The thread shall be cotton, machine thread, soft finish, unbleached, 3-ply, ticket No. 30, conforming to Federal Specification V-T-276 for type IA3. Color of the thread shall match the color of the sheeting (see 3.1.1.1). Where green thread is furnished, the color of the thread shall show good fastness to light and to 15 launderings, and fair fastness to chlorine bleaching, when tested as specified in 4.4.

3.1.3 *Ink.*—Ink for marking shall conform to Federal Specification TT-I-542.

3.2 **Construction.** — Drapes shall be as shown on figures 1 and 2 for the appropriate size and type. They shall be constructed to give a drape of double-thickness sheeting. This may be accomplished by folding one piece of sheeting on itself or by using two pieces of sheeting; or, if narrower width material is used, by using two pieces of sheeting, properly joined, as shown on section "D-D" of figure 1, for each thickness of the drape. Sheeting used to reinforce the opening in each drape shall be placed between the two thicknesses of the material forming the drape, and shall be joined in the seaming as shown on figure 1.

3.2.1 *Type I.*—In addition to the requirements specified in 3.2, the type I drape shall conform to the following: The opening for the leggings shall be cut straight, and the stitching of the leggings to the drape shall result in a straight, narrow, slotted opening with rounded ends. Inside corners of leggings shall be bartacked to the main body of the drape with 42 stitches per bartack. An opening 4 by 8 inches shall be provided with a 2-inch reinforcement, and shall be located in the center of the width and 34 inches from the bottom of the drape. Two patch pockets of single thickness shall be located as shown on figure 1. Top of pocket shall have a ½-inch hem, and ends shall be bartacked with 42 stitches per bartack.

3.3 **Dimensions.**—The surgical drapes shall conform to the dimensions shown on figures 1 and 2. Unless otherwise specified, a tolerance of plus or minus 1 inch in the dimensions of the drapes (length or width) and a tolerance of plus or minus ¼ inch for other dimensions will be permitted.

3.4 **Seams.**—For type II, sizes 1 and 2, seams shall be ¼ inch wide; for type II, sizes 3 and 4, and for type I the seams shall be 5/16 inch wide. All seam dimensions shall be minimum. The following types of seams, conforming to Federal Specification DDD-S-751, shall be used:

Seam type SSc-2 or SSp-1—for sides without selvages.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.

Seam type SSa-2 or SSp-1—for sides composed of two selvages.

Seam type SSb-2 or SSp-1—for sides composed of one selvage and one cut edge.

Seam type SSc-2—for joining reinforcing pieces to double thickness of sheeting at edge of openings in drapes (as shown in section A of figure 1).

Seam type SSa-2—for seams in forming leggings of drape.

Seam type EFb-1 — for top of patch pockets.

Seam type LSd-1—for sides and bottom of patch pockets.

Seam type LSr-2—for joining leggings of drape to drape proper (as shown in section B-B on figure 1).

Seam type OSf-2 — for folded edge of double sheeting, when only one piece of cloth is used.

3.5 Stitches.—All stitches shall be type 301 conforming to Federal Specification DDD-S-751 and shall consist of not less than 14 stitches per inch, except that seams for forming type I leggings may be a combination of a 301 and an overedge stitch of the 500 class, or a 401 and an overedge stitch of the 500 class.

3.6 Stitching.—Unless otherwise shown on figures 1 and 2, each row of seam stitches shall be approximately ⅛ inch from the edge of the cloth and shall be back-stitched for not less than ¼ inch at each end of the row. The folded edge of the double sheeting, when only one piece of cloth is used, shall have a double row of stitching approximately ⅛ inch from the edge. Each drape shall be double-stitched around the edges, the opening, and the reinforcement pieces of sheeting, and shall have rows of stitching as indicated by broken lines on figures 1 and 2.

3.7 Identification marking.—One outside corner of each surgical drape shall be marked with nontoxic indelible black ink, as specified in 3.1.3. The marking shall consist of the name or registered trade-mark of the manufacturer. The letters shall be block letters. Marking shall be clear, legible, and distinct. The color of the marking shall show good fastness to chlorine bleach and to 15 launderings, when tested as specified in 4.4.

3.8 Workmanship.—Workmanship shall be first class throughout. The surgical drapes shall be free from defects which detract from their appearance or which may impair their serviceability. The finished drapes shall be clean and free from loose ends and ravelings. The seams and stitching shall be made in such manner that a smooth drape, free from bulges, distortions, raw edges, or other imperfections shall result.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 General.—The provisions contained in this section are applicable to inspection performed by and for the Government. Sampling, inspection, and test procedures for components or materials described shall be in accordance with this specification and with specifications and standards referenced herein to the extent applicable, except that this specification shall govern in the event of conflict.

4.1.1 *Supplier responsibilities for inspection.*—The supplier shall perform examinations and tests set forth in this specification to substantiate conformance of supplies to specification requirements. The examinations and tests shall be at the expense of the supplier. Suppliers shall have adequate test facilities or shall arrange for test facilities acceptable to the Government to be used for executing specific prescribed tests. Records of examinations and tests performed by the supplier shall be maintained by the supplier and shall be made available to the Government, upon the Government's request, at any time or from time to time for a period of 2 years after the delivery of the supplies to which these records relate. The supplier shall be responsible for compliance with all requirements of this specification, and for all other technical requirements of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.

4.1.2 Inspection, as used in this specification, is defined as both examination (visual, auditory, etc. investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and the test results obtained and indicating that material is as specified, may be furnished.

4.2 **Sampling.** — Except when otherwise specified by civil agencies of the Government, sampling shall be conducted in accordance with Military Standard MIL–STD–105 and Appendix thereto.

	Inspection level	AQL (percent defective)
For visual examination:		
Major defects	II	1.0
Total defects	II	4.0
For dimensional examination	L6	1.0

For component testing. — Sufficient samples of the components shall be selected from each lot of material used in the manufacture of the drapes to perform tests as required by the applicable subsidiary specifications or by tests specified herein. When sample size for components covered by the subsidiary specifications is not specified, the sample size shall be as indicated for inspection level L2 in Appendix to Military Standard MIL–STD–105. No test result shall fall below the minimum or exceed the maximum values specified. The sample unit for testing shall be the quantity necessary to perform all required tests one time each. Not less than three samples shall be taken regardless of lot size. Lot sizes are expressed as follows:

Sheeting ---------- yards
Thread ---------- spools or cones
Identification marking --- each

4.2.1 Where possible, the same sample unit shall be used for the determination of two or more tests.

4.3 **Inspection.**—The drapes shall be inspected to determine compliance with all requirements contained in sections 3 and 5 of this specification. Nonconformance with these requirements will be permitted to the extent indicated in 4.2.

4.3.1 *Classification of defects.*—Inspection shall be conducted in accordance with the following classification of defects:

*Categories and defects**

Major:

101. Drape not type and size specified.
102. Drape not free of cuts, tears, or holes.
103. Breaks or damages in stitching not repaired.
104. Ends of each row not backstitched as specified.
105. Stitching type not as specified.
106. Drape not color specified, or color not uniform to a degree where appearance is seriously affected.

Minor:

201. Drape color departs significantly from specified standard but shade is uniform.
202. Thread color does not match color of drape.
203. Stitching not a minimum of 14 stitches per inch.
204. Seams not free of bulges, distortions, or puckering.
205. Drape not free of dirt or stains.
206. Markings omitted or not clear, distinct, or legible.
207. Location of identification marking not as specified.

* Inspection is not restricted to the classified defects listed above.

Note.—Numerals listed adjacent to description of defects are for use in recording of defects applicable only to the end item covered by this specification.

4.3.2 *Dimensional examination.* — The drapes shall be inspected for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.4 **Tests.**—The following test methods of Federal Specification CCC–T–191 shall be used:

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.

Component	Requirement paragraph	Characteristic	Test method
Sheeting	3.1.1	Weight	5040 or 5041
	3.1.1	Yarns per inch	5050
	3.1.1	Breaking strength	5100
	3.1.1.1	Colorfastness to laundering	5610
	3.1.1.1	Colorfastness to light	5660
	3.1.1.1	Colorfastness to chlorine bleaching	5600
	3.1.1.1	Colorfastness to crocking	5650
Thread	3.1.2	Colorfastness to light	4660
	3.1.2	Colorfastness to chlorine bleaching	4600
	3.1.2	Colorfastness to laundering	4610
Identification marking	3.7	Colorfastness to laundering	5610
	3.7	Colorfastness to chlorine bleaching	5600

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 *Unit of issue.*—One drape, as specified, constitutes one unit.

5.1.2 *Packaging quantities.*—The number of units of issue indicated in table I shall be packaged in each polyethylene bag, intermediate, and exterior container, as applicable for the required level of protection specified in the procurement document.

TABLE I.—*Packaging quantities*

Federal stock number	Number of units in polyethylene bag	Intermediate package	Shipping container
6530-299-9604	1	5	10
6530-299-9605	1	8	16
6530-299-9606	1	6	12
6530-299-9607	1	30	60
6530-299-9608	6	120	240

5.1.2.1 *Packing variation permitted.* — If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which will insure safe delivery to destination.

5.1.3 *Level A.*

5.1.3.1 *Polyethylene bag.*—The number of units indicated in table I shall be packaged in a bag fabricated from virgin polyethylene seamless tubing, having an average wall thickness of not less than 0.004 inch with no wall thickness at any point below 0.00325 inch. Excess air shall be expelled or evacuated, and closure effected by heat sealing.

5.1.3.2 *Intermediate package.*—Intermediate package shall be a weatherproof fiberboard box constructed in accordance with Federal Specification PPP-B-636, compliance symbol W5c or W5s, except that the manufacturer's joint shall be effected by the application of a water-resistant tape, or by gluing integral lap to outer face of end or side panel using water-resisting adhesive, in lieu of metal stitches. Box shall be sealed with tape conforming to Federal Specification PPP-T-76. The tape shall be not less than 2 inches wide and shall extend at least 3 inches onto each of the end panels.

5.1.4 *Level C.*—Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose within the continental limits of the United States of America.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.

5.2 **Packing.**

5.2.1 *Level A.*

5.2.1.1 *Exterior container.*—Exterior container shall be a box constructed in accordance with Federal Specification PPP–B–636, compliance symbol V3c or V3s. Closure shall comply with appendix thereto, except that strapping will not be required.

5.2.2 *Level C.* — The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order. Shipping containers shall comply with carrier rules and regulations applicable to the mode of transportation.

5.3 **Marking.**

5.3.1 *Civil agencies.*—In addition to any special marking specified in the contract or order, each unit, intermediate package, and shipping container shall be marked in accordance with Federal Standard No. 123.

5.3.2 *Military agencies.*

5.3.2.1 *Polyethylene bag.*—Each polyethylene bag shall be marked in accordance with section 5 of Military Standard MIL–STD–129. The required marking shall be printed directly on the bag or on a label inserted within the bag in such manner as to permit ready identification.

5.3.2.2 *Intermediate package.*—Each intermediate package shall be marked in accordance with section 5 of Military Standard MIL–STD–129.

5.3.2.3 *Shipping container.*—Shipping container shall be marked in accordance with Military Standard MIL–STD–129. Service color and service symbol markings are required only on direct shipments from the contractor's plant to overseas activities.

5.4 Federal Standard No. 102 shall be referred to for definitions and applications of the various levels of packaging protection for supplies and equipment.

6. NOTES

6.1 **Ordering data.**—Purchasers should exercise any desired options offered herein, and procurement documents should specify the following:

(*a*) Title, number, and date of this specification.
(*b*) Type and size required (see 1.2.1).
(*c*) Color, if other than green is required (see 3.1.1.1).
(*d*) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 This specification covers the following items appearing in the Armed Services Medical Stock List:

6530–299–9604 DRAPE, SURGICAL, Green, 94 by 108 inches.
6530–299–9605 DRAPE, SURGICAL, Green, 72 by 94 inches.
6530–299–9606 DRAPE, SURGICAL, Green, 72 by 84 inches, with Leggings.
6530–299–9607 DRAPE, SURGICAL, Green, 34 by 66 inches.
6530–299–9608 DRAPE, SURGICAL, Green, 24 by 24 inches.

6.3 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Federal Government requirements.

6.4 **Transportation description.**—The transportation description applicable to these items is:

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.

Dry goods not otherwise indexed by name.
Carload minimum weight, 20,000 pounds subject to Rule 34, Uniform Freight Classification.
Motor volume minimum weight—any quantity.

Notice. — When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

MILITARY INTERESTS:
Army—M
Navy—Md
Air Force.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:35Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:35Z
Check the source to verify that this is the current version before use.