INCH-POUND


MIL-DTL-3628/257
9 June 2011

DETAIL SPECIFICATION SHEET


BADGE, FIELD MEDICAL READINESS AND INSIGNIA, COLLAR, U.S. PUBLIC HEALTH SERVICE

This specification is approved for use by all Departments and Agencies of the Department of Defense.

The requirements for acquiring the product described herein shall consist of this specification sheet and the latest issue of MIL-DTL-3628.

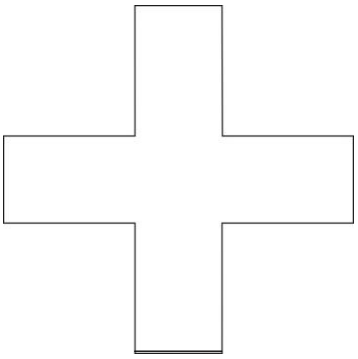

BADGE, BASE

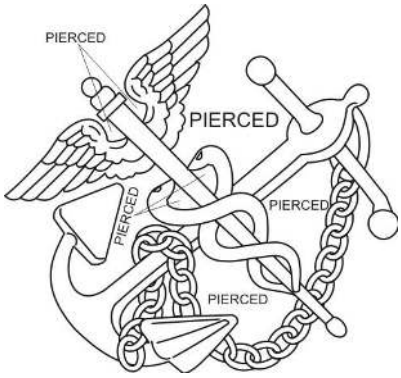

BADGE, DEVICE & COLLAR INSIGNIA



BADGE, ASSEMBLED

DASH NUMBERS:
-1 Badge, Base, Regular Size
-2 Badge, Base, Miniature Size
-3 Badge, Device, Regular Size
-4 Badge, Device, Miniature Size
-5 Badge, Assembled, Regular Size
-6 Badge, Assembled, Miniature Size
-7 Collar Insignia

MATERIAL: Red Brass 85/15 (UNS Alloy C-23000)

FINISH: 24K Gold Plated, Mirror-like Polished, and shall match The Institute of Heraldry (TIOH) Metal Finish Chip #6.

Source: https://assist.dla.mil -- Downloaded: 2026-10-16T20:24Z
Check the source to verify that this is the current version before use.

DIMENSIONS:

HEIGHT (overall) & WIDTH (overall):

-1, -5: 1 inch (REF)

-2, -6: 3/4 inch (REF)

-3, -7: 23/32 inch (REF)

-4: 19/32 inch (REF)

THICKNESS:

-1, -2 (at center): 0.053 inch ± 0.005 inch

-3, -7 (along staff of Caduceus): 0.053 inch ± 0.005 inch

-4 (along staff of Caduceus): 0.050 inch ± 0.005 inch

-5 (where wings meet staff of Caduceus): 0.106 inch ± 0.010 inch

-6 (along staff of Caduceus): 0.103 inch ± 0.010 inch

NOTES:

1. The term (REF) refers to the measurements taken from the Government furnished hub or die.

2. The hub and die used for the production of -3 shall also be used for the production of -7.

3. Piercings for -3, -4, and -7 shall be as indicated above.

4. The badge shall be constructed as follows. The base and device pieces shall be secured by two rivets in a location to correctly position the device to the base as indicated above. The rivets may be an integral part of the device or fabricated from any type brass or soldered to the reverse of the device. Rivets shall be securely peened or swaged to ensure a tight and close fit between the base and device.

5. Attaching device shall be prong and clutch type. For -1, two prongs shall be positioned on the vertical center line 1/16 inch ± 1/64 inch from the top and bottom of the base, and shall be 3/4 inch apart ± 1/32 inch. For -2, two prongs shall be positioned on the vertical center line 1/32 inch ± 0.008 inch from the top and bottom of the base, and shall be 5/8 inch apart ± 1/64 inch. For -7, two prongs shall be positioned on the diagonal center line from the upper wing of the Caduceus to the bottom fluke of the anchor 1/32 inch ± 0.008 inch from the ends, and shall be 1/24 inch apart ± 1/64 inch.

Source: https://assist.dla.mil -- Downloaded: 2026-10-16T20:24Z
Check the source to verify that this is the current version before use.

Custodian:
Army - IH

Preparing activity:
Army - IH

Review activity:
DLA - CT

Civil agency:
HHS - CCFM

(Project No. 8455-2011-026)

NOTE: The activities listed above were interested in this document as of the date of this document. Since organizations and responsibilities can change, you should verify the currency of the information above using the ASSIST Online database at https://assist.daps.dla.mil.

Source: https://assist.dla.mil -- Downloaded: 2026-10-16T20:24Z
Check the source to verify that this is the current version before use.