
FED. SUP CLASS
6640

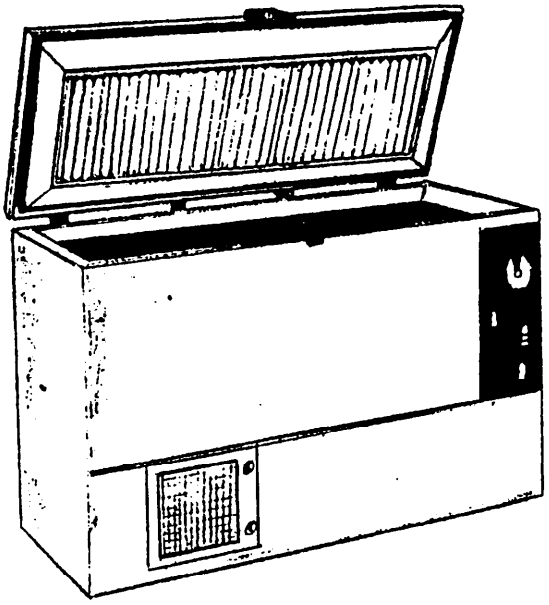

PART NUMBER	TEMPERATURE RANGE °C	CHAMBER SIZE m^3 (ft^3)	CABINET DIM. (cm) LENGTH	WIDTH	DEPTH	VOLTAGE PH/Hz
MS36381-1	+10 to -40	.23 (8.2)	133.0	7.11	109.5	115/1/60
MS36381-2	-60 to -85	.23 (8.2)	133.0	7.11	109.5	115/1/60
MS36381-3	-60 to -86	.23 (8.2)	133.0	7.11	109.5	230/1/60*
MS36381-4	-65 to -100	.23 (8.2)	133.0	7.11	109.5	230/1/60*
MS36381-5	-60 to -75	.35 (12.7)	182.9	7.11	111.1	115/1/60
MS36381-6	-60 to -85	.35 (12.7)	182.9	7.11	111.1	230/1/60*
MS36381-7	-60 to -85	.31 (11.3)	177.8	71.1	136.4	230/1/60*
MS36381-8	-60 to -95	.31 (11.3)	177.8	71.1	136.4	230/1/60*
MS36381-9	-60 to -85	.52 (18.7)	231.0	71.0	112.0	230/1/60*
MS36381-10	-60 to -95	.75 (26.5)	239.0	81.0	112.0	230/1/60*

* See Note 1.

MATERIAL: The inside chamber shall be made of 16 gauge zinc coated cold roller steel and the exterior shall be heavy gauge cold roller steel with baked enamel finish. Steel shall be in accordance with ASTM Specification A366. All other materials as required for reliable service.

DESIGN: The cabinet shall be the chest type with a hinged lid. The cabinet shall have a minimum of 127 mm of poured-in-place rigid urethane insulation around a steel chamber. The lid shall have a vacuum formed inner panel lined with polyurethane foam insulation and backed with the same high impact breaker strip as the chamber, where they form a seal. The entire breaker strip area shall be heated to prevent condensation and ice build up. The lid mechanism shall be counterbalanced and equipped with a key locking handle. The gaskets shall be the magnetic type. A liquid drain shall be located in the chamber bottom. The freezer shall be furnished with a temperature indicating control, a fail-safe relay and external alarm adapter plug with "overtemp" alarm signal light, a power light, 76 mm (3") diameter casters, chamber drain, inserts for rails, a 2.5 m (8 ft.) power cord on single phase models and a sliding plastic subcover at top of chamber to retain cold air when lid is open.

USER ACTIVITIES: ARMY - MD, DM
NAVY - MS

REVIEWER ACTIVITIES: ARMY - ME
NAVY - OS
AIR FORCE - 82

This military standard is approved for use by all Departments and Agencies of the Department of Defense. Selection for all new engineering and design applications and for repetitive use shall be made from this document.

APPROVED 30 JUN 1983 REVISED

P.A. EA	INTERNATIONAL INTEREST	TITLE	MILITARY STANDARD
Other Cust MS 99		CABINET, CONSTANT TEMPERATURE	MS36381
Procurement Specifications NONE	SUPERSEDES:		SHEET 1 OF 2

DD FORM 1 MAY 73 672 (COORDINATED) PREVIOUS EDITIONS OF THIS FORM ARE OBSOLETE

PROJECT NUMBER 6640-1181

Source: https://assist.dla.mil -- Downloaded: 2026-10-23T17:39Z
Check the source to verify that this is the current version before use.

FED. SUP CLASS
6640

All electrical components shall conform to the standards of Underwriters Laboratories, Incorporated.

NOTES:

1. All cabinets shall be available in voltage 230/1/50. Cabinets marked * shall also be available in voltages 208/1/60, 208/3/60, and 230/3/60. To specify the above voltages that are different from the table, add the voltage desired as a suffix number to the basic MS part number (example, MS36381-1 - 230/1/50).

2. Items differing from this Military Standard by minor variations in design or dimensions are considered standard under this document, provided such variations do not affect performance and are not in conflict with the material requirements specified herein.

REVIEWER ACTIVITIES:
USER ACTIVITIES:

This military standard is approved for use by all Departments and Agencies of the Department of Defense. Selection for all new engineering and design applications and for repetitive use shall be made from this document.

REVISED
APPROVED

P.A. / Other Cust	INTERNATIONAL INTEREST	TITLE: CABINET, CONSTANT TEMPERATURE	MILITARY STANDARD MS36381
Procurement Specifications	SUPERSEDES:		SHEET 2 OF 2

DD FORM 1 MAY 73 672 (COORDINATED) PREVIOUS EDITIONS OF THIS FORM ARE OBSOLETE PROJECT NUMBER 6640-1181

Source: https://assist.dla.mil -- Downloaded: 2026-10-23T17:39Z .
Check the source to verify that this is the current version before use.