A-A-50182
April 30 1992

SUPERSEDING
X-1628B
June 15, 1988

COMMERCIAL ITEM DESCRIPTION

URINAL, INCONTINENT (External Catheter)

The General Services Administration has authorized the use of this commercial item description in preference to VA Specification X-1628B, dated June 15, 1988.

Salient characteristics. URINAL, INCONTINENT (External Catheter), shall be a urinary drainage sheath tube system. All dimensions shall conform to the respective drawing.

The external catheters shall be of the following types and conform to their respective drawing:

Type I	Figure #1	with foam-lined plastic disc and ring
Type II	Figure #2	without plastic disc and ring
Type III	Figure #3	one-piece latex catheter and integral tube section

Tubing. Tubing for Type I and II shall be polyvinylchloride (PVC). Tubing for Type III shall be an integrally formed latex. The tubing shall be nontoxic substance compatible with human tissue.

Plastic Fitment. The fitment for Type I and II shall be nontoxic, nonporous and compatible with human tissue. The plastic fitment is not applicable to Type III.

Prophylactic sheath. Sheath shall be free of tears or pinholes and shipped tightly rolled.

Self-adhesive strip. A 1 inch x 6 inches (2.54 cm x 15 cm) medical grade, nonporous, one-sided, self-adhesive strip shall be supplied with each catheter for Type III only. (width tolerance, plus or minus 1/8 inch (3 mm) and length tolerance, plus or minus 1/4 inch (6 mm).

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:37Z
Check the source to verify that this is the current version before use.

Bidder certification. Upon request, the bidder shall certify that the plastic fitment, tubing and latex are nontoxic, nonporous and compatible with human tissue.

Pinhole and assembly test. The prophylactic sheath is filled with 16 ounces (473 ml) of water after a tube clamp has been used to close the distal end of the tube. The entire assembly is suspended for 4 hours. No sign of leakage or disassembly shall be observed.

Workmanship. The urinal, incontinent (external catheter) shall be free from defects which detract from its appearance or impair its serviceability.

Unit. The Unit for Type I, II and III shall be BAG (50). The unit for Type III, NSN 6530-01-081-5304 is EACH, 144 catheters (bulk).

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract of purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the government. The government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with this commercial item description requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:37Z
Check the source to verify that this is the current version before use.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, with an AQL of 1.0 (percent defective) and an inspection level of S-4. The unit of product for examination purposes shall be one male patient urinal, incontinent as specified in this description.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description, and conforms to the producer's own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:37Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE. The following National Stock Numbers are covered by this document:

NSN	TYPE	NOMENCLATURE
6530-00-290-8292	Type I	URINAL, INCONTINENT (External Catheter), 50s
6530-01-004-8969	Type II	URINAL, INCONTINENT (External Catheter), 50s
6530-01-081-5303	Type III	URINAL, INCONTINENT (External Catheter), 50s
6530-01-081-5304	Type III	URINAL, INCONTINENT (External Catheter), 144 (bulk)

Copies of Federal Standard No. 376, Preferred Metric Units for General Use by the Federal Government and MIL-STD-105, Sampling Procedures and Tables for Inspection by Attributes may be obtained from the Superintendent of Documents, U.S. Government Printing Office, Washington, DC 20420.

Ordering data. Purchasers should select the preferred options permitted herein, and include the following information in procurement documents:

(a) Title, number, and date of this commercial item description

(b) Type

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:37Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Military Coordinating Activity:

DoD-MB

AGENT:

DLA-DM

Custodians:

Army-MD
Navy-MS
Air Force-03

CIVIL AGENCY COORDINATING ACTIVITIES:

FDA-MPQAS
PHS


PREPARING ACTIVITY:

VA-OSS VAMKC (904)
Agent VA-OSS VACO (92A)


Project No. 6530-2348

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:37Z
Check the source to verify that this is the current version before use.

TYPE I

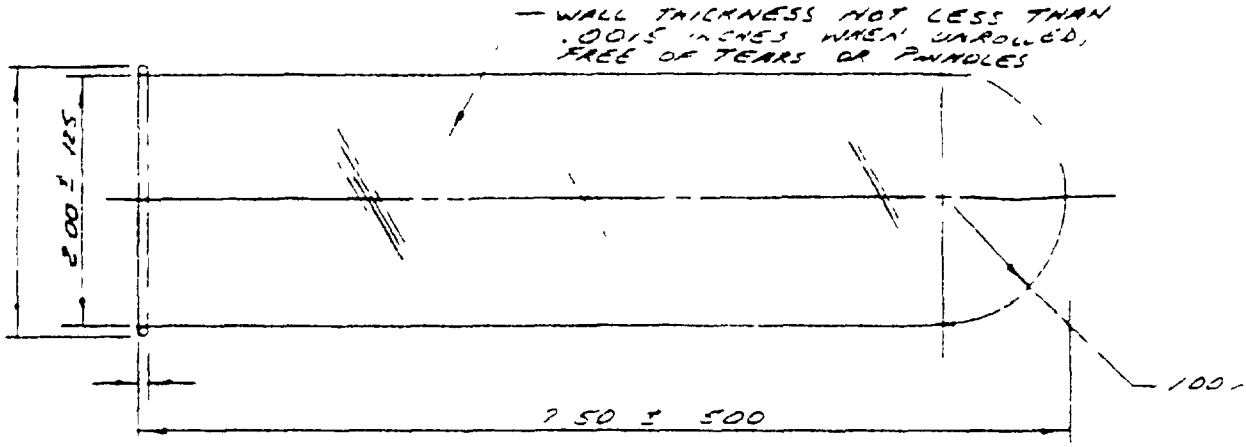


1 PROPHYLACTIC SHEATH
SCALE FULL

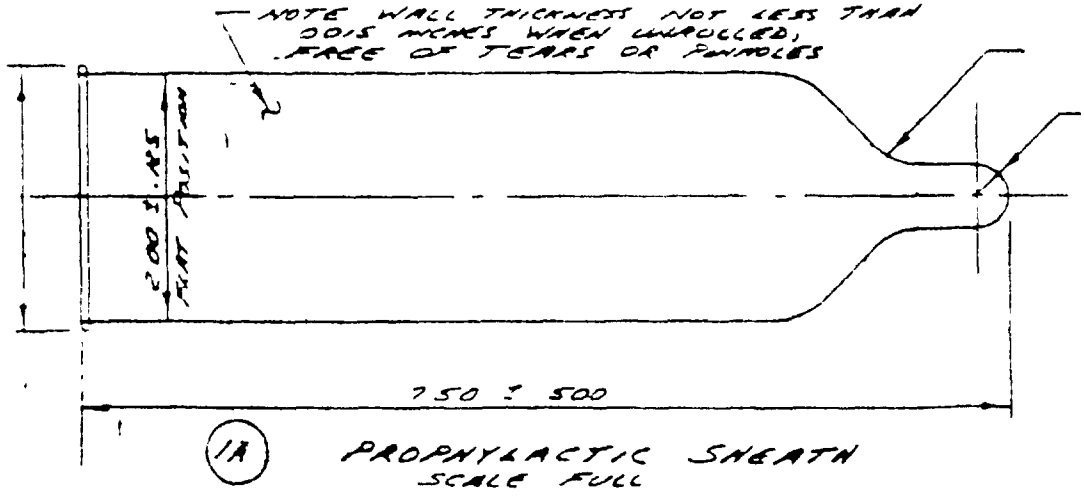


1A PROPHYLACTIC SHEATH
SCALE FULL

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:37Z
Check the source to verify that this is the current version before use.

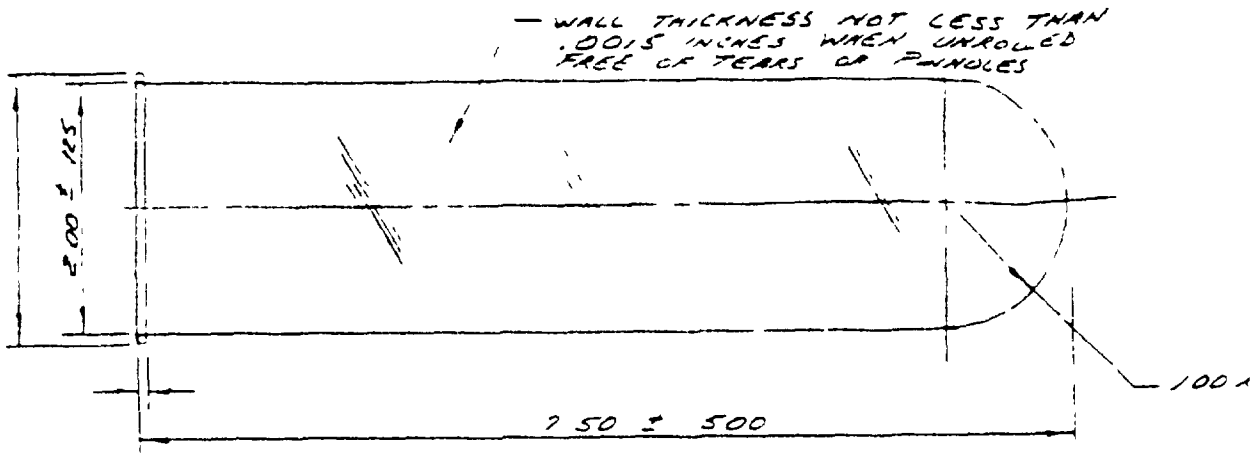


1 PROPHYLACTIC SHEATH
SCALE FULL

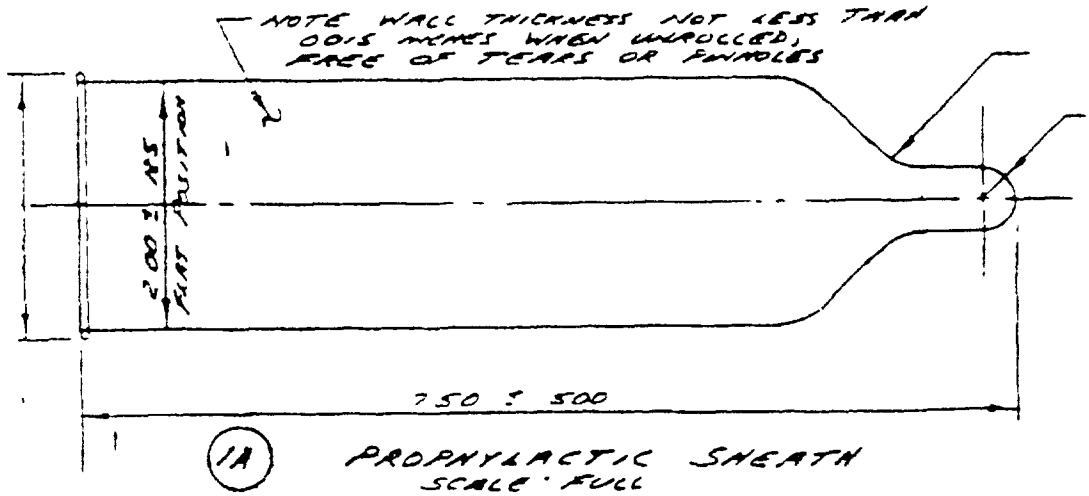

1A PROPHYLACTIC SHEATH
SCALE · FULL

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:37Z
Check the source to verify that this is the current version before use.


TYPE I

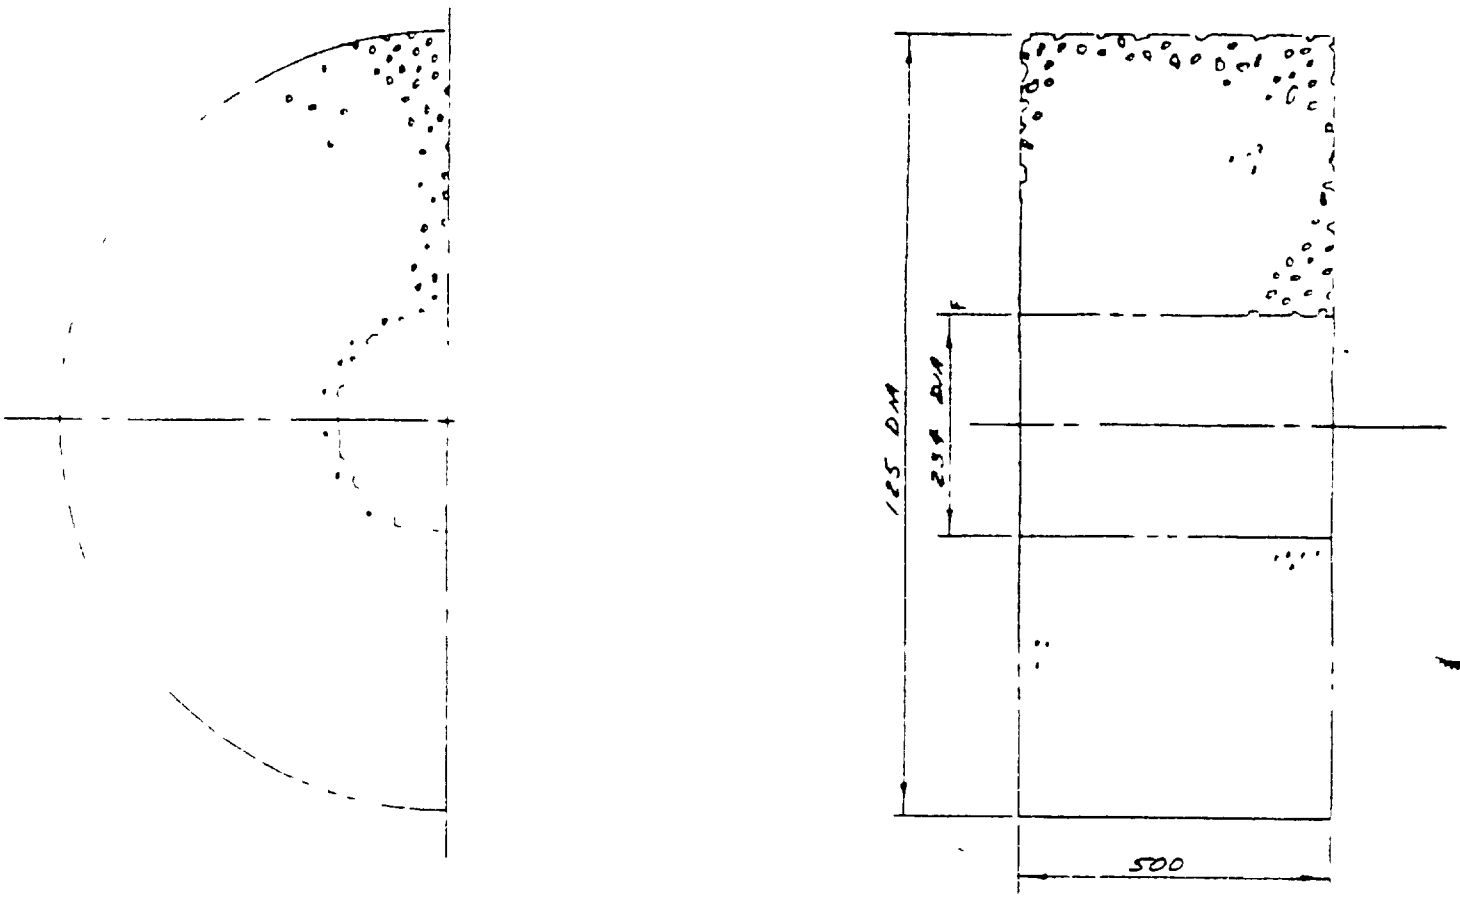

(2) FOAM DISC

SCALE 5x SIZE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:37Z
Check the source to verify that this is the current version before use.

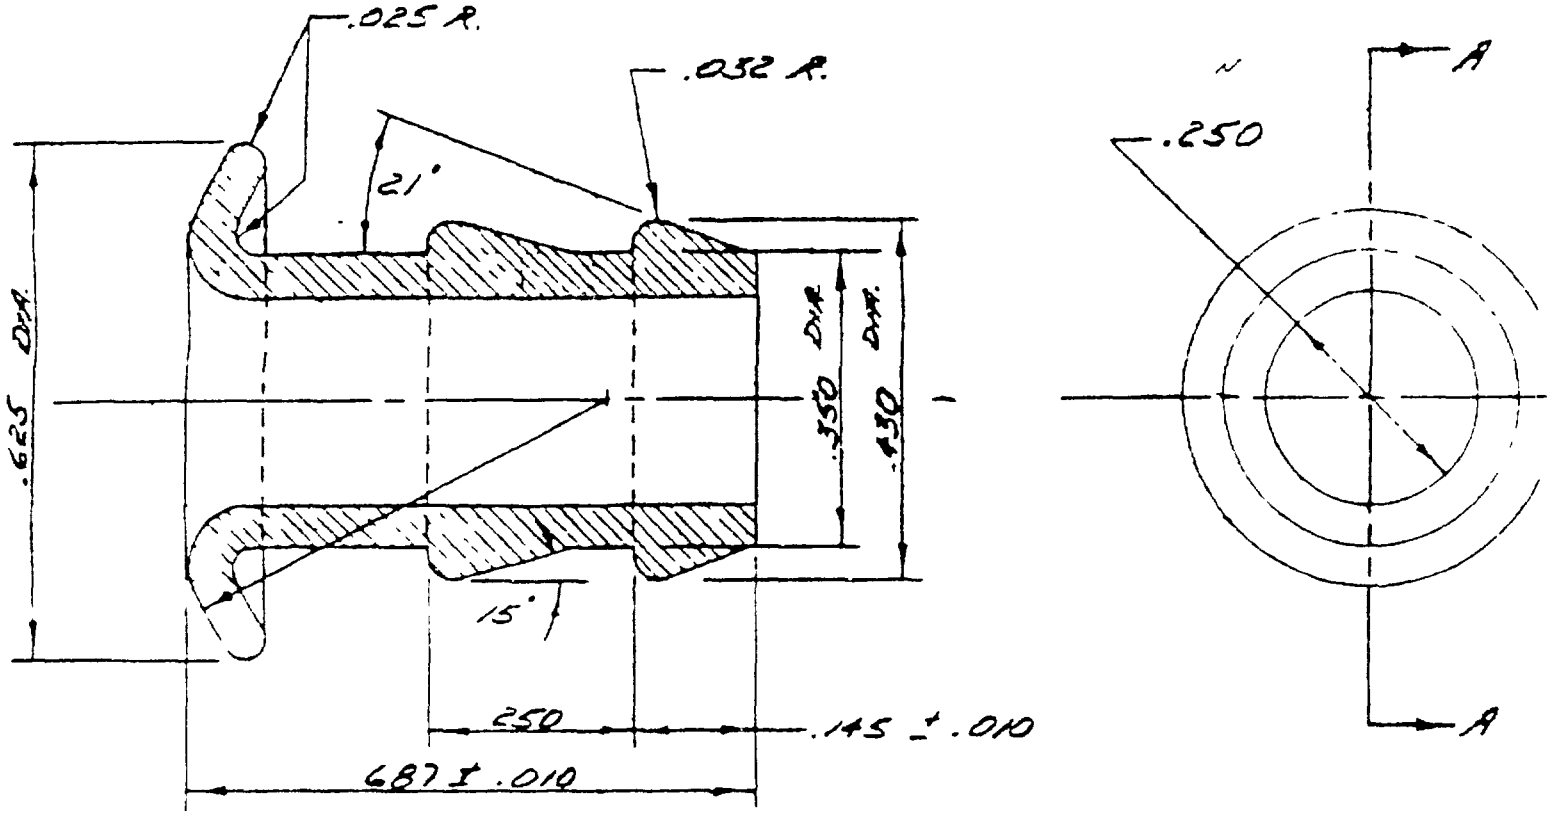

SECTION A-A

(3) PLASTIC FITMENT


SCALE 5 x SIZE

NOTES:

1. TOLERANCE UNLESS OTHERWISE SPECIFIED ± .002.
2. MATERIAL REQ'D - SEE PURCHASE DESCRIPTION
3. SUPERCEDES ALL PREVIOUS PRINTS
4. MAY 25 RD, 1977 1° DRAFT ON CENTER HOLE ALLOWED

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:37Z
Check the source to verify that this is the current version before use.

TYPE I

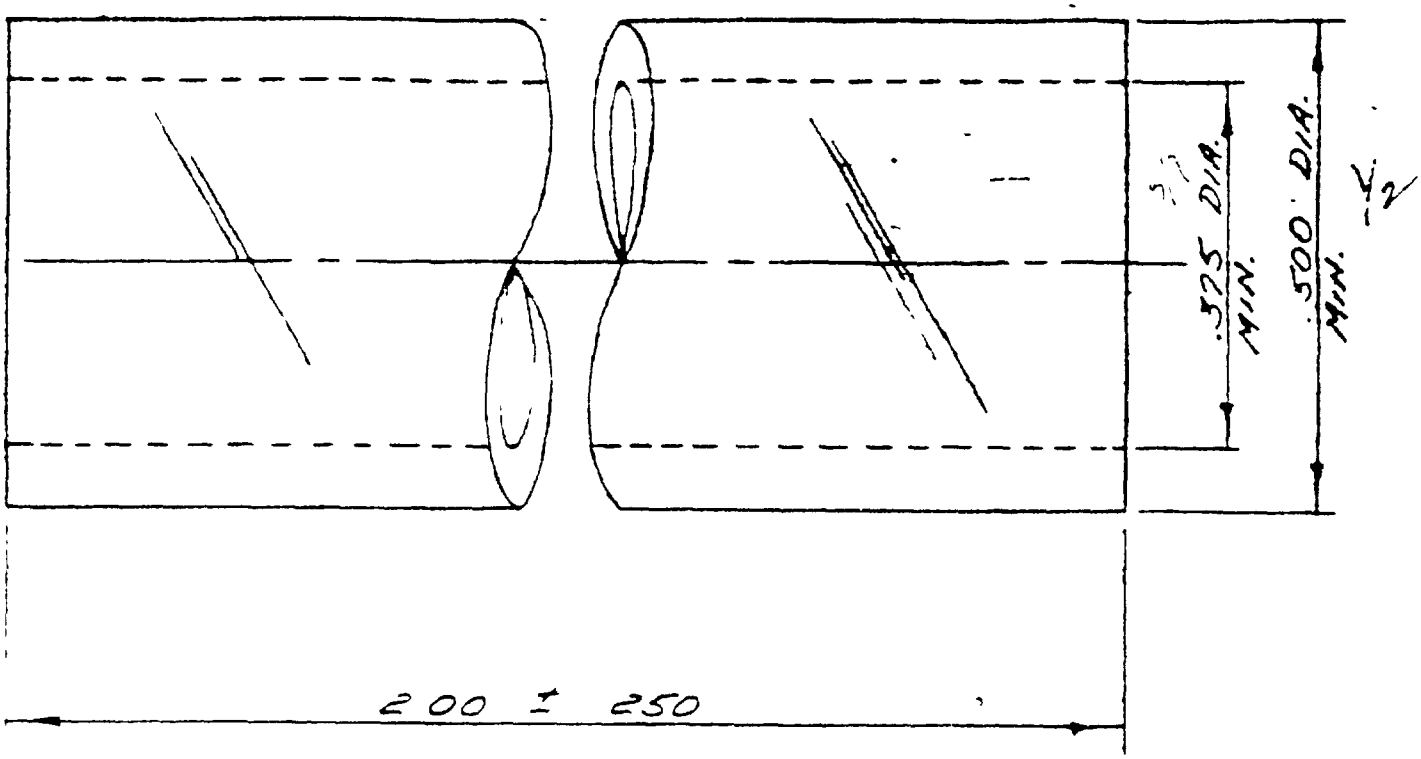


4 TUBE

SCALE · 5 × SIZE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:37Z
Check the source to verify that this is the current version before use.


TYPE I

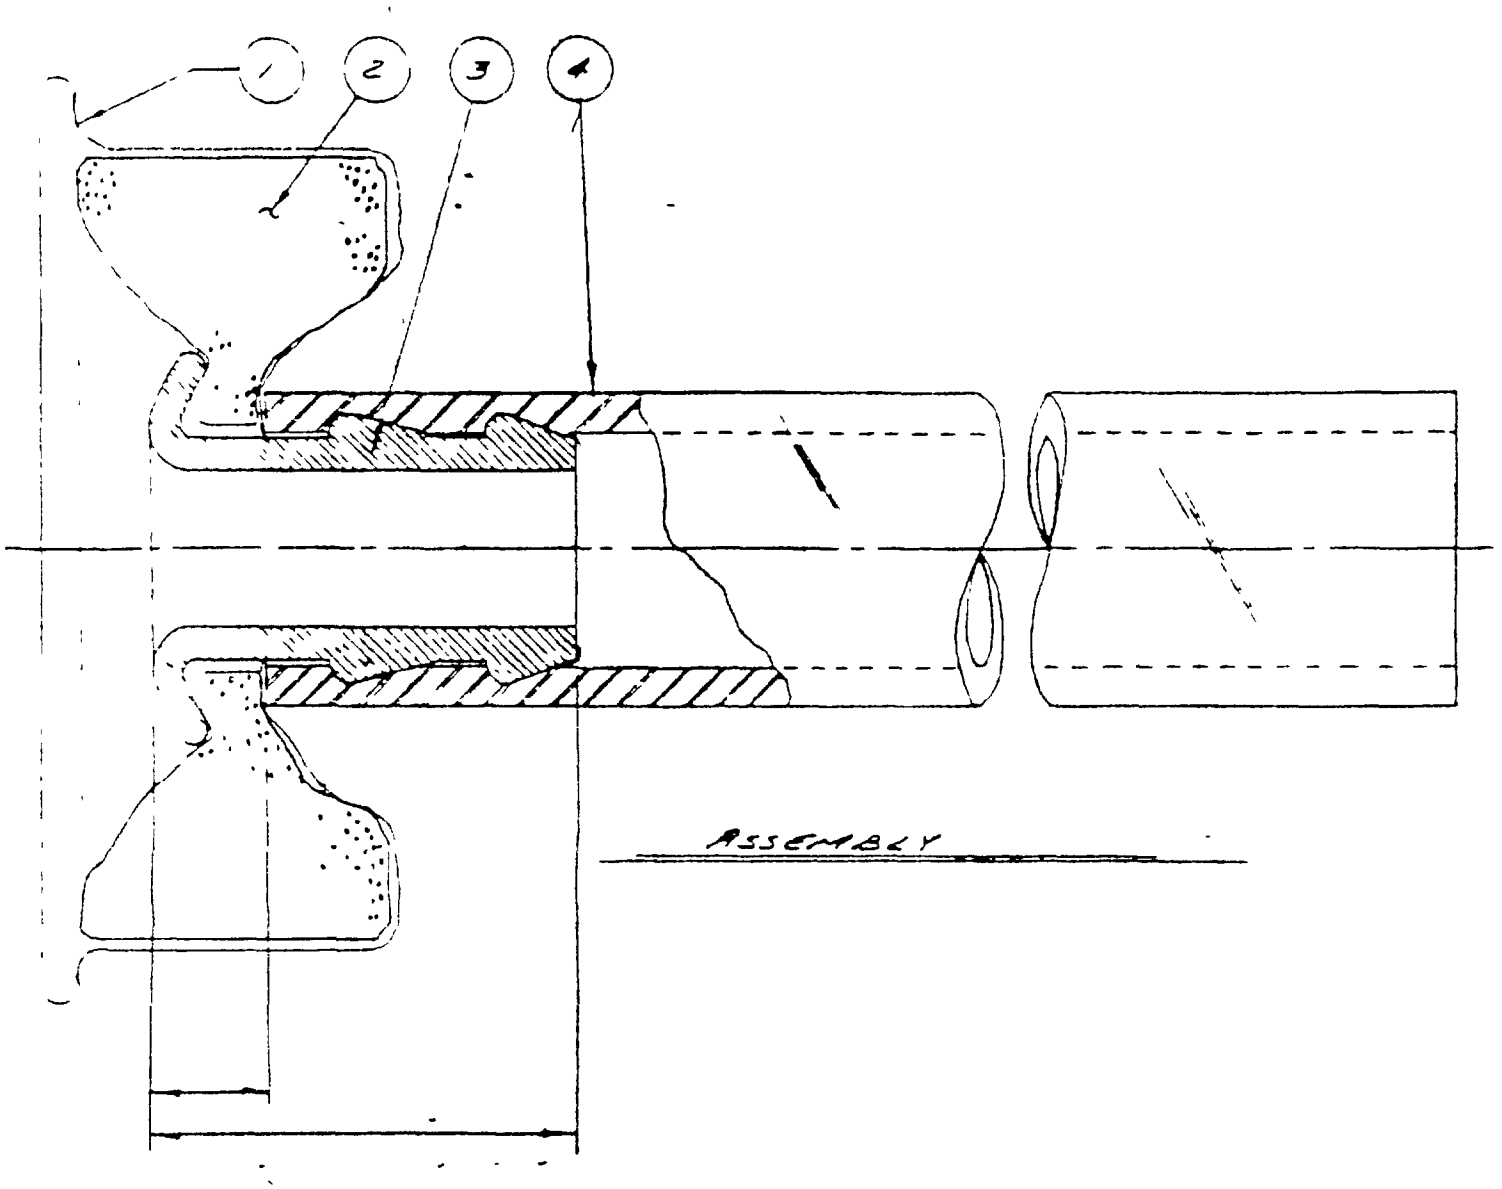

ASSEMBLY

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:37Z
Check the source to verify that this is the current version before use.

TYPE II

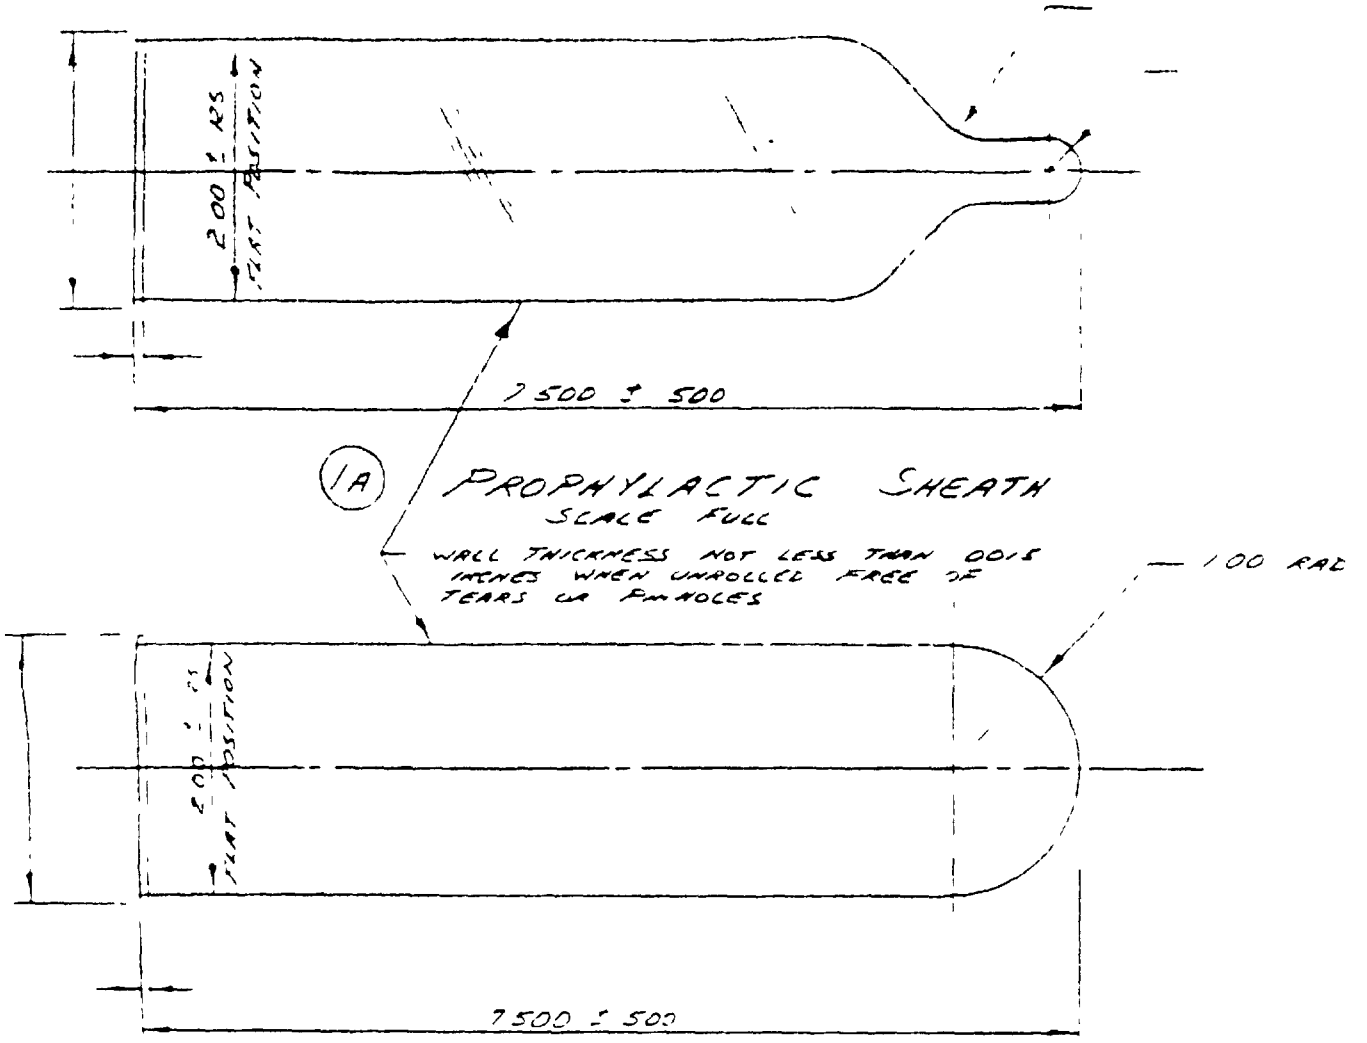


(1A) PROPHYLACTIC SHEATH
SCALE FULL

WALL THICKNESS NOT LESS THAN 0015 INCHES WHEN UNROLLED FREE OF TEARS OR PINHOLES

(1) PROPHYLACTIC SHEATH
SCALE FULL

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:37Z
Check the source to verify that this is the current version before use.

TYPE II

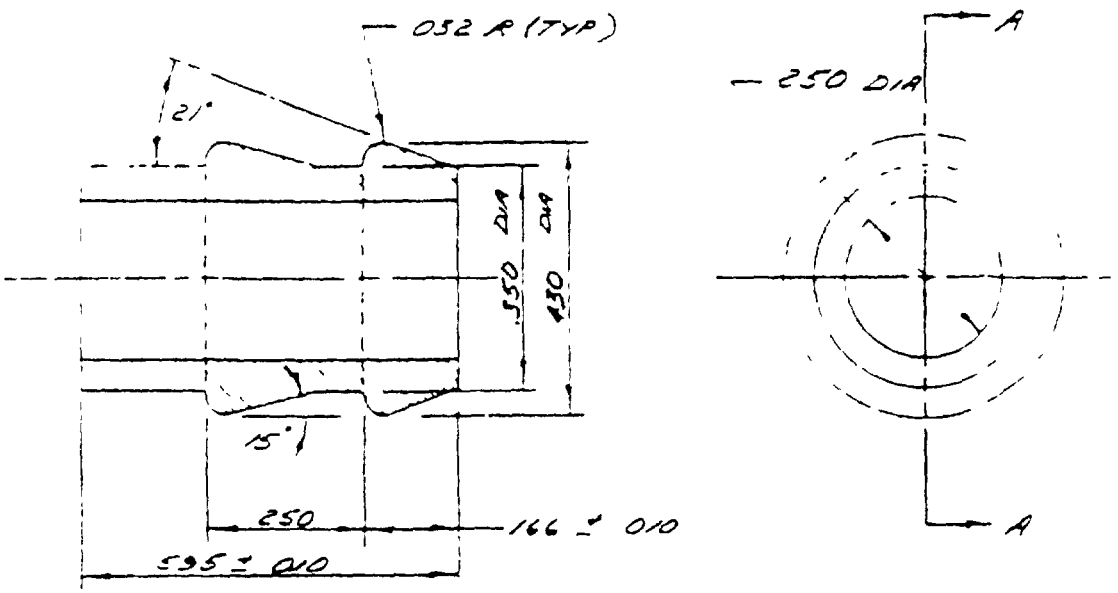

SECTION A-A
SCALE: 5 x SIZE

(2) PLASTIC FITMENT

FITMENT WITHOUT PLASTIC DISC

NSN 6530-01-004-8969 (JAN 20 1977)
CARINAL, INCONTINENT (EXTERNAL CATHETER)

NOTES
1 TOLERANCE UNLESS OTHERWISE SPECIFIED ± .002
2 MATERIAL REQ'D. SEE PURCHASE DESCRIPTION

3 SUPERCEDES ALL PREVIOUS PRINTS
4: MAY 25 AD 1977. 1st DRAFT ON CENTER HOLE ALLOWED

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:37Z
Check the source to verify that this is the current version before use.

TYPE II


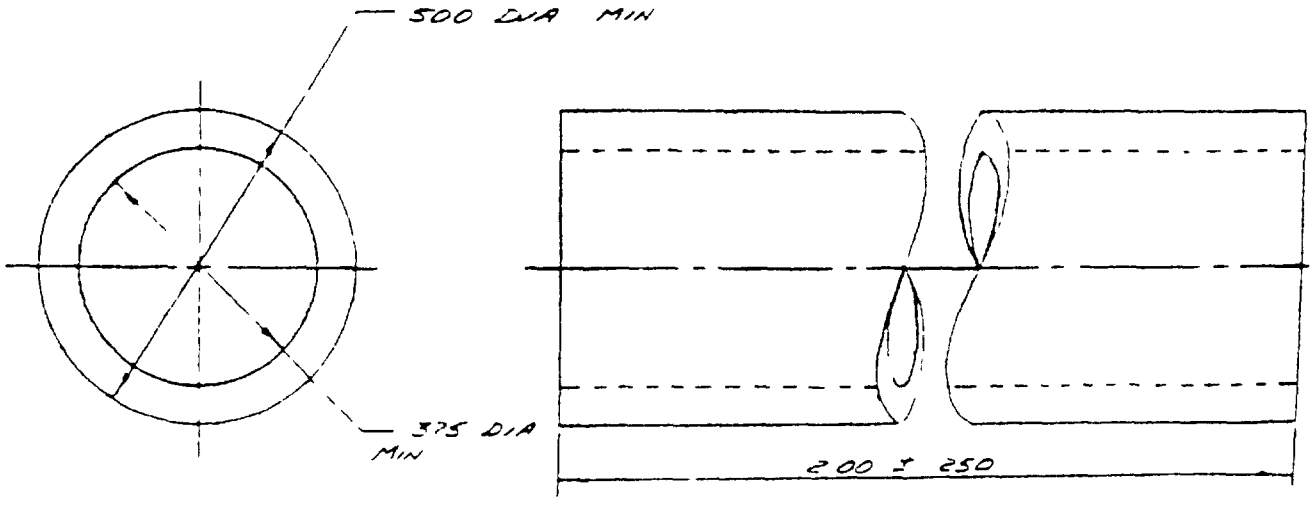


FIG 5 TYPE II

SCALE 5 × SIZE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:37Z
Check the source to verify that this is the current version before use.

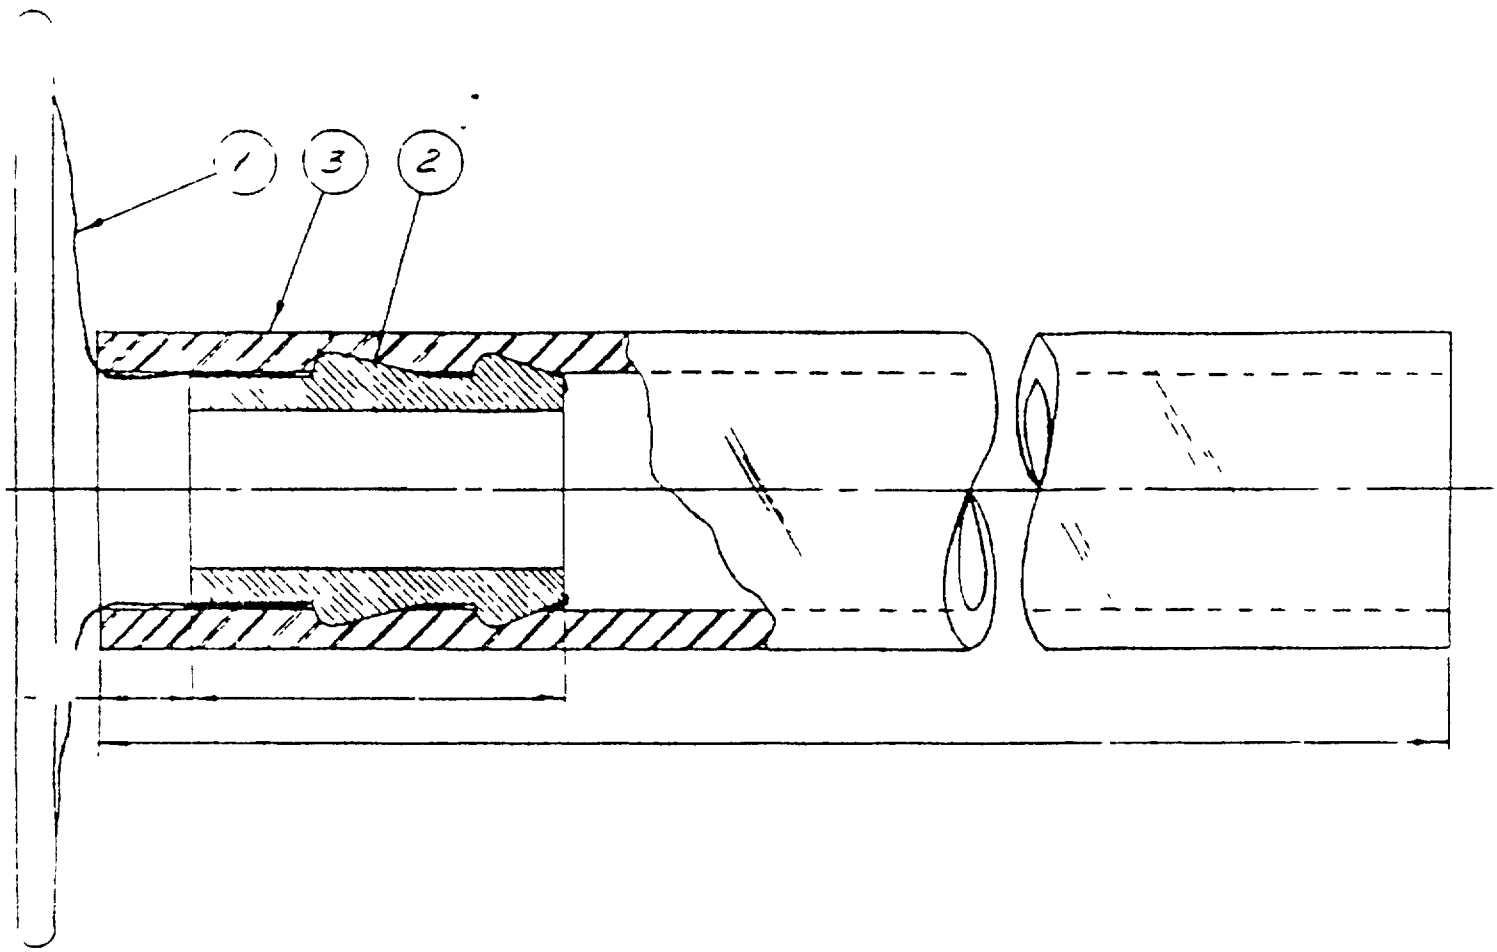


ASSEMBLY

SCALE: 5 x SIZE

VETERANS ADMINISTRATION SPECIFICATION

- URINAL, INCONTINENT (EXTERNAL CATHETER)
- TYPE II - WITHOUT PLASTIC DISC AND RING

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:37Z
Check the source to verify that this is the current version before use.

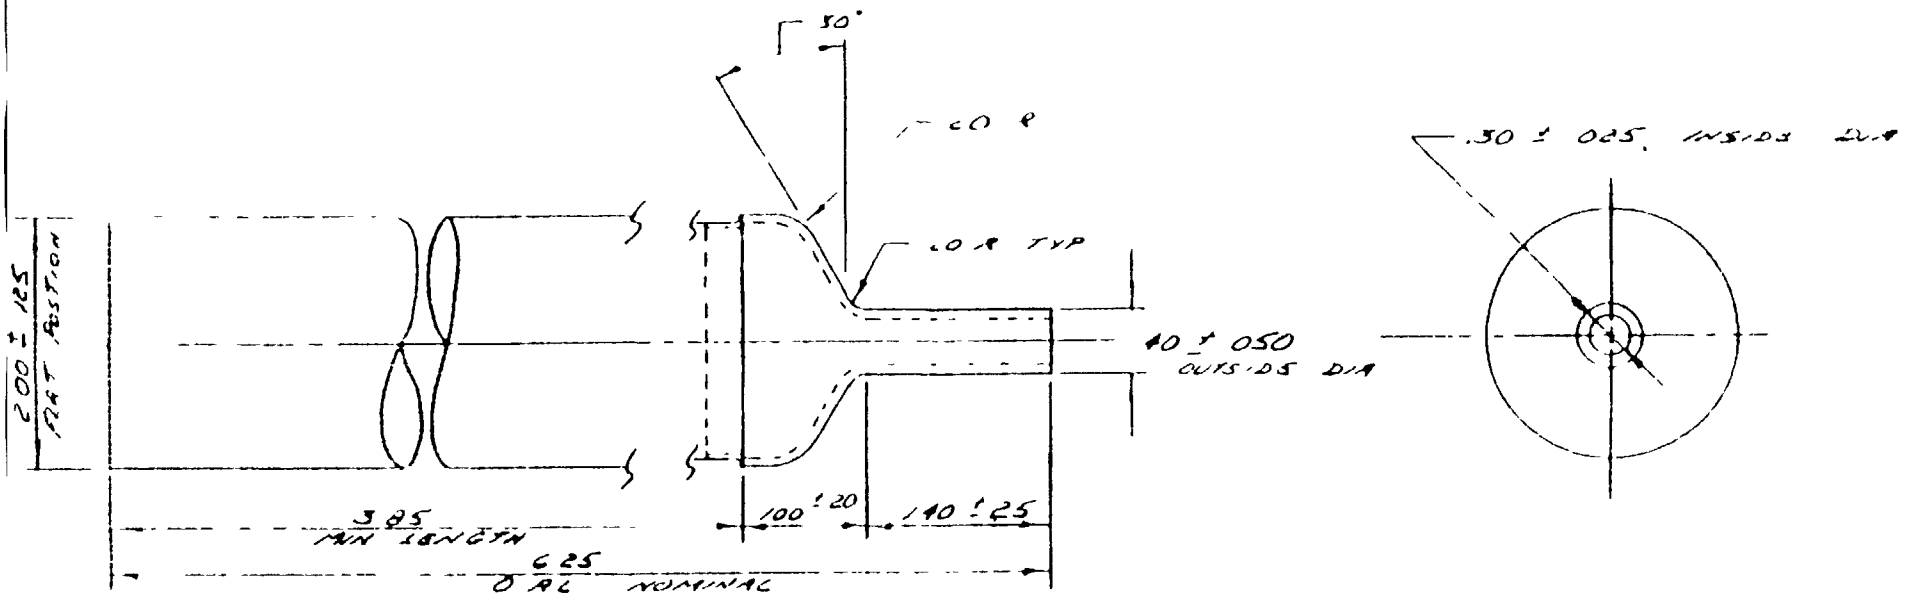

NOTE WALL THICKNESS .040 TO .050 FOR TIP SECTION OF CATHETER
SHEATH THICKNESS .005 ± .002

TYPE III ONE PIECE LATEX CATHETER

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:37Z
Check the source to verify that this is the current version before use.