A-A-53457
19 April 1988

COMMERCIAL ITEM DESCRIPTION

FORCEPS, FOREIGN BODY INTRAOCULAR

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers an intraocular forceps suitable for grasping, holding, and removing foreign bodies during ophthalmic surgical procedures.

Salient characteristics:

Material. Internal surfaces of the jaw tips shall have a coating of diamond dust. The jaws shall be fabricated of martensitic corrosion-resistant steel in accordance with American Society for Testing and Materials (ASTM) Designation F899.

Hardness. Jaw tips shall have a Rockwell Hardness C scale (HRC) of 50 to 55. The hardness shall be tested in accordance with ASTM Designation E18 or ASTM Designations E92 and E140.

Style and design. Forceps shall be in accordance with Figure 1. The jaw tips shall open by means of a lever. Upon release of the lever, the jaw tips shall be self-closing. Forceps shall be cylindrically shaped. The base of the forceps shall have a female Luer taper in accordance with ANSI/HIMA MD70.1. The Luer opening shall be connected internally, so as to permit flushing of the jaw tips with water.

Finish. The finish of the forceps shall be mirror or satin.

Passivation. The forceps shall be properly passivated.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

Corrosion resistance. Forceps shall show no corrosion when subjected to the Boil Test and Copper Sulfate Test as specified in ASTM Designation F1089.

Sterilization. The forceps shall also be capable of steam autoclaving for 10 minutes at 135°C (36 psi) and ethylene oxide sterilization. The forceps shall have a mechanism for retaining the jaw tips in an open position during sterilization.

Identification markings. The forceps shall bear the contractor's name or registered trademark and the word "stainless". Forceps of foreign manufacture shall bear the name of the country of manufacture.

Workmanship. The forceps shall be processed in such a manner as to be uniform and free from defects which affect life, utility or appearance.

PRODUCT QUALITY LEVEL.

Visual and dimensional examination. Shall be examined to verify that the design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Certificate of quality. Certificate of quality supplied by the manufacturer of the steel may be furnished in lieu of actual performance of composition testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the National Stock Number, the item identification, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

Unit. Each (EA). One forceps, as specified, constitutes one unit.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Certificate of quality. Certificate of quality, supplied by the manufacturer of the materials, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of manufacturer or supplier, the NSN, the item identification, the name of the component/material, the lot number and the lot size.

Examination. The forceps shall be examined to determine compliance with specification requirements.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one forceps. Sampling shall be S-4 and an AQL of 1.0 percent.

Source: https://assist.dla.mil -- Downloaded: 20260-26T09:20Z
Check the source to verify that this is the current version before use.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable. The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-243-0512	FORCEPS, FOREIGN BODY INTRAOCULAR

Ordering data. (Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4059

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:20Z
Check the source to verify that this is the current version before use.

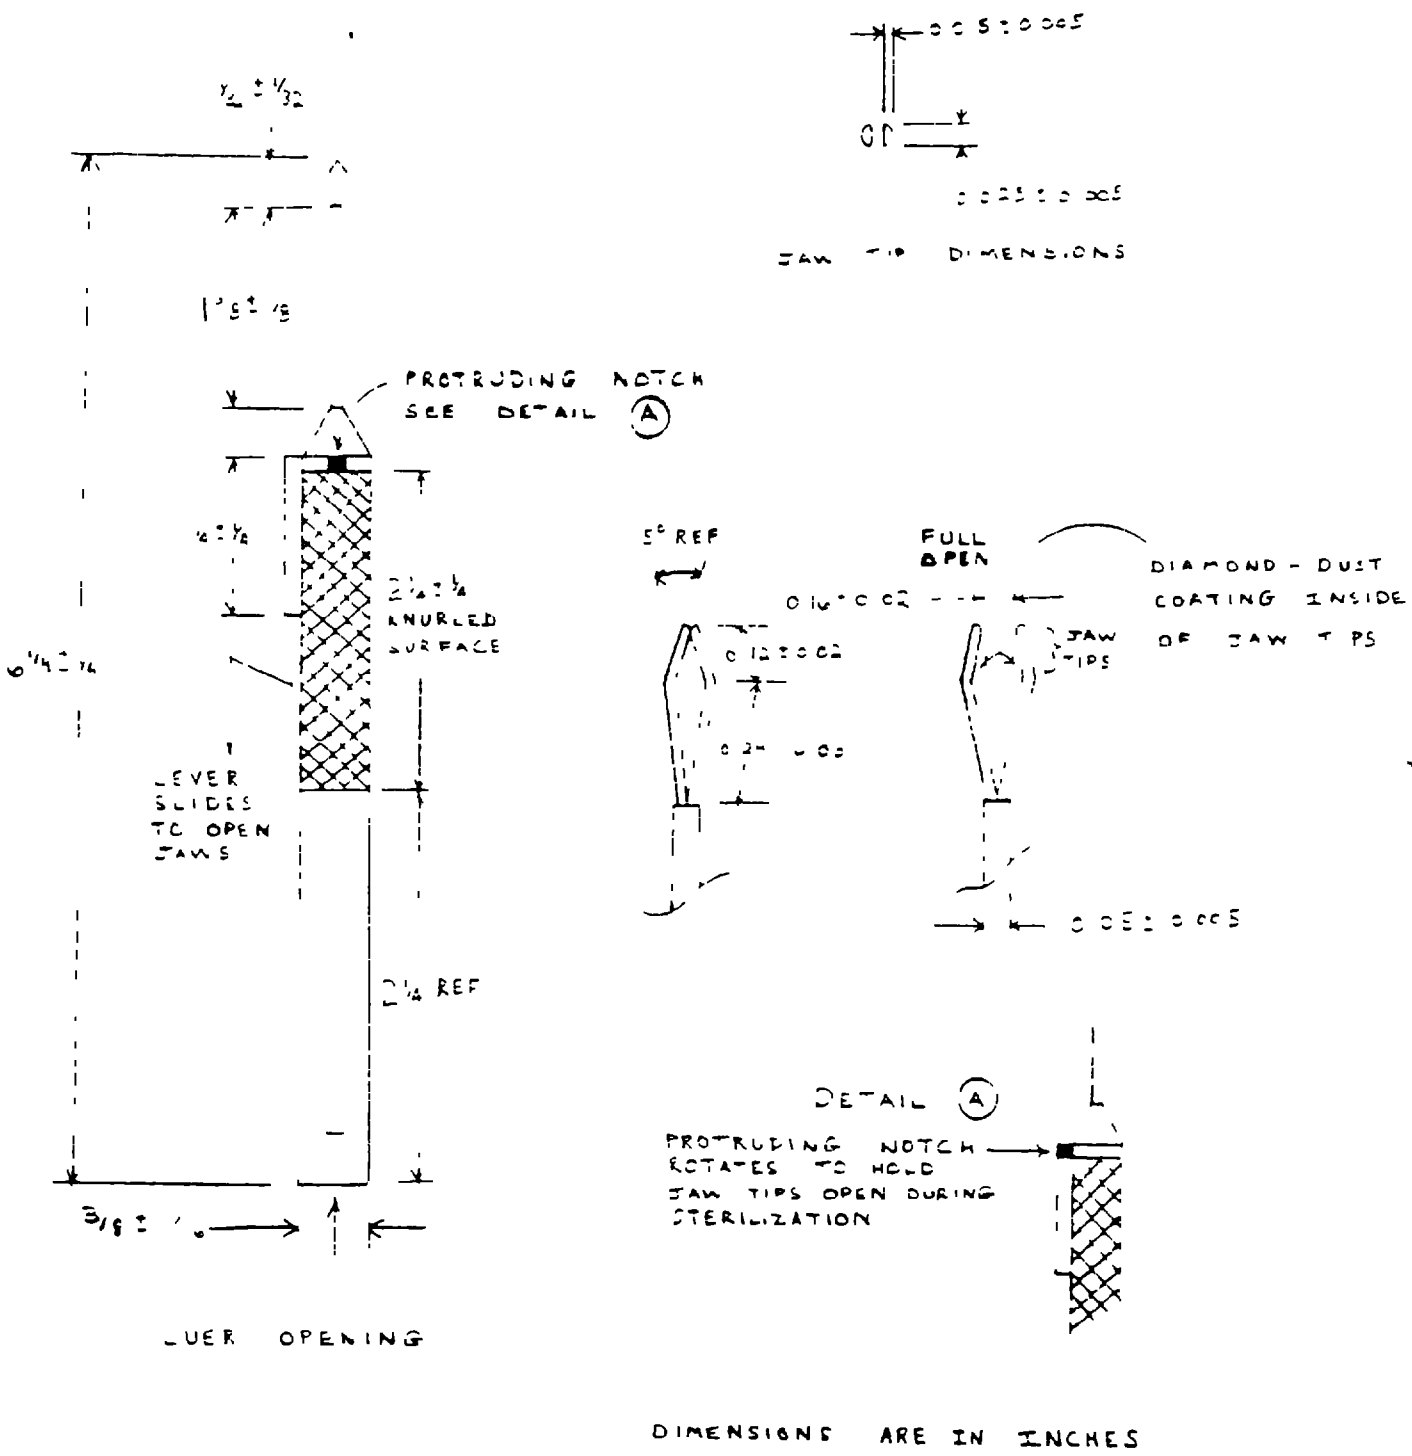


FIGURE 1: FORCEPS, FOREIGN BODY, INTRAOCULAR

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS In a continuing effort to make our standardization documents better the DoD provides this form for use in submitting comments and suggestions for improvements All users of military standardization documents are invited to provide suggestions This form may be detached, folded along the lines indicated taped along the loose edge (*DO NOT STAPLE*), and mailed In block 5 be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive loose ambiguous or was incompatible and give proposed wording changes which would alleviate the problems Enter in block 6 any remarks not related to a specific paragraph of the document If block 7 is filled out an acknowledgement will be mailed To ensure that you know that your comments were received and are being considered

NOTE This form may not be used to request copies of documents nor to request waivers deviations or clarification of specification requirements or current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements

Fold along this line

Fold along this line

DEFENSE LOGISTICS AGENCY

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4956 WASHINGTON D C
POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

NO POSTAGE
NECESSARY
IF MAILED
IN THE
UNITED STATES

Commander
Defense Personnel Support Center
ATTN DPSC-ATTS
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:20Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1 DOCUMENT NUMBER	2 DOCUMENT TITLE
A-A-53457	FORCEPS, FOREIGN BODY INTRAOCULAR

3a NAME OF SUBMITTING ORGANIZATION	4 TYPE OF ORGANIZATION (Mark one)
	☐ VENDOR
b ADDRESS (Street, City, State, ZIP Code)	☐ USER
	☐ MANUFACTURER
	☐ OTHER (Specify)

5 PROBLEM AREAS

a Paragraph Number and Wording

b Recommended Wording

c Reason/Rationale for Recommendation

6 REMARKS

7a NAME OF SUBMITTER (Last, First, MI – Optional)	b WORK TELEPHONE NUMBER (Include Area Code) – Optional
c MAILING ADDRESS (Street, City, State, ZIP Code) – Optional	8 DATE OF SUBMISSION (YYMMDD)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.