A-A-53458
20 April 1988

COMMERCIAL ITEM DESCRIPTION

ELEVATOR-RETRACTOR, PERIOSTEAL (Crego)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a Crego periosteal elevator-retractor suitable for stripping ligament and capsular attachments from the talus and its joints during orthopedic surgery and can serve as an atraumatic retractor for soft tissue.

Salient characteristics:

General. The elevator-retractor shall have an overall length of eight inches. The handle shall be hollow with longitudinal indentations to facilitate grasping.

Materials. The elevator-retractor shall be fabricated of Class 4 martensitic stainless steel in accordance with ASTM Designation F899. As an alternate, the handle may be fabricated from Class 3 austenitic stainless steel in accordance with American Society for Testing and Materials (ASTM) Designation F899.

Hardness. The elevator-retractor shall have a Rockwell Hardness C scale (HRC) of 40 to 45 for Class 4 material and a Rockwell Hardness B scale (HRB) of 75, minimum for Class 3 material. The hardness shall be tested in accordance with ASTM Designation E18 or ASTM Designations E92 and E140.

Style, design and dimensions. The elevator-retractor shall have a curved blade 1-3/8 inch in diameter and 9/16 inch wide. The blade shall be blunt edged. The handle shall have separate indentations for the thumb and forefinger on the top and bottom of the handle. The elevator-retractor shall be in accordance with Figure 1.

Finish. The finish of the elevator-retractor shall be entirely mirror, satin or matte. The matte finish shall exhibit a uniform non-directional surface equivalent to that produced by blasting the prepared surface with fine abrasives under pressure.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as follows: At an inspection level of S-2, dimension testing shall be conducted at a 2.5 percent AQL, hardness testing at a 1.5 percent AQL. Boil testing and copper sulfate testing shall be conducted at a 1.0 percent AQL. The unit of product shall be one elevator-retractor.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric product. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerance specified in the inch/pound units. A request should be made to the contracting officer to determine if the product is acceptable. The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:20Z
Check the source to verify that this is the current version before use.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as follows: At an inspection level of S-2, dimension testing shall be conducted at a 2.5 percent AQL, hardness testing at a 1.5 percent AQL. Boil testing and copper sulfate testing shall be conducted at a 1.0 percent AQL. The unit of product shall be one elevator-retractor.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric product. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerance specified in the inch/pound units. A request should be made to the contracting officer to determine if the product is acceptable. The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-139-8269	ELEVATOR-RETRACTOR, PERIOSTEAL, CREGO, Curved Blade, 1-3/ Inch Inside Diameter, 9/16 Inch Wide, Blunt Edge

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.)

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA - OSS
PHS
FDA-MPQAS

Project No. 6515-3883

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

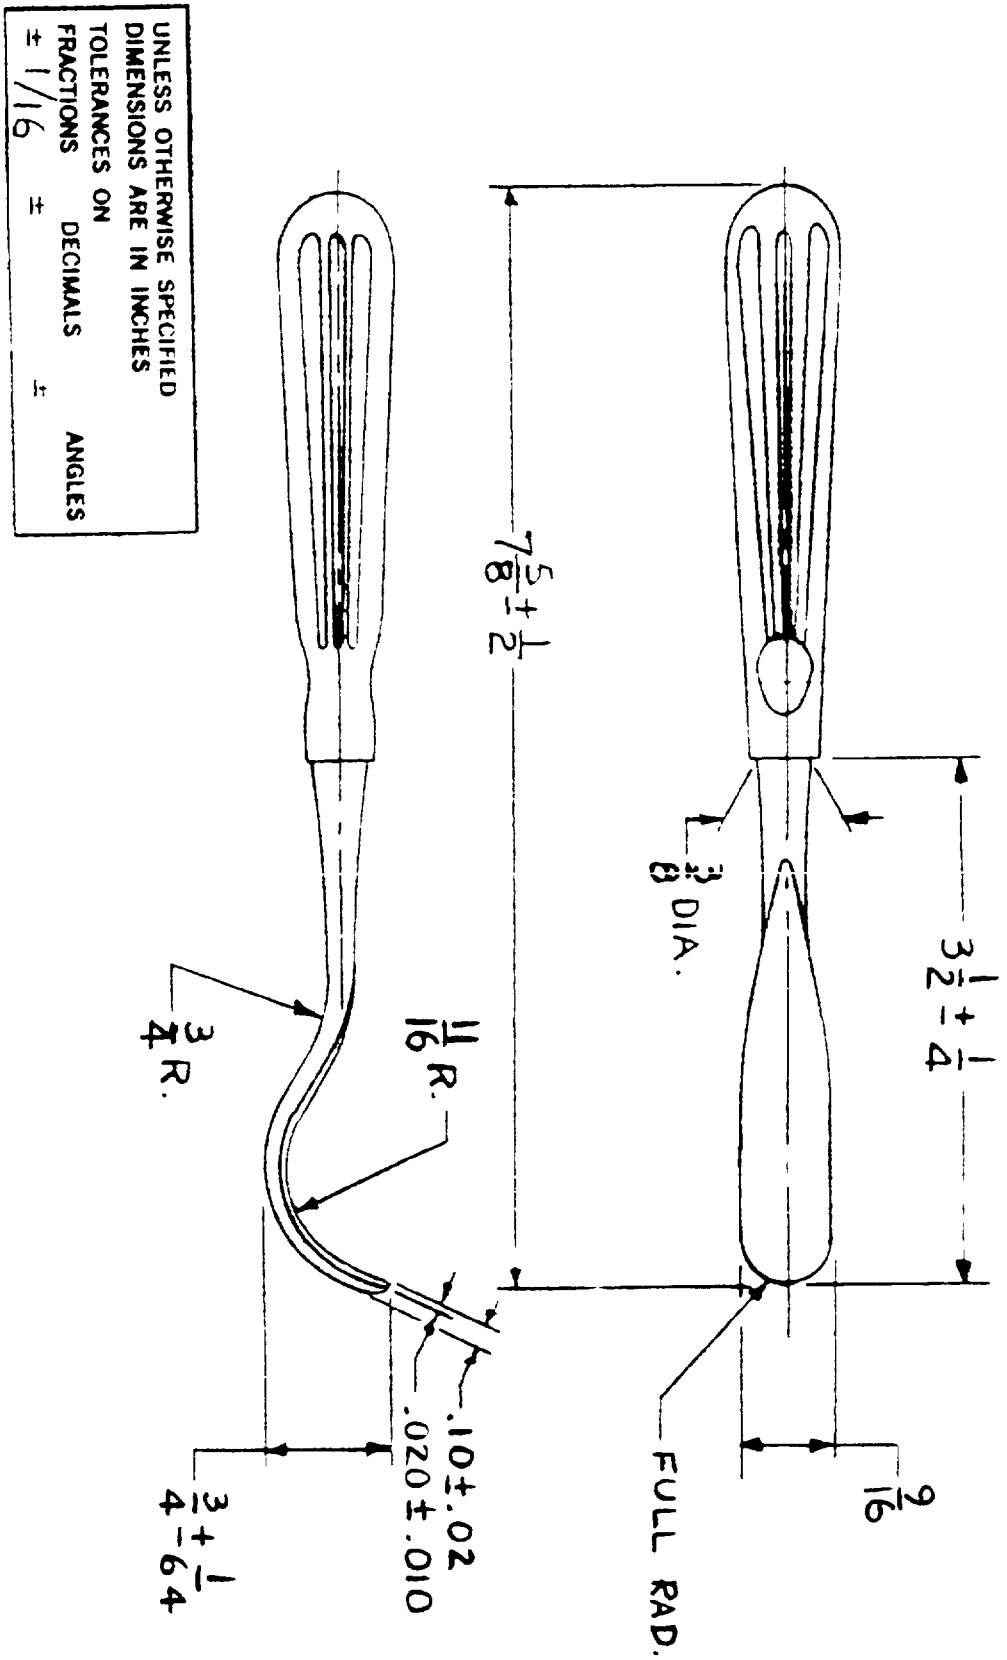


FIGURE 1 ELEVATOR-RETRACTOR, PEREOSTEAL, CREGO

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:20Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS. In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE. This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 Alexandria, VA

POSTAGE WILL BE PAID BY

Commander
Defense Personnel Support Center
ATTN: DPSC-RSTS
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:20Z
Check the source to verify that this is the current version before use.

(TO DETACH THIS FORM CUT ALONG THIS LINE.)

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1 DOCUMENT NUMBER	2 DOCUMENT TITLE
A-A-53458	ELEVATOR-PERIOSTEAL (Crego)

3a NAME OF SUBMITTING ORGANIZATION	4 TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
	☐ USER
b ADDRESS *(Street City State ZIP Code)*	☐ MANUFACTURER
	☐ OTHER *(Specify)* _____

5 PROBLEM AREAS

a Paragraph Number and Wording

b Recommended Wording

c Reason/Rationale for Recommendation

6 REMARKS

7a NAME OF SUBMITTER *(Last First MI)* – Optional	b WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c MAILING ADDRESS *(Street City State ZIP Code)* – Optional	8 DATE OF SUBMISSION *(YYMMDD)*

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:20Z
Check the source to verify that this is the current version before use.