
USER ACTIVITIES: ARMY - CE
NAVY - MC

FED. SUP CLASS
6630

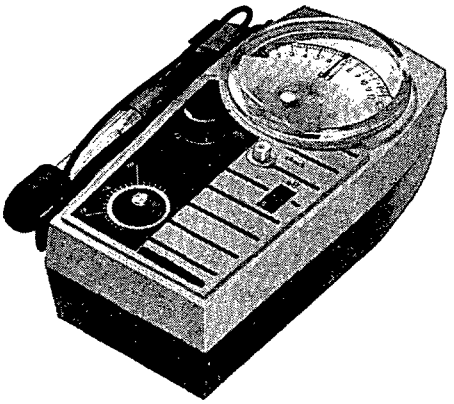

PART NUMBER	pH RANGE	O/A DIMENSIONS (in.)		
		LG	W	H
MS36469-1	0 - 14	6	3	2

MATERIAL: Meter housing shall be of molded melamine plastic.

Carrying case shall be of leather.

DESIGN: Meter shall be of the hand-sized, battery-operated type which has a combination glass and reference electrode, with a three-foot lead, which can be used as a probe in liquids and semi-solid samples. Meter scale shall be graduated from 2 to 12 pH in 0.2 pH divisions and shall be readable to 0.1 pH with an accuracy of $\pm$ 0.05 pH unit. Carrying case shall be designed to accommodate the meter and all accessories.

PURPOSE: To measure the hydrogen ion concentration of semi-solids and liquids.

COMPONENTS: Meter shall include a vial of pH 7 buffer, buffer vial with sponge, potassium chloride-silver chloride crystals, a box of tissue paper, and the six batteries required for operation.

NOTE: Items differing from this Mititary Standard by minor variations in design or dimensions are considered standard under this document, provided such variations do not affect performance and are not in conflict with the material requirements as specified herein.

☆ U. S. GOVERNMENT PRINTING OFFICE: 1968-341-512/A-2119

APPROVED REVISED

This military standard is approved by the Department of Defense and is mandatory on all activities. Selection for all new engineering and design applications and for repetitive use shall be made from this document

P.A.	MU	TITLE	MILITARY STANDARD
Other Cust	MS 82	METER, HYDROGEN ION TEST Pocket Type	MS 36469
Procurement Specification NONE		SUPERSEDES:	SHEET 1 OF 1

DD FORM 1 SEP 63 672 (Coordinated) EDITION OF 1 SEP 57 MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 2026-10-23T17:41Z
Check the source to verify that this is the current version before use.