INCH-POUND

A-A-54823
28 May 1993

COMMERCIAL ITEM DESCRIPTION

RETRACTOR, HEMILAMINECTOMY, HAVERFIELD-SCOVILLE AND BLADES, INTERCHANGEABLE

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Military Specification MIL-R-37103B which is cancelled.

This Commercial Item Description covers a hemilaminectomy retractor with detachable and interchangeable blades that is suitable for use in hemilaminectomy procedures.

Salient characteristics:

General. The hemilaminectomy retractor shall be of the Haverfield Scoville body design having selected styles and sizes of detachable and interchangeable blades as follows:

Style I - Scoville Hook

Size	Description
1	Blunt hook, 2 inches deep.
2	Blunt hook, 3 inches deep.

Style II - Taylor Laminectomy

Size	Description
1	Small, 3 prongs, 1-3/4 inches deep, 1-1/2 inches wide.
2	Medium, 4 prongs, 1-7/8 inches deep, 2 inches wide.
3	Large, 4 prongs, 2-1/2 inches deep, 2-1/4 inches wide.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Style III - Scoville Laminectomy

Size	Description
1	4 Prongs, 1-5/8 inches deep, 1-1/2 inches wide.
2	4 Prongs, 2-5/8 inches deep, 1-3/4 inches wide.

Style IV - Epstein Hemilaminectomy, 2-1/4 inches deep, 1 inch wide.

Style V - Hibbs

Size	Description
1	2 inches deep, 1 inch wide.
2	2 inches deep, 2 inches wide.
3	3 inches deep, 1 inches wide.
4	3 inches deep, 2 inches wide.
5	4 inches deep, 2 inches wide.

Style VI - Meyerding Laminectomy

Size	Description
1	2-1/4 inches deep, 1 inch wide
2	3 inches deep, 1 inch wide.
3	3-1/2 inches deep, 2 inches wide.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Material. The retractor assembly components shall be fabricated from class 3 austenitic corrosion-resistant steel or class 4 martensitic corrosion-resistant steel in accordance with ASTM F899. The retractor assembly individual component material breakdown shall be as shown in Figure 1. Type I Blades and the wing nuts shall be fabricated from class 3 austenitic corrosion-resistant steel in accordance with ASTM F899. As an alternate to the designs shown in figures 1-7, a knurled locking device may be used in lieu of a wing nut. The knurled locking device shall be fabricated of class 3 corrosion-resistant stainless steel. Types II, III, IV, V, and VI Blades shall be fabricated from class 4 martensitic corrosion-resistant steel in accordance with ASTM F899.

Hardness. The retractor assembly components or blades fabricated of class 3 material shall have a Rockwell Hardness (HRB) scale of 85 to 100, components or blades fabricated of class 4 material shall have a Rockwell hardness (HRC) scale of 40 to 47 for the appropriate stainless steel type when tested in accordance with ASTM E18 or E92 whichever is applicable. Conversion of hardness values shall be in accordance with ASTM E140.

Style, design and dimensions. The retractor assembly and blades shall be in accordance with Figures 1 thru 7 for appropriate style, design and dimensions.

Performance. Under no circumstances shall looseness or free play permit misalignment of the attachments or blades during normal use of the instrument assembly.

Finish. The retractor assembly and blades shall have a satin or matte finish. The carriage shall have a smooth finish which may be produced by sandblast.

Passivation. The retractor assembly and blades shall be properly passivated.

Corrosion resistance. The retractor assembly and blades shall no evidence of corrosion or plating of copper when tested for corrosion resistance in accordance with ASTM F1089.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Interchangeability and substitutability. Interchangeable parts having the same manufacturer's part number will be functionally and dimensionally interchangeable. Components parts except for blades need not be interchangeable between manufacturers and may not be interchangeable with different model produced by the same manufacturer. All blades regardless of source of manufacture shall be capable of being attached to any manufacturers retractor.

Identification marking and labeling. The retractor assembly and blades shall be legibly marked with the contractor's name or registered trademark and the word "stainless". Foreign manufactured retractor assembly and blades shall bear the name of the country of origin.

Workmanship. The retractor assembly and blades shall be free from defects which detract from its appearance or impair its serviceability.

Unit.

Each (EA) One retractor, as specified, constitutes one unit.

Each (EA). One blade, of the style and size specified, constitutes one unit.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:39Z
Check the source to verify that this is the current version before use.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and as specified herein. Unit of product for examination purposes shall be one retractor assembly and blades. Sampling shall be Inspection level II with an acceptable quality level (AQL) of 1.0.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for test purposes shall be one retractor assembly and blades. Sampling shall be Inspection level S-2 with an AQL of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more text characteristics.

Contractor Certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:39Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction , the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug, and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

NOTE: The following National Stock Numbers are covered by this document:

NSN	Item Identification	Style	Size
6515-00-385-3685	RETRACTOR, LAMINECTOMY, Haverfield-Scoville.	-	-
6515-00-392-0722	BLADE, LAMINECTOMY RETRACTOR, Single Hook, 2 inches Long.	I	1
6515-00-392-0723	BLADE, LAMINECTOMY RETRACTOR, Scoville, Single Hook, 3 inches Long.	I	2

Source: https://assist.dla.mil -- Downloaded: 20260-26T09:39Z
Check the source to verify that this is the current version before use.

NSN	Item Identification	Style	Size
6515-00-379-4389	BLADE, LAMINECTOMY RETRACTOR, Tayler, 3 Prong, 1-3/4 inches Long, 1-1/2 inches Wide.	II	1
6515-00-376-7776	BLADE, LAMINECTOMY RETRACTOR, Tayler, 4 prong, 1-7/8 inches Long, 2 inches Wide.	II	2
6515-00-376-7784	BLADE, LAMINECTOMY RETRACTOR, Taylor, 4 Prong, 2-1/2 inches Long, 2-1/4 inches Wide.	II	3
6515-00-376-7789	BLADE, LAMINECTOMY RETRACTOR, Scoville, 4 Prong, 1-5/8 inches Long, 1-1/2 inches Wide.	III	1
6515-00-385-3687	BLADE, LAMINECTOMY RETRACTOR, Scoville, 4 Prong, 2-5/8 inches Long, 1-3/4 inches Wide.	III	2
6515-00-385-3710	BLADE, LAMINECTOMY RETRACTOR, Epstein, Single Prong, 2-1/4 inches Long, 1 inch Wide.	IV	-
6515-00-385-3711	BLADE, LAMINECTOMY RETRACTOR, Hibbs, Single Prong, 2 inches Long, 1 inch Wide.	V	1
6515-00-385-3739	BLADE, LAMINECTOMY RETRACTOR, Hibbs, Single Prong, 2 inches Long, 2 inches Wide.	V	2
6515-00-385-3740	BLADE, LAMINECTOMY RETRACTOR, Hibbs, Single Prong, 3 inches Long, 1 inch Wide.	V	3
6515-00-385-3751	BLADE, LAMINECTOMY RETRACTOR, Hibbs, Single Prong, 3 inches Long, 2 inches Wide.	V	4
6515-00-111-6383	BLADE, LAMINECTOMY RETRACTOR, Hibbs, Single Prong, 4 inches Long, 2 inches Wide.	V	5
6515-00-389-9289	BLADE, LAMINECTOMY RETRACTOR, Meyerding, Single Prong 2-1/4 inches Long, 1 inch Wide.	VI	1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

A-A-54823

NSN	Item Identification	Style	Size
6515-00-389-9291	BLADE, LAMINECTOMY RETRACTOR, Meyerding, Single Prong 3 inches Long, 1 inch Wide.	VI	2
6515-00-392-0724	BLADE LAMINECTOMY RETRACTOR, Meyerding, Single Prong, 3-1/2 inches Long, 2 inches Wide.	VI	3

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project No. 6515-5240

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:39Z
Check the source to verify that this is the currentversion before use.

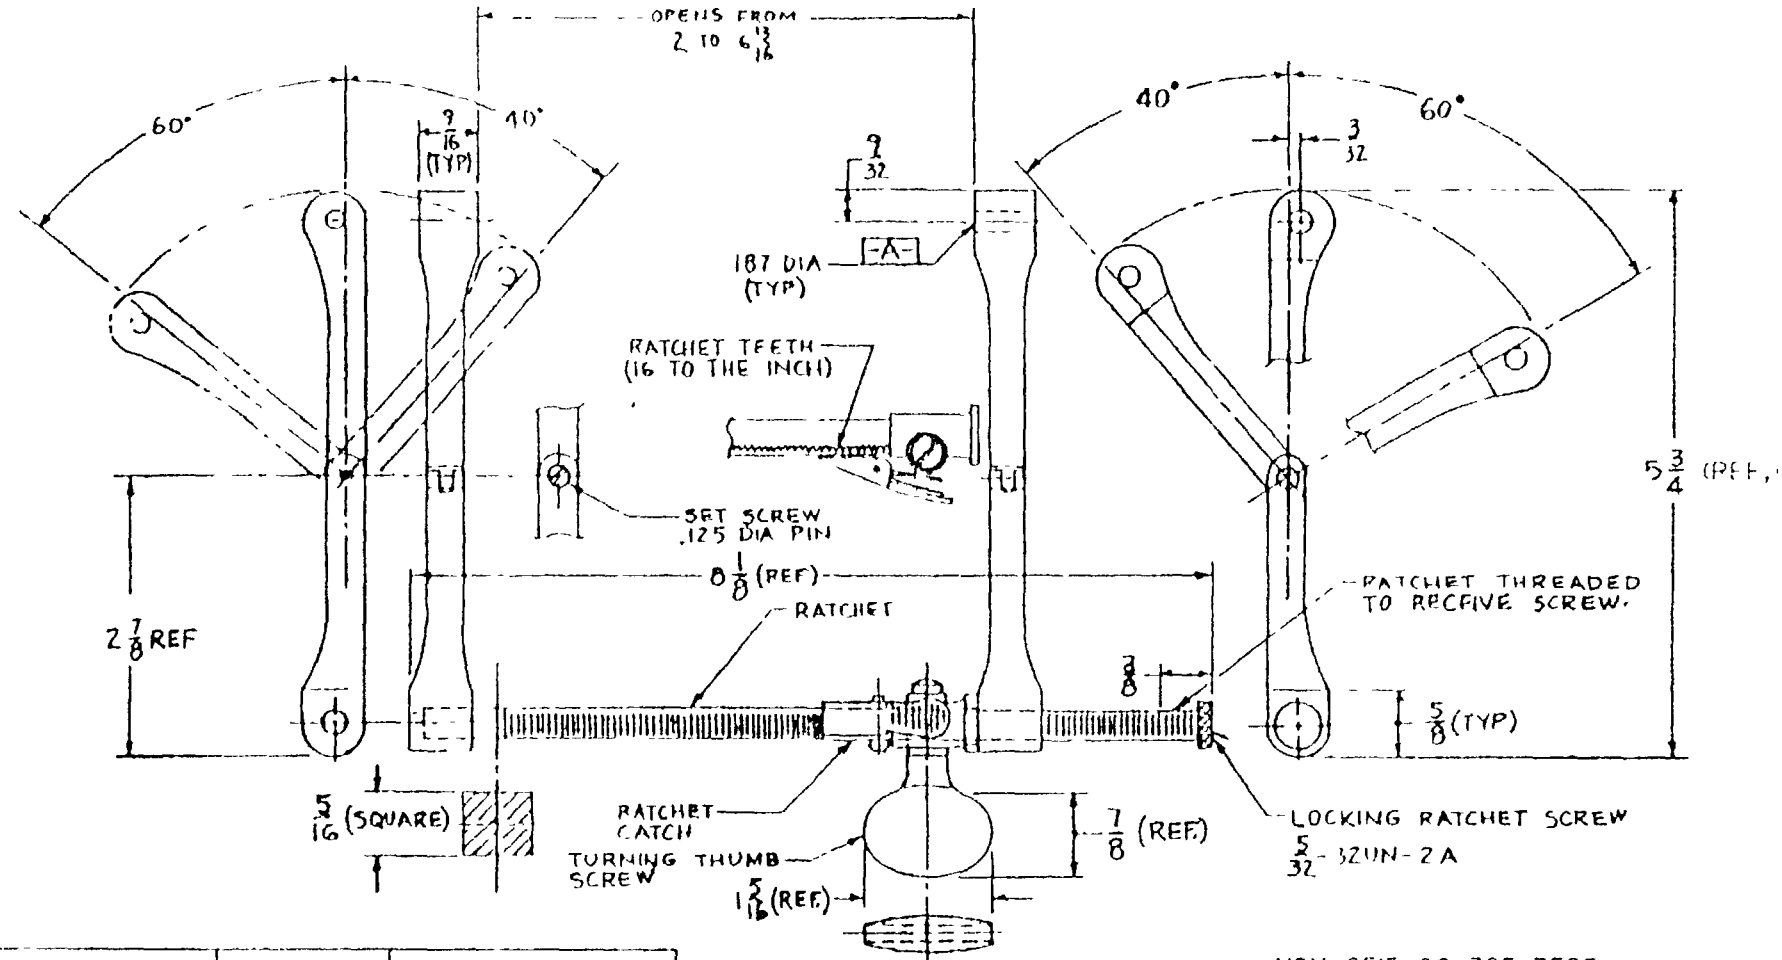


COMPONENT PART	QUANTITY	STAINLESS STEEL CLASS
ARMS	2	1
ARM SCREWS	2	1
CARRIAGE	1	3
CARRIAGE SPRING	1	3
PAWL	1	3
PAWL SCREWS	1	3
RACK	1	1
RACK SCREWS	1	3
CARRIAGE SCREWS	1	3
THUMB PIECE	1	3
PINION GEAR	1	1

NSN 6515-00-385-3585

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES.
TOLERANCES ON:
FRACTIONS ±1/32 DECIMALS ± ANGLES ±3°


FIGURE 1. RETRACTOR, LAMINECTOMY, HAVERFIELD-SCOVILLE

Source: https://assist.dla.mil -- Downloaded: 2026/10-26T09:39Z
Check the source to verify that this is the current version before use.

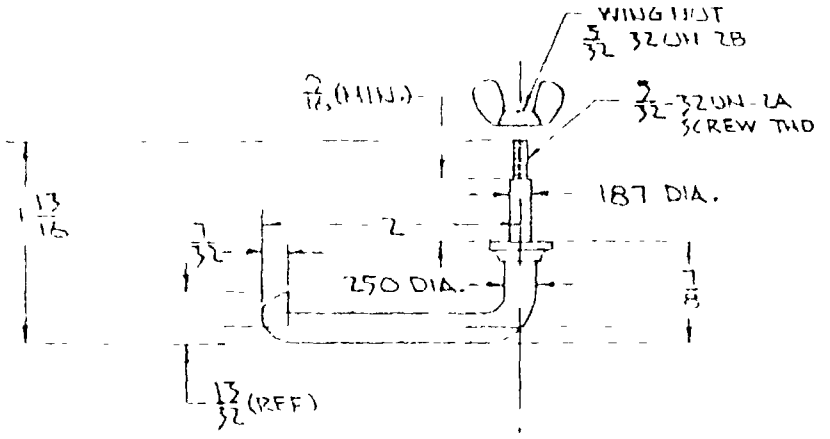

NSN 6515-00-392-0122

BLADE, LAMINECTOMY RETRACTOR, SCOVILLE, SINGLE HOOK, TYPE 1, SIZE 1

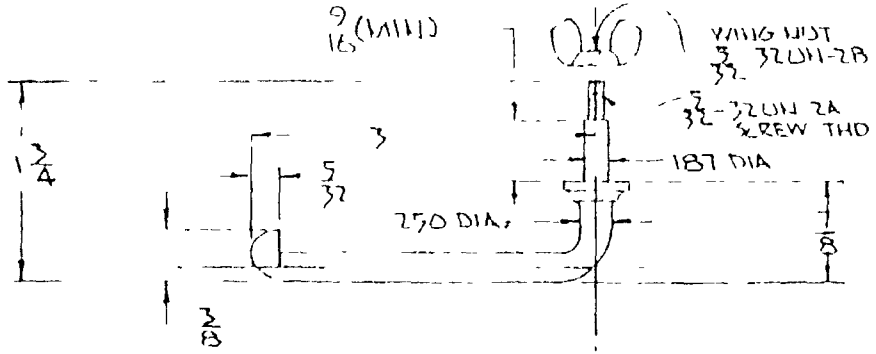

NSN 6515 00 392 0123

BLADE, LAMINECTOMY RETRACTOR, SCOVILLE, SINGLE HOOK, TYPE 1, SIZE 2

FIGURE 2


TOLERANCE NOTES

REMOVE BURRS AND BREAK ALL SHARP EDGES, UNLESS OTHERWISE SPECIFIED


UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES

UNLESS OTHERWISE SPECIFIED TOLERANCES ON FRACTIONS ± 1/32
DECIMALS ± .002
ANGLES ± 1°


Source: https://assist.dla.mil -- Downloaded: 2026/10-26T09:39Z
Check the source to verify that this is the current version before use.

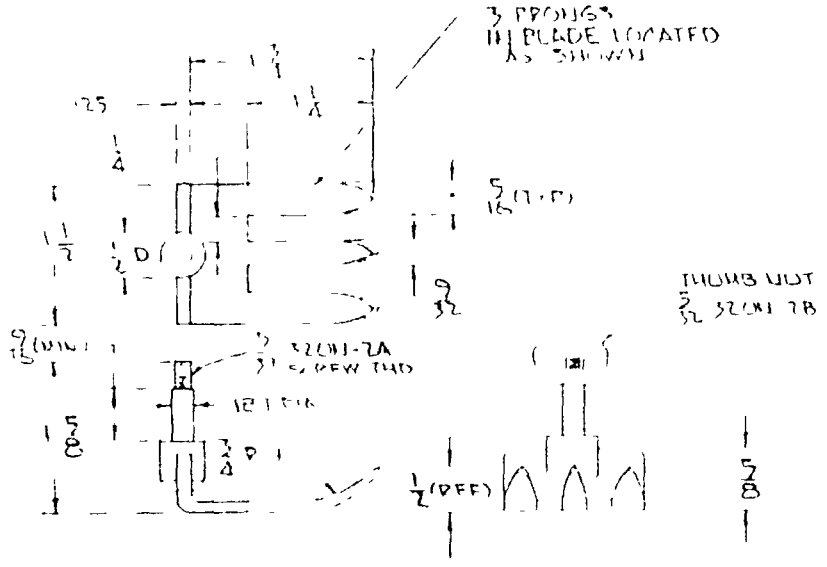

NSN 6515 00 379 4389
BLADE, LAMINECTOMY RETRACTOR, TAYLOR, TYPE II, SIZE 1

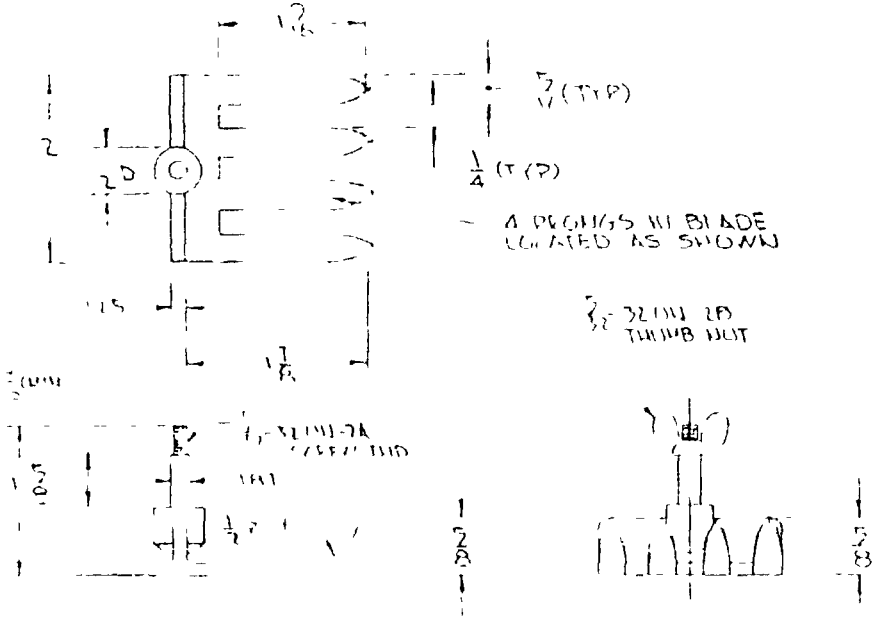

NSN 6515 00 376 7176
BLADE, LAMINECTOMY RETRACTOR, TAYLOR, TYPE II, SIZE 2

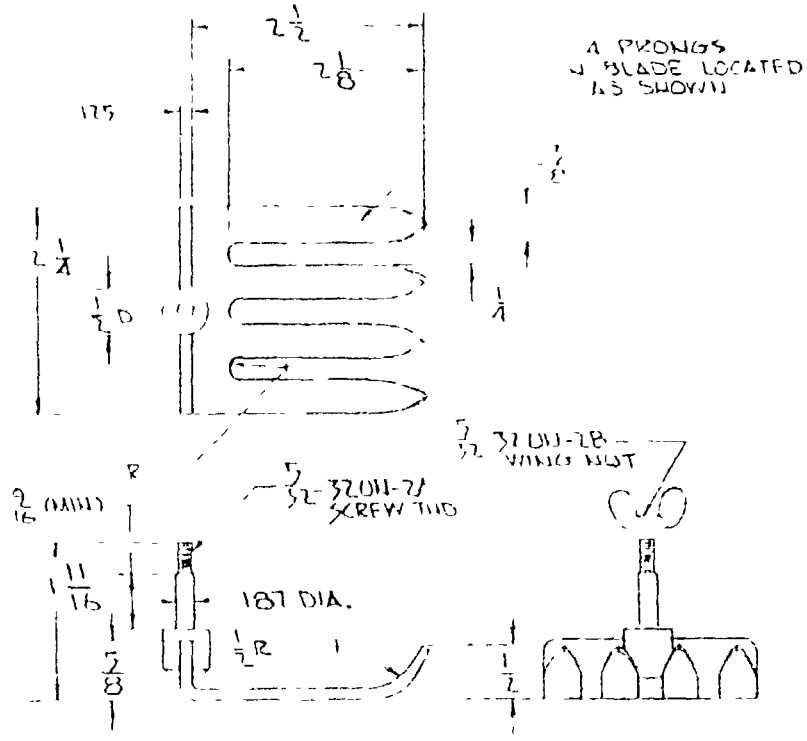


NSN 6515-00-376 7184
BLADE, LAMINECTOMY RETRACTOR, TAYLOR, TYPE II, SIZE 3

TOLERANCE NOTES
REMOVE BURRS AND BREAK ALL SHARP EDGES
UNLESS OTHERWISE SPECIFIED
UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
UNLESS OTHERWISE SPECIFIED
TOLERANCES ON FRACTIONS ± 1/32
DECIMALS ± .002
ANGLES ± 1°


FIGURE 3.

Source: https://assist.dla.mil -- Downloaded: 20260-26T09:39Z
Check the source to verify that this is the current version before use.

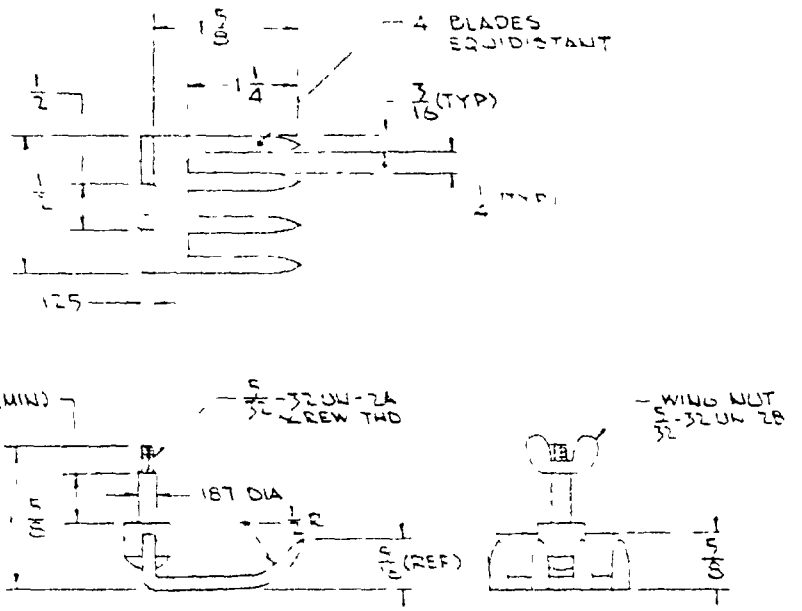

LSN 6515-00-376-7780

BLADE LAMINECTOMY RETRACTOR SCOVILLE 4 PRONG TYPE III SIZE 1

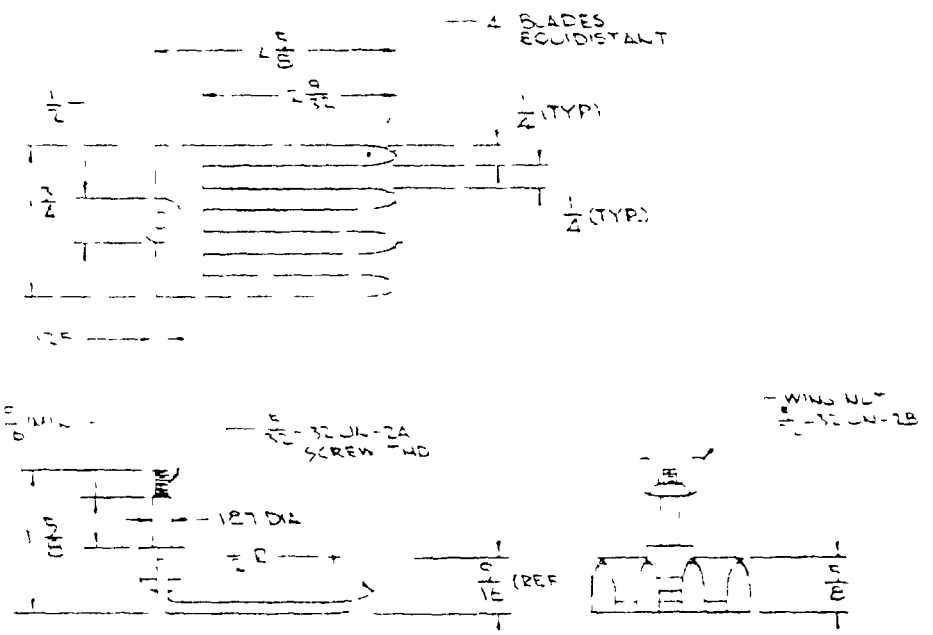


NSN 6515 00 355-3065

BLADE LAMINECTOMY RETRACTOR SCOVILLE 4 PRONG, TYPE III, SIZE 2

FIGURE 4

TOLERANCE NOTES
UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
UNLESS OTHERWISE SPECIFIED
FRACTIONS ± 1/32
DECIMALS ± .02
ANGLES ± 1°

Source: https://assist.dla.mil -- Downloaded: 2026-04-26T09:39Z
Check the source to verify that this is the current version before use.

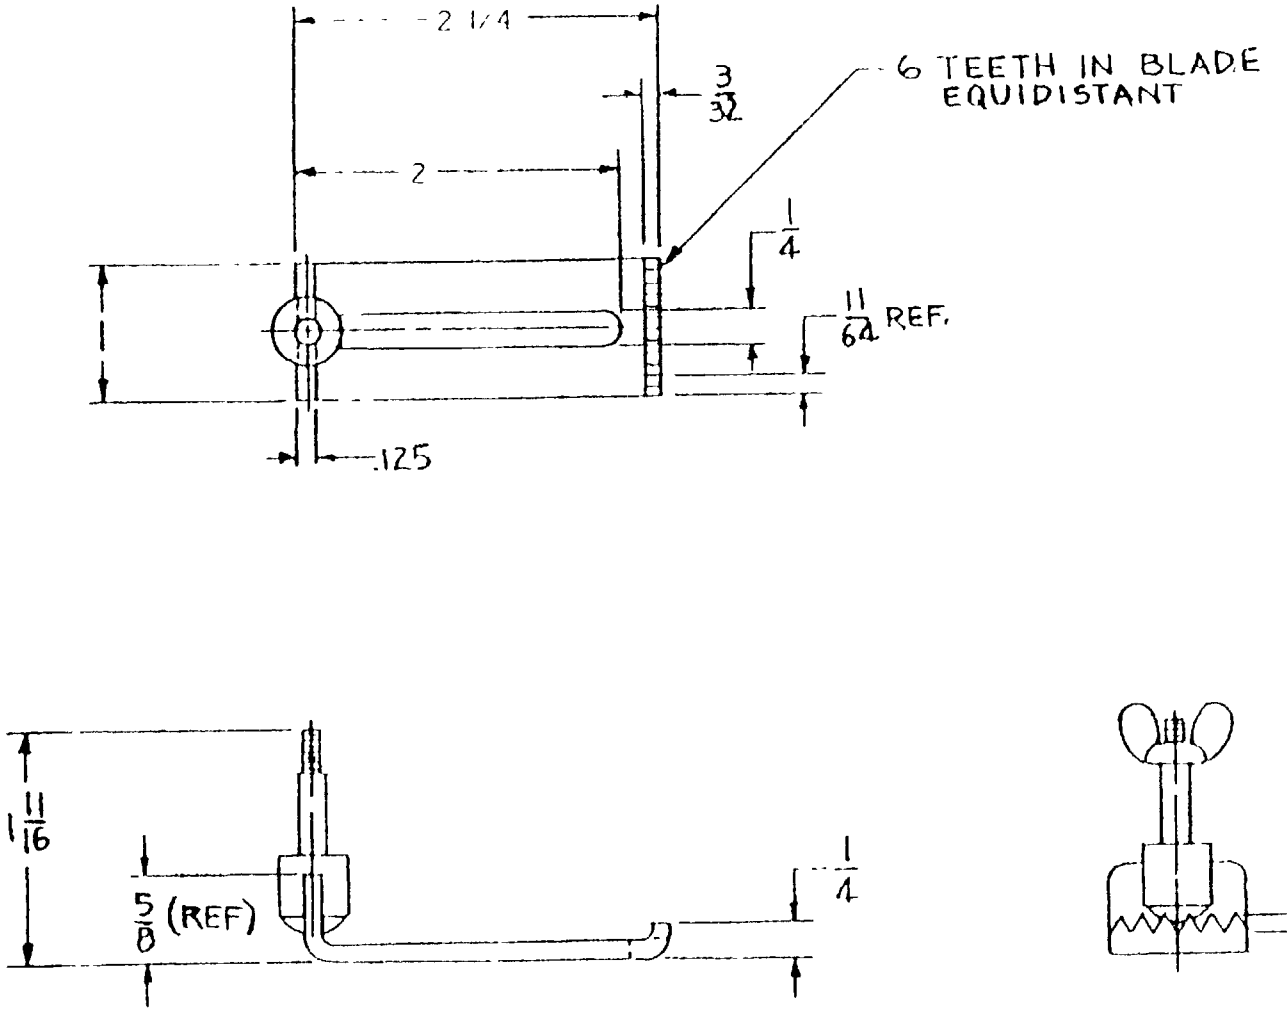


NSN 6515-00-385-3710

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES		
TOLERANCES ON:		
FRACTIONS	DECIMALS	ANGLES
± 1/32	± .002	± °

FIGURE 5 BLADE, LAMINECTOMY RETRACTOR, EPSTEIN, SINGLE PRONG, TYPE IV

Source: https://assist.dla.mil -- Downloaded: 2026/10-26T09:39Z
Check the source to verify that this is the current version before use.

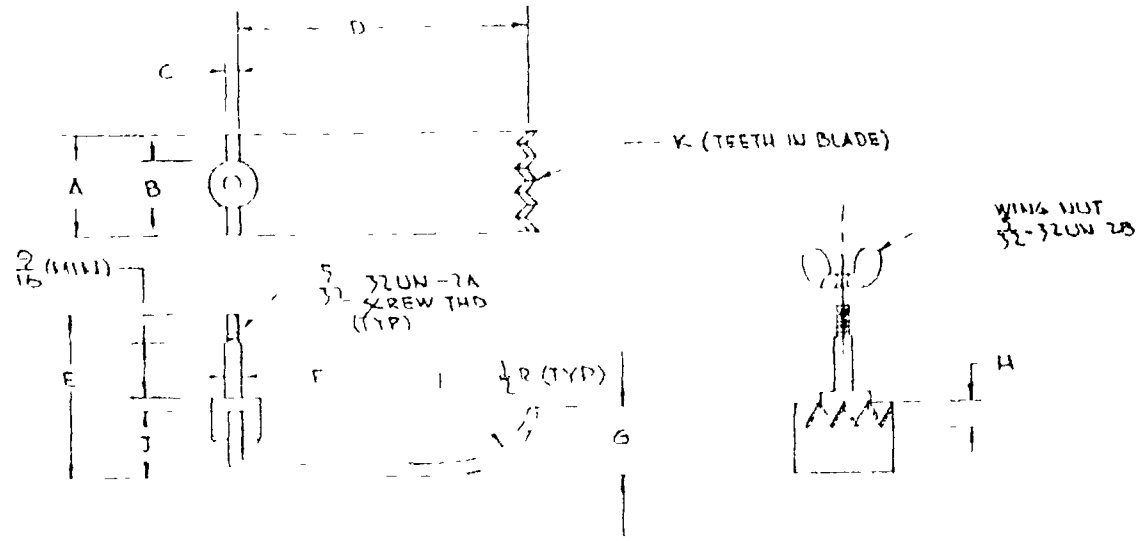


BLADE, LAMINECTOMY RETRACTOR, HIBBS, SINGLE PRONG, TYPE V

SIZE	NSN	DIMENSIONS									
		A	B	C	D	E	F	G	H	J	K
1	6515-00-385-3711	1	1/2 D	.125	2	1 5/8	.187 DIA	1/2	3/16	5/8	5
2	6515-00-385-3139	2"	1/2 D	.125	2	1 11/16	.187 DIA	1/2	3/16	5/8	9
3	6515-00-385-3140	1"	1/2 D	.125	3	1 13/16	.187 DIA	5/8	3/16	5/8	5
4	6515-00-385-3751	1"	1/2 D	.125	3	1 7/8	.187 DIA	1/2	3/16	5/8	8
5	6515-00-111-6383	1"	1/2 D	.125	4	1 11/16	.187 DIA	19/32	3/16	5/8	8

TOLERANCE NOTES
REMOVE BURRS AND BREAK ALL SHARP EDGES UNLESS OTHERWISE SPECIFIED
UNLESS OTHERWISE SPECIFIED
DIMENSIONS ARE IN INCHES.
UNLESS OTHERWISE SPECIFIED
TOLERANCES ON FRACTIONS ± 1/32
DECIMALS ± .002
ANGLES ± 5°

FIGURE 6

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

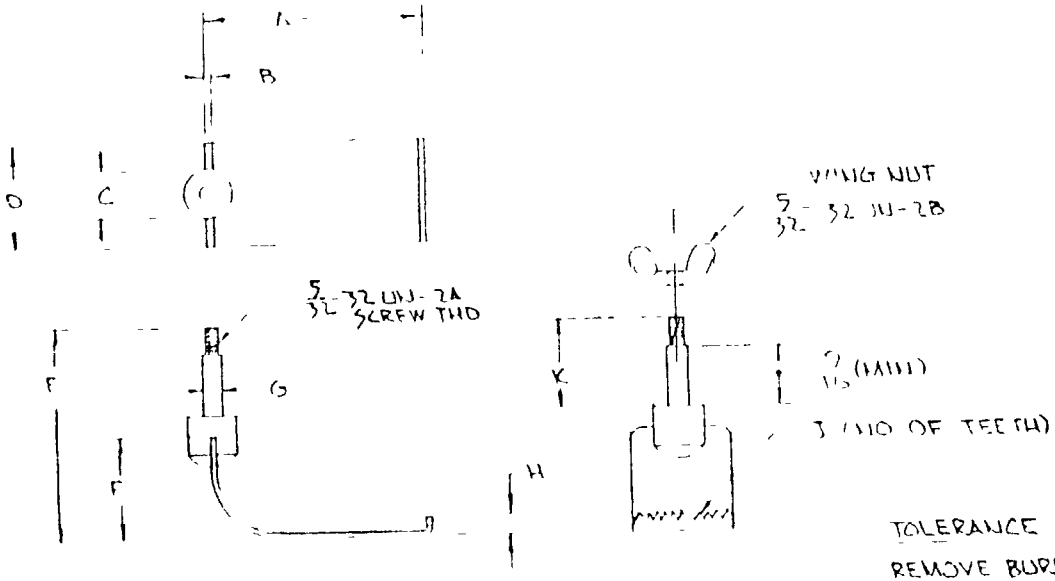

TOLERANCE NOTES

REMOVE BURRS AND BREAK ALL SHARP EDGES -- UNLESS OTHERWISE SPECIFIED
UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
UNLESS OTHERWISE SPECIFIED TOLERANCES ON FRACTIONS ± 1/32
DECIMALS ± .002
ANGLES ± 1°

SIZE	NSN	DIMENSIONS									
		A	B	C	D	E	F	G	H	J	K
1	6515-00-383-3283	2¼	.062	½D	1"	2⅛	1⅛6	3/16D	3/16	11	⅞
2	6515-00-383-3291	3	.062	½D	1"	2⅛	1⅛6	3/16D	3/16	11	⅞
3	6515-00-382-0124	3½	.062	½D	2"	2⅛	1⅛6	3/16D	3/16	22	⅞

BLADE, LARYNGOSCOPE, MAYERDING, SINGLE PRONG, TYPE VI

FIGURE 7

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1 The preparing activity must complete blocks 1, 2, 3, and 8 In block 1, both the document number and revision letter should be given

2 The submitter of this form must complete blocks 4, 5, 6, and 7

3 The preparing activity must provide a reply within 30 days from receipt of the form

NOTE This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER A-A-54823	2 DOCUMENT DATE (YYMMDD) 28 May 1993

3 DOCUMENT TITLE
RETRACTOR, HEMILAMINECTOMY, HAVERFIELD-SCOVILLE AND BLADES, INTERCHANGEABLE

4 NATURE OF CHANGE (*Identify paragraph number and include proposed rewrite if possible Attach extra sheets as needed*)

5 REASON FOR RECOMMENDATION

6 SUBMITTER

a NAME (Last, First, Middle Initial)	b ORGANIZATION	
c ADDRESS (Include Zip Code)	c TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7 DATE SUBMITTED (YYMMDD)

8 PREPARING ACTIVITY

a NAME	b TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON
c ADDRESS (Include Zip Code)	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike Suite 1403 Falls Church VA 22041 3466 Telephone (703) 756 2340 AUTOVON 289 2340

DD Form 1426, OCT 89 *Previous editions are obsolete*

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:39Z
Check the source to verify that this is the current version before use.