A-A-54538
20 December 1991

COMMERCIAL ITEM DESCRIPTION

INJECTOR, TUBE, Plastic, Reusable

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a plastic medical cartridge injector suitable for use with 1 or 2 ml cartridge-needle units.

Salient characteristics:

General. The injector shall be a cartridge injector which is top-loading and clamps to the proximal end of the cartridge-needle unit by means of a collet mechanism comprised of a ribbed collar and splines attached to a finger guard. By unscrewing the collar, the cartridge-needle unit can be discarded without touching it.

Material. The injector shall be made of polycarbonate or Acrylonitrile Butadiene Styrene (ABS) plastic or combinations of the two plastics. The type of the plunger shall be made of austenitic stainless steel type 303, 304, or 316 in accordance with ASTM Designation F899 or brass which has been nickel or chromium-over-nickel plated.

Style, design and dimensions. The cartridge injector shall consist of a plunger with threaded tip and round thumb rest, a ribbed collar, and a threaded finger grip. The injector shall accommodate 1 or 2 ml cartridge-needle units having an 11/32 inch outside diameter (See Note 2). The injector shall be designed so that the plunger can not be withdrawn completely. The plunger tip shall be attachable to the screw of the rubber piston or plug in the cartridge-needle unit. The finger grip shall be threaded to allow the cartridge-needle unit to be clamped within the collar. Inside the splines shall be a band of elastomeric material to enhance grip on the cartridge-needle unit. The overall length of the injector shall be 4-1/2 to 5 inches. The injector assembly shall have adequate mechanical strength to move the cartridge piston or plug without undergoing any distortion. The ribbed collar shall have "open" and "close" and the appropriate directional arrow printed on it. The injector shall be in accordance with Figure I.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:35Z
Check the source to verify that this is the current version before use.

Instructions. The injector shall be provided with instructions for use.

Workmanship. Workmanship shall be first class throughout. The injector shall be free from incorrect thread size, inoperable plunger, crazing or cracking, non-rigid construction, presence of rough or sharp edges, presence of foreign matter, lack of instructions and any defects which detract from its appearance or impairs its serviceability.

Unit. Each (EA). One injector tube, as specified, constitutes one unit.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and as specified herein. Unit of product for examination purposes shall be one injector. Sampling shall be Inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:35Z
Check the source to verify that this is the current version before use.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for test purposes shall be one injector. Sampling shall be Inspection level S-2 with an AQL of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more text characteristics.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the lastet revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the products is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction , the offeror/contractor shall comply, and be responsible for compliance by its subcontractors suppliers, with the requirements of the Federal Food, Drug Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal State, and local statutes, ordinances, and regulations.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:35Z
Check the source to verify that this is the current version before use.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and /or order.

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

NOTE 1: The following National Stock Number and its Item Identification is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-344-8487	INJECTOR, TUBE, Plastic Reusable, Each

NOTE 2: The National Stock Number for one such cartridge-needle unit is 6505-00-058-6590 (Heparin, Sodium, Injection, USP).

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

PGC 62535

Project No. 6515-4778
Location: AA54538/S11
Disk 1

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:35Z
Check the source to verify that this is the current version before use.

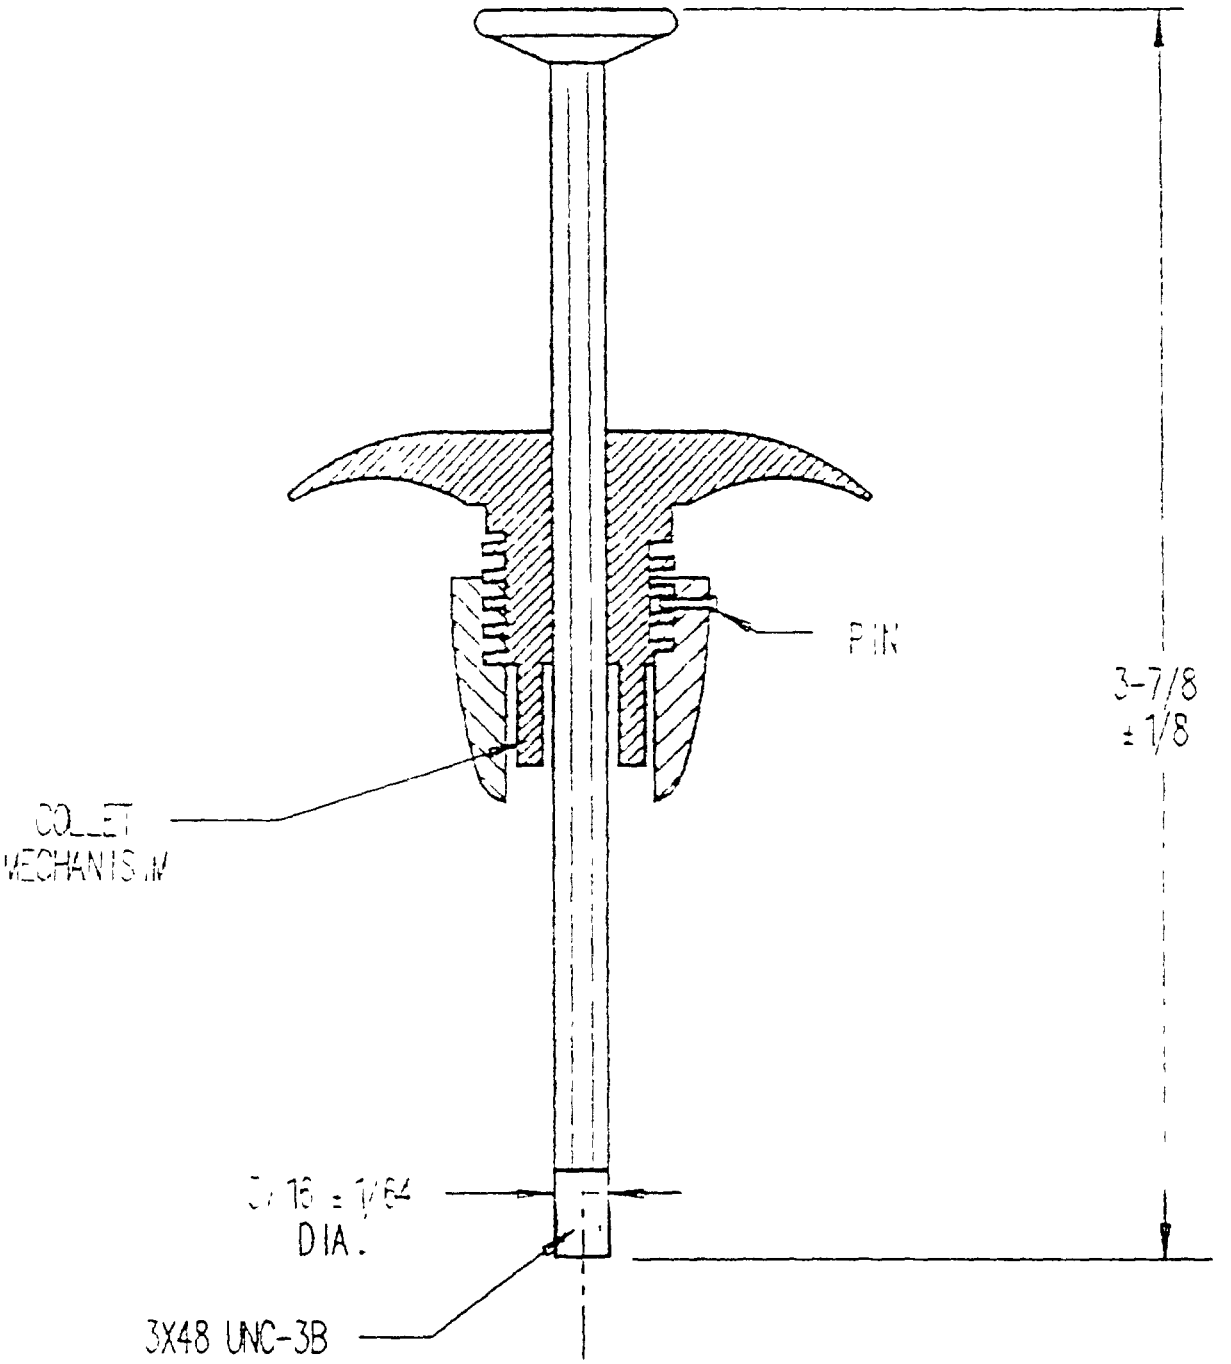


FIGURE 1. INJECTOR TUBE, PLASTIC, REUSABLE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:35Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8 In block 1, both the document number and revision letter should be given
2. The submitter of this form must complete blocks 4, 5, 6, and 7
3. The preparing activity must provide a reply within 30 days from receipt of the form

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER A-A-54538	2 DOCUMENT DATE (YYMMDD) 20 December 1991

3 DOCUMENT TITLE
INJECTOR, TUBE, Plastic, Reusable

4 NATURE OF CHANGE (Identify paragraph number and include proposed rewrite if possible Attach extra sheets as needed.)

5 REASON FOR RECOMMENDATION

6 SUBMITTER

a NAME (Last, First, Middle Initial)	b ORGANIZATION	
c ADDRESS (Include Zip Code)	d TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7 DATE SUBMITTED (YYMMDD)

8 PREPARING ACTIVITY

a NAME Defense Personnel Support Center ATTN: DPSC-MSE	b TELEPHONE (Include Area Code) (1) Commercial (215)7372870	(2) AUTOVON 444-2870
c ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

DD Form 1426, OCT 89 Previous editions are obsolete '98/290

Source: https://assist.dla.mil - Downloaded: 2024-10-26T09:35Z
Check the source to verify that this is the current version before use.