A-A-0051712(DM)
9 October 1986

INTERIM COMMERCIAL ITEM DESCRIPTION

TONGS, SKULL TRACTION, GARDNER-WELLS

The General Services Administration has authorized the use of this interim commercial item description which was developed by the Defense Personnel Support Center, Directorate of Medical Materiel, DPSC-RST, 2800 South 20th Street, Philadelphia, PA, 19101, based upon currently available technical information.

This interim commercial item description covers skull tongs of the Gardner-Wells design.

Salient characteristics.

Style and design. The skull tongs shall be of the Gardner-Wells design and suitable for traction and/or immobilization of the cervical spine.

The style shall be that of a half circle bar to partially encompass the head. One end of the bar shall have a spring loaded point for insertion into the skull. Screws shall have sharp needle points. The points shall have a small diameter hollow rod for protection, and in their maximum open position shall be 6-1/4 inches (16 cm). The design and dimensions shall comply with Figure 1.

Securely attached to the bar shall be an S-shaped hook plate for the attachment of weights. The plate shall be legibly marked with instructions for antiseptic wipe of both screws and skull. The plate shall also be marked to tighten the screws until proper set force exists. The screws shall have a means of locking them in the set position.

Material. The complete instrument shall be manufactured from class 3 austenitic corrosion-resisting steel as specified in American Society for Testing and Materials (ASTM) Standard F899.

Hardness. The complete instrument shall be properly passivated and have a hardness range of Rockwell B-75 to B-100.

Finish. The instrument shall have a mirror or satin finish. Screws shall have knurled handles.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

Corrosion resistance. The complete instrument shall be capable of withstanding repeated sterilization with steam or ethylene oxide. No signs of corrosion shall be evident after 10 hours of soaking in high level disinfectant solution, nor shall signs of corrosion be evident after remaining submerged 24 hours after a 30 minute boil in distilled water.

Workmanship. The skull tongs shall be free from defects which detract from its appearance or impair its serviceability. The skull tongs shall be without rough edges, burrs, cracks, pits, dents and corrosion.

Unit. Each (EA). One skull tongs, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. The skull tongs shall be examined to determine compliance with specification requirements. Sampling shall be in accordance with MIL-STD-105, sampling level II, AQL 2.5.

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:00Z
Check the source to verify that this is the currenversion before use.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one skull tongs. Sampling shall be at an inspection level of S-2 with an AQL of 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-125-6616	TONGS, SKULL TRACTION, GARDNER-WELLS

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-3908

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

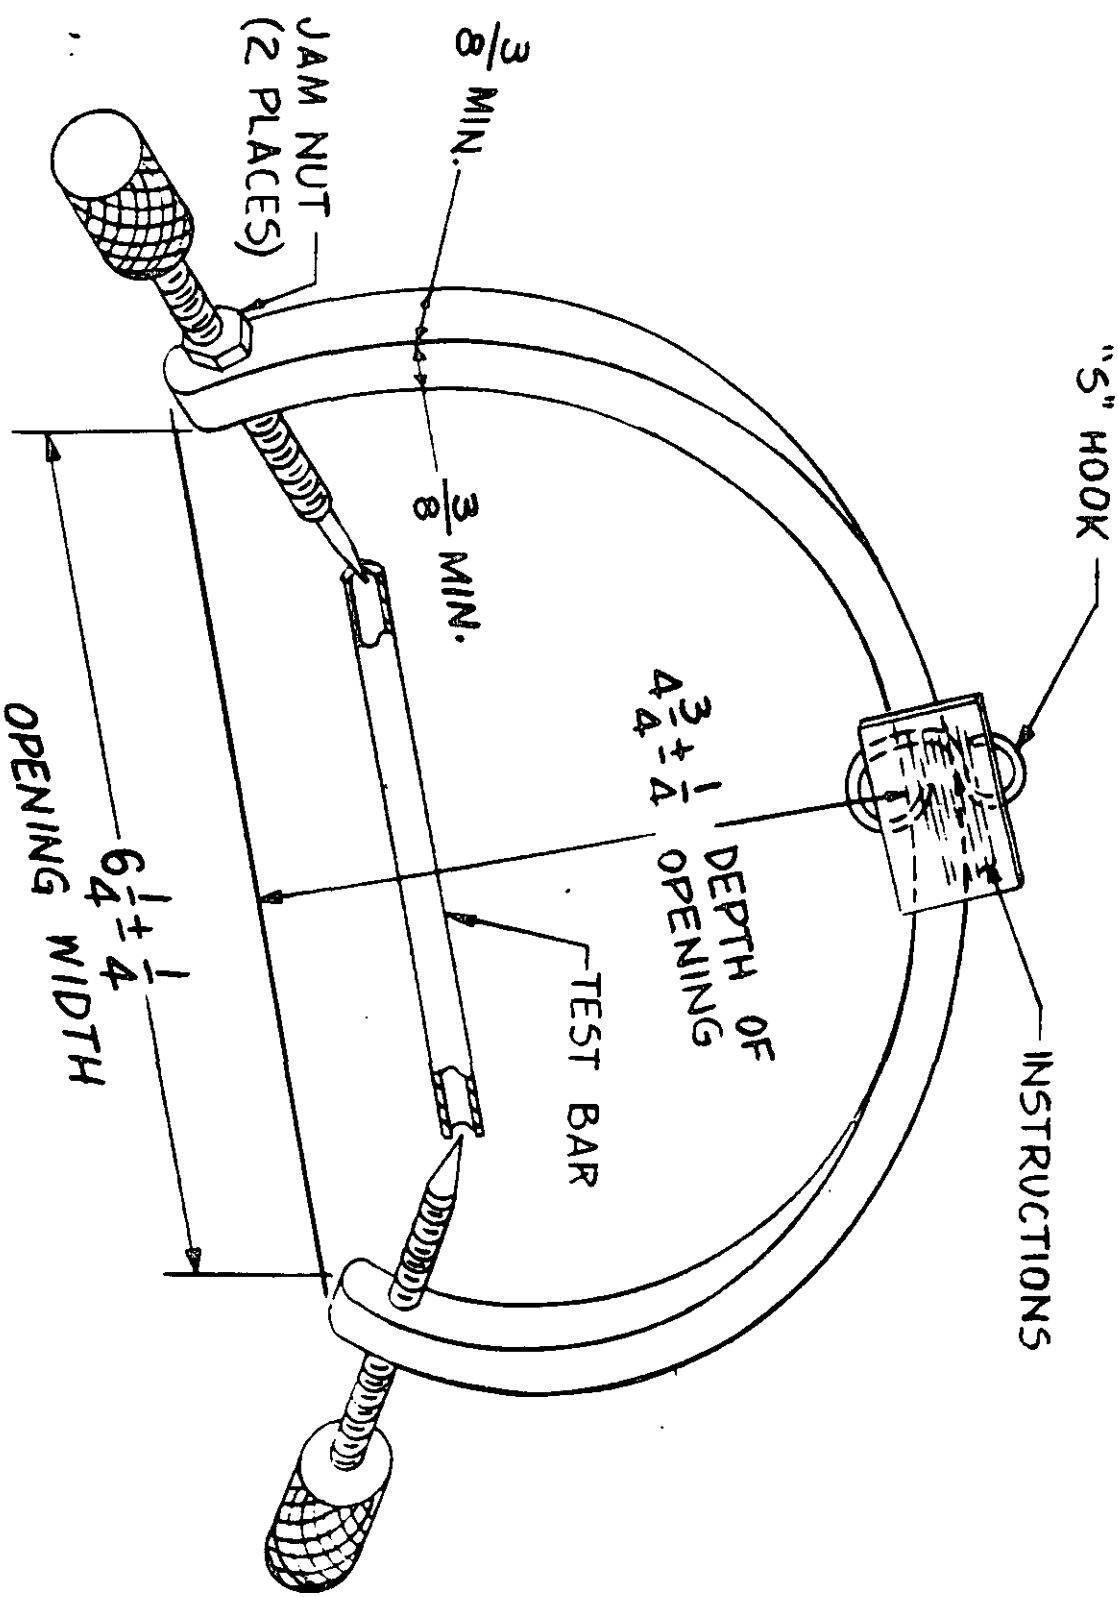


FIGURE 1. TONGS, SKULL TRACTION

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.