A-A-51724
27 October 1986

COMMERCIAL ITEM DESCRIPTION

CARRIER, SUTURE WIRE (RUSH)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers Rush suture wire carriers for use in placing wire suture during orthopedic surgical procedure.

Salient characteristics:

General. The Rush suture carriers shall be designed to place wire sutures around comminuted fractures during orthopedic surgical procedures. This specification covers suture wire carriers with loop diameters of 15/16, 1-1/4 and 2 inches.

Material. The Rush wire carrier shall be fabricated from class 4 martensitic stainless steel in accordance with ASTM F899. The Rockwell hardness shall be C-38 to C-45 when tested in accordance with ASTM E18. The handle shall be fabricated from aluminum or other suitable metal.

Characteristics. The Rush wire carrier shall have a loop at the distal end for reaching around the bone. There shall be a hole at the distal end to allow threading of the suture wire. The rush wire carrier shall meet the dimensional requirements indicated in Figure 1. The handle design shall provide a secure grip. The entire carrier shall be capable of repetitive steam sterilization at temperatures up to 275°F.

Corrosion testing. The Rush wire carrier shall meet the copper sulfate and boil test requirements as specified in Federal Specification GG-I-526.

Identification marking. The Rush wire carrier shall bear the name or registered trademark of the manufacturer and the word "stainless." In addition, instruments of foreign manufacture shall bear the name of the country of manufacture.

Passivation. Material used in the fabrication of the mallet shall be passivated, if required.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

Workmanship. Each Rush wire shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One suture wire carrier, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105. The unit of product for test purposes shall be one suture wire carrier. AQL shall be 1.0 percent defective. Inspection level shall be S-2.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE 1: The following National Stock Numbers are covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-139-7954	CARRIER, SUTURE WIRE, 15/16 Inch Loop Diameter
6515-01-139-7955	CARRIER, SUTURE WIRE, 1-1/4 Inch Loop Diameter
6515-01-139-7956	CARRIER, SUTURE WIRE, 2 Inch Loop Diameter

Ordering data (Interior/exterior package quantities and labeling and marking must be specified in the contract and/or order.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

COMMERCIAL ITEM DESCRIPTION A-A-51724

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM


CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

PGC SF015

Project No. 6515-3696

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

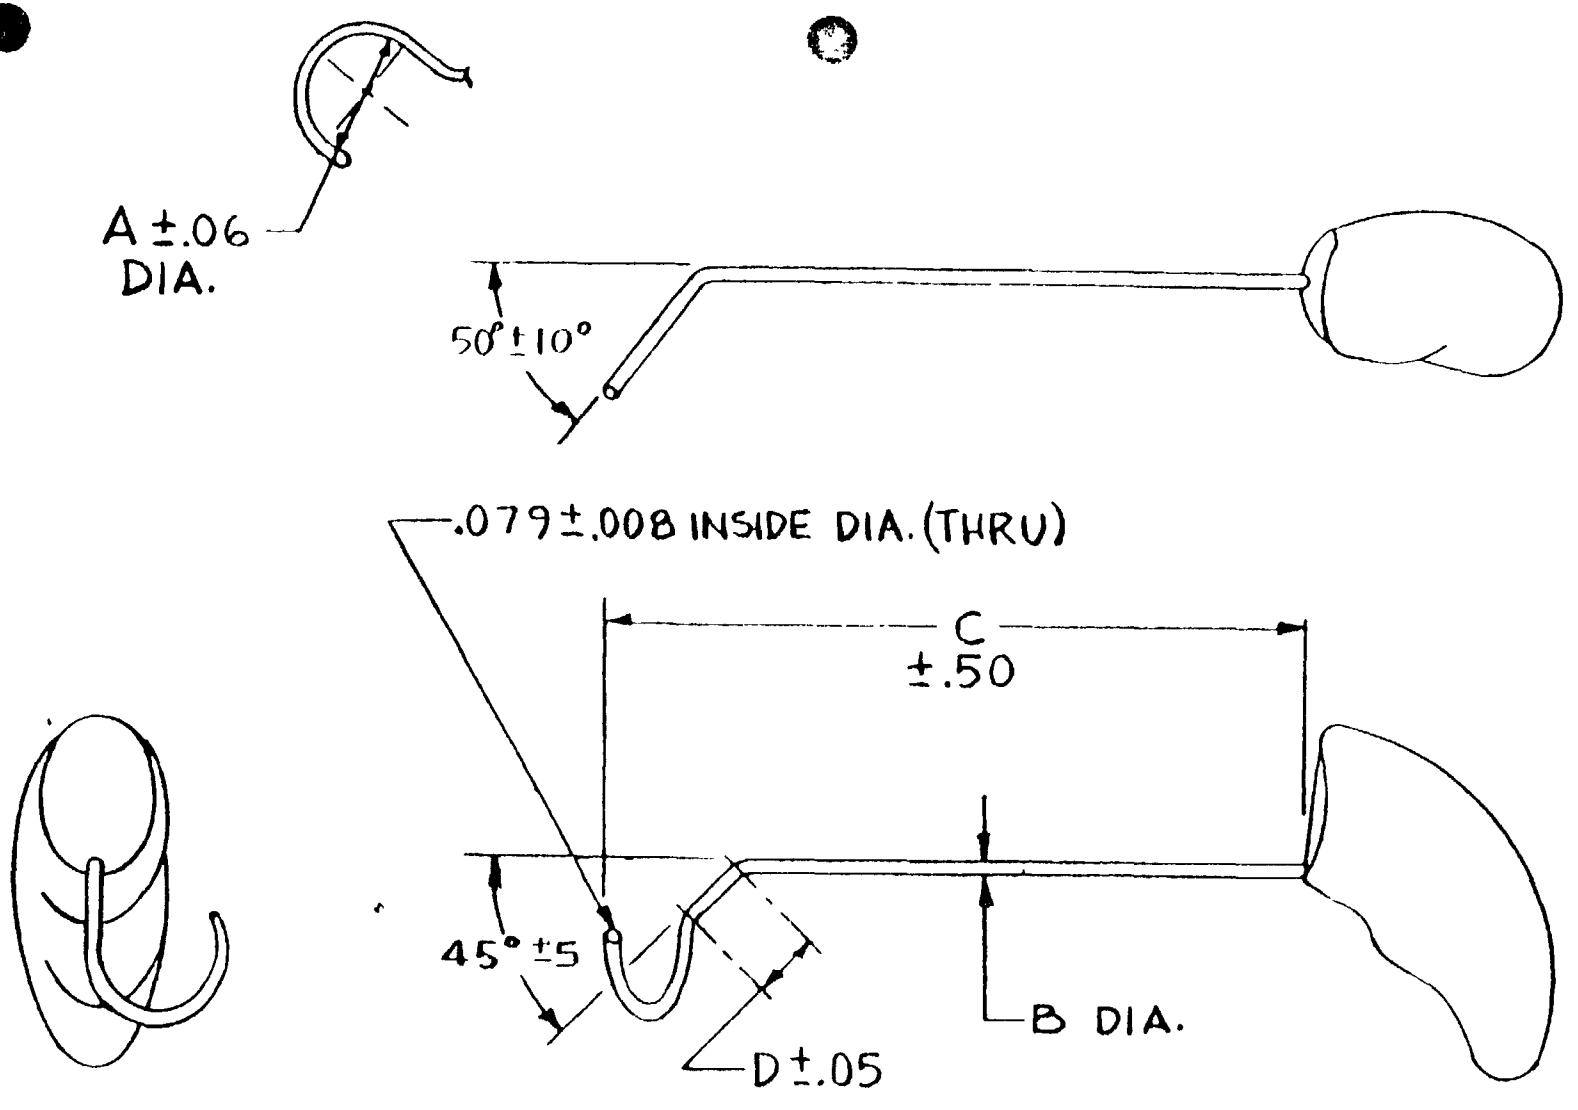

NOTE:
ALL DIMENSIONS IN INCHES.

NSN	A	B	C	D
6515-01-139-7954	.94	.120	5.50	.37
6515-01-139-7955	1.26	.177	6.61	.50
6515-01-139-7956	2.00	.177	8.27	.50

FIGURE 1 CARRIER, SUTURE WIRE, RUSH

Source: https://assist.dla.mil - Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 6, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE. This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
Attn: DPSC-STS
2800 South 20th Street
Philadelphia, PA 19101

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-51724	CARRIER, SUTURE WIRE (RUSH)

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ USER
	☐ MANUFACTURER
	☐ OTHER *(Specify)* _____

5. PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.