A-A-51742A
27 June 1988
SUPERSEDING
A-A-0051742(DM)
10 November 1986

COMMERCIAL ITEM DESCRIPTION

DRILL, HAND, BONE (Bunnell)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a Bunnell bone hand drill suitable for use in orthopedic surgical procedures.

Salient characteristics.

Style and design. Style, design and dimensions of the drill shall be in accordance with Figure 1.

Components. Components of the drill shall be in accordance with the following:

Handle. The handle shall have a nominal width of 1-1/4 inches and nominal thickness of 3/4 inch. The handle shall be contoured for a comfortable grip and possess no sharp edges. The handle shall be fabricated of aluminum.

Chuck key. The chuck key shall be able to be secured into the underside of the handle so as not to interfere with the operation of the drill or hands of the surgeon. The chuck key shall have teeth to mate with the chuck. The chuck key shall be able to open and close the jaws of the chuck completely. The chuck key shall be fabricated of Class 4 martensitic corrosion-resistant steel in accordance with ASTM Designation F899 and shall have a Rockwell Hardness C Scale (HRC) 35, minimum. The chuck key shall be marked "stainless".

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

Chuck. The chuck shall be a 3-jaw, Jacobs type chuck capable of accepting bone pins and drills having diameters up to and including 5/32 inch. The chuck shall be cannulated to accept 3/32 inch diameter pins and shall mate with the teeth of the chuck key. The chuck shall be permanently secured to the shaft. The chuck shall be fabricated of Class 4 martensitic corrosion-resistant steel in accordance with ASTM Designation F899 and shall have a Rockwell Hardness C Scale (HRC) 35, minimum. The finish of the chuck shall be mirror or mirror and satin. The chuck shall be marked "stainless."

Shaft. The shaft shall be cannulated to accept 5/64 inch diameter pins. The shaft shall be permanently attached to the chuck. A shaft collar shall be affixed to the shaft to restrict shaft movement along the centerline of the shaft but not to impede its rotation around its axial centerline. The shaft shall be fabricated of Class 3 or Class 4 corrosion-resistant steel in accordance with ASTM Designation F899 and shall have a Rockwell Hardness C Scale (HRC) 25, minimum.

Gear assembly. The gear assembly shall operate smoothly and continuously when hand-rotated by the knob. Gears shall be fabricated of Class 3 or Class 4 corrosion-resistant steel in accordance with ASTM Designation F899. As an alternate, gears shall be fabricated of nickle-chrome plated brass. The screw that extends down through the threaded hole shall be short enough so as not to come in contact with the shaft.

Guard-brackets. The guard-brackets shall be mounted on both sides of the handle and shall protect the gears. The guard-brackets shall be fabricated of a corrosion-resistant steel.

Knob. The knob shall be free to rotate on its spindle. The spindle shall be connected to a handpiece which in turn shall be connected to the gears. The knob shall be fabricated of aluminum.

Trigger. The trigger shall be able to stop or release gear rotation instantly. The trigger shall be fabricated of Class 3 austentic corrosion-resistant steel in accordance with ASTM Designation F899.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

Sterilization. The hand drill shall be capable of withstanding repeated sterilization via steam, ethylene oxide, or long-term, 10 hour soaking in cold sterilization solution. The hand drill shall show no evidence of corrosion when autoclaved as follows:

The drill shall be cleaned and placed in an autoclave. The drill shall then be autoclaved at 270 ± 5 degrees F of a minimum of 5 minutes. Upon removal of drill from autoclave, the entire surface area of the drill shall be examined for evidence of corrosion.

Workmanship. The hand drill shall be free from defects which detract from its appearance or impair its serviceability.

PRODUCT QUALITY LEVEL.

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Each (EA). One hand drill, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical prope).

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105. The acceptable quality level (AQL) shall be 1.0 for an inspection level of S-2. The unit of product for test purposes shall be one hand drill.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-060-1641	DRILL, HAND, BONE, Bunnell

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM


Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

A-A-51742A

CIVIL AGENCY COORDINATING ACTIVITIES:
VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4283

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

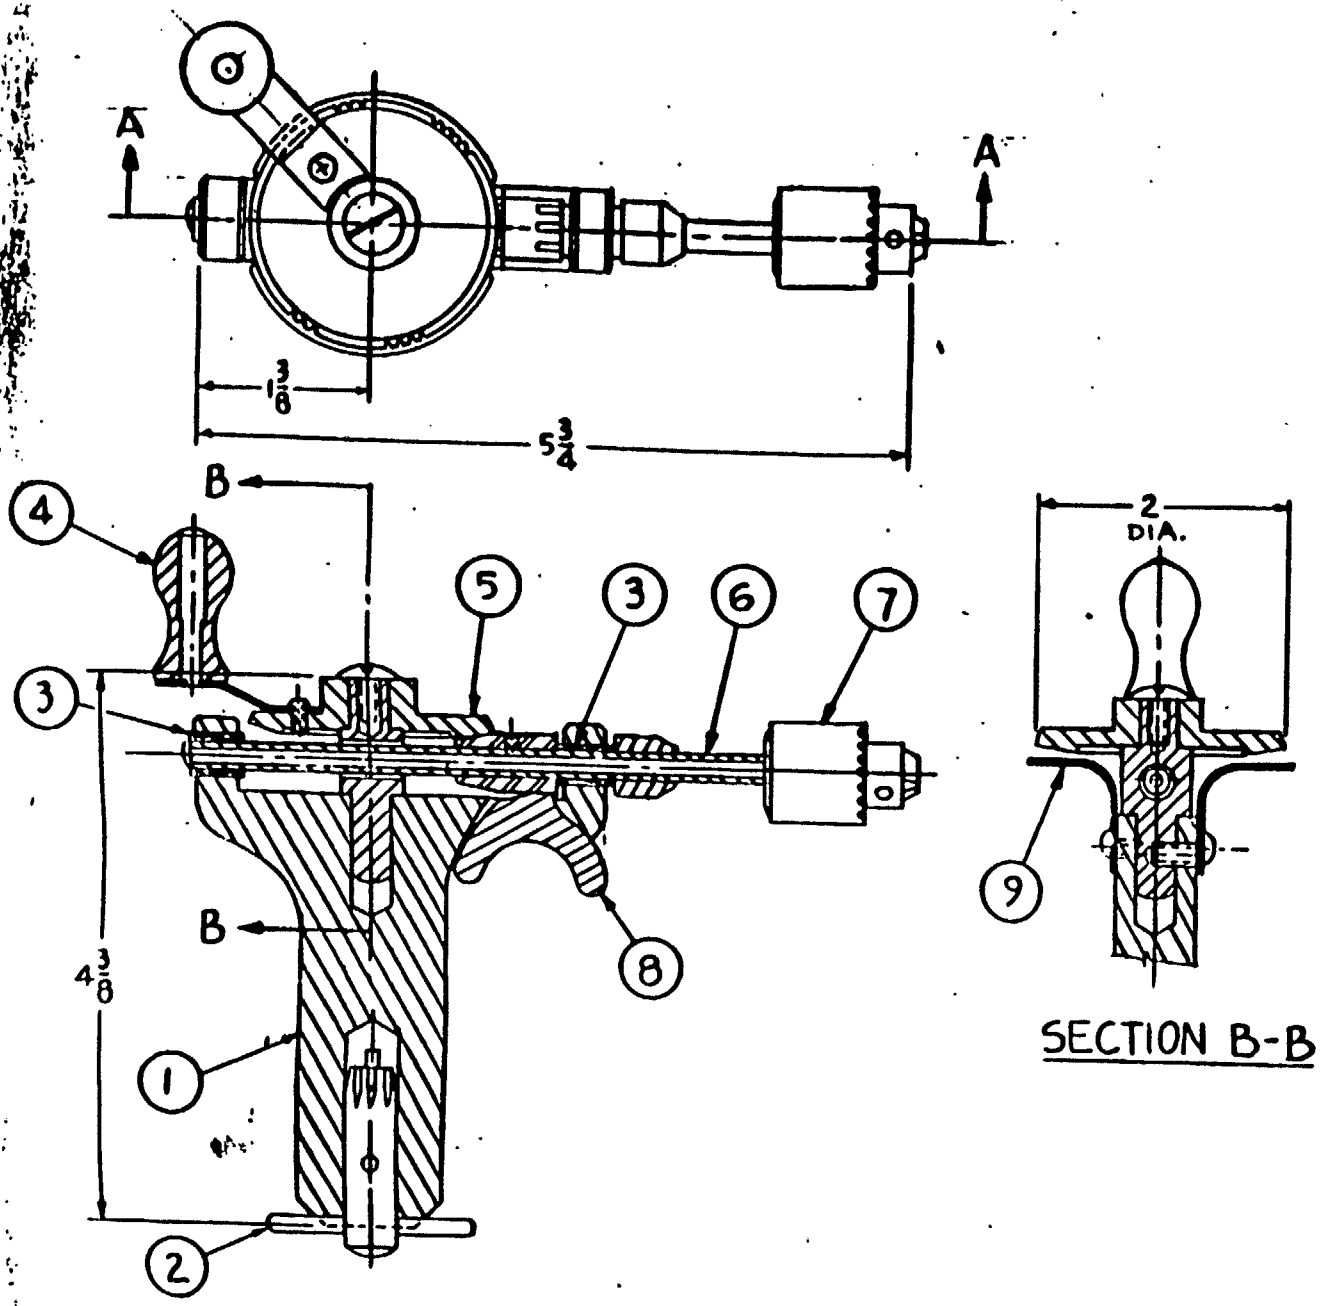

ITEM	QTY	DESCRIPTION
1	1	HANDLE
2	1	CHUCK KEY
3	2	BUSHING
4	1	KNOB
5	1	GEAR ASSEMBLY
6	1	SHAFT
7	1	JACOBS CHUCK
8	1	TRIGGER
9	2	BRACKET

FIGURE 1 DRILL, HAND, BONE, BUNNEL

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.