A-A-51549
15 July 1986

COMMERCIAL ITEM DESCRIPTION

DILATOR SET (BAKES)

The General Services Administration has authorized the use of this commercial item description in preference to Military Specification MIL-D-37371 dated 2 January 1976.

This commercial item description covers a set of nine Bakes-design common bile duct dilators, sizes 3 mm to 11 mm.

Salient characteristics:

General. Shall be a set of nine (9) common bile duct dilators in a folding canvas case. Dilators shall conform to the requirements listed below.

Specific requirements.

Material. Dilators shall be fabricated from Class 3, Type 302, 303, or 304 steel conforming to ASTM F899.

Style and design. Shall be Bakes-design common bile duct dilators. Style and design of the dilators shall conform to Figure 1. Dilators shall be supplied in 3, 4, 5, 6, 7, 8, 9, 10 and 11 millimeter sizes.

Physical and Chemical Properties.

Hardness. The shaft portion of the dilators shall have a minimum Rockwell hardness of B25 when tested as specified in GG-I-526.

Corrosion-resistance. Dilators shall pass the Boil test specified in GG-I-526.

Identification marking. Dilators shall comply with the marking requirements of GG-I-526. Dilator size shall be embossed on the handle of each dilator. Dilators of foreign manufacture shall be marked with the legend "stainless."

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:57Z
Check the source to verify that this is the current version before use.

Finish. Dilator tips shall have a mirror finish. Dilator shafts and handles shall have a mirror or satin finish.

Workmanship. Dilators shall be free from nicks, dents, burrs, sharp edges, corrosion, and any other defects that detract from their appearance or impair their serviceability.

Unit. Set (SE). One dilator set, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Inspection shall be conducted at level II, AQL (Acceptable Quality Level) 1.0 percent. The unit of product for test purposes shall be one set.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:57Z
Check the source to verify that this is the current version before use.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: This document covers the following National Stock Number (NSN):

NSN	ITEM IDENTIFICATION
6515-00-325-2800	DILATOR SET, Common Bile Duct, Bakes, Set of 9

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:57Z
Check the source to verify that this is the current version before use.

COMMERCIAL ITEM DESCRIPTION A-A-51549

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:.

DoD-MB

Agent:

DLA-DM


CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS

PGC 45218

Project No. 6515-3579

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:57Z
Check the source to verify that this is the current version before use.

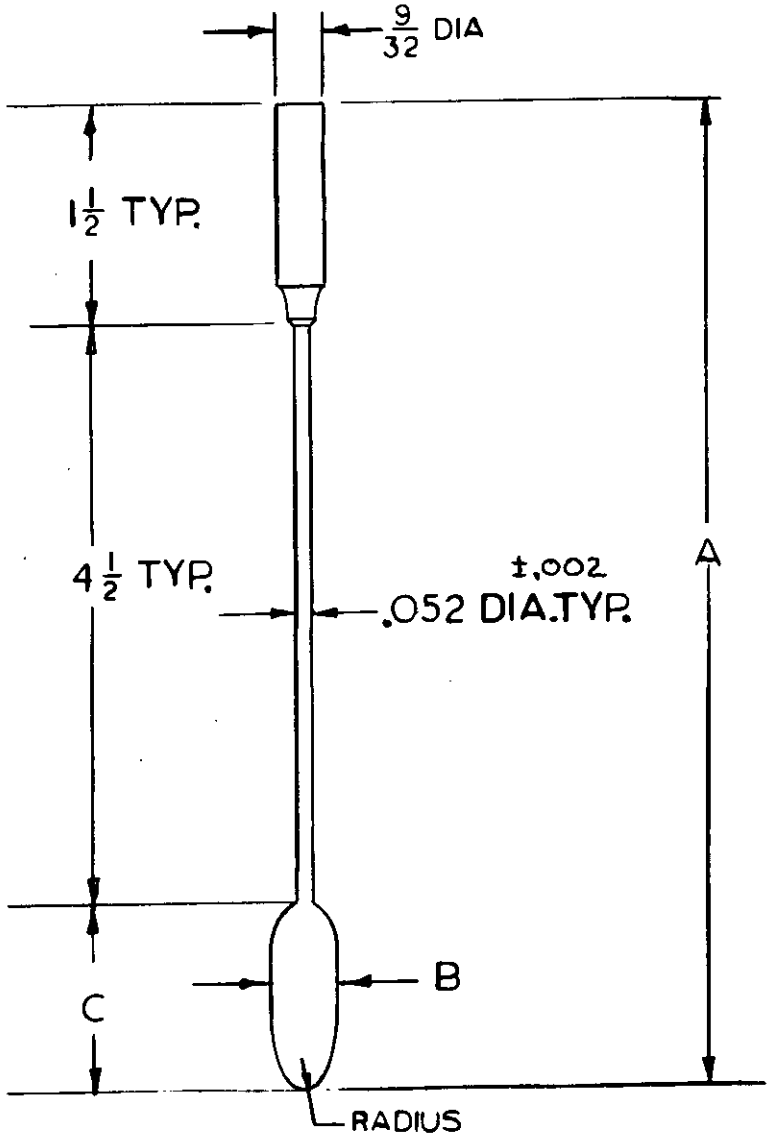

SIZE	"A"	"B" DIA	"C"
3 MM	6-11/16	1/8	11/16
4 MM	6-13/16	5/32	11/16
5 MM	6-7/8	3/16	13/16
6 MM	7	1/4	15/16
7 MM	7	9/32	31/32
8 MM	7-1/8	5/16	31/32
9 MM	7-5/16	3/8	1-1/4
10 MM	7/3 8	13/32	1-3/8
11 MM	7-7/16	7/16	1-7/16
TOLERANCE	± 1/32	± 1/64	± 1/16

DIMENSIONS IN INCHES

FIGURE 1. Dilator set, common bile duct, bakes, set of 9

Source: https://assist.dla.mil -- Downloaded: 202610-26T08:57Z
Check the source to verify that this is the current version before use.