A-A-51557A
10 July 1989
SUPERSEDING
A-A-0051557 (DM)
28 July 1986

COMMERCIAL ITEM DESCRIPTION

KNIFE-ELEVATOR (Paparella)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a knife-elevator of the Paparella design suitable for surgical procedures on the ear canal.

Salient characteristics:

Style and design. The knife-elevator shall be of the Paparella design with a duckbill distal end suitable for incising and elevating canal skin. The handle shall be round etched to facilitate a sure grip. The design and dimensions shall comply with Figure 1.

Material. The knife-elevator shall be manufactured from Class 3 austenitic corrosion-resisting steel as specified in ASTM Designation F899.

Hardness. The knife-elevator shall have a Rockwell Hardness B scale (HRB) of 75 to 100 when tested in accordance with ASTM Designation E18. Conversion of hardness values shall be in accordance with ASTM Designation E140.

Finish. The knife-elevator shall have a mirror or satin finish.

Passivation. The knife-elevator shall be passivated after completion of all fabricating and finishing operations.

Corrosion-resistance. The knife-elevator shall show no signs of corrosion when tested as specified in ASTM Designation F1089.

AMSC N/A FSC 6515
DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:57Z
Check the source to verify that this is the current version before use.

Identification markings. The elevator-knife shall bear the name or registered trademark and the word "stainless". Elevators of foreign manufacture shall bear the name of the country of manufacture.

Workmanship. The knife-elevator shall be free from defects which detract from its appearance or impair its serviceability. The knife-elevator shall be without rough edges, burrs, cracks, pits, dents and corrosion.

Unit. Each (EA). One knife-elevator, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. The knife-elevator shall be examined to determine compliance with specification requirements. Sampling shall be in accordance with MIL-STD-105, sampling level II, AQL 2.5.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:57Z
Check the source to verify that this is the current version before use.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one knife-elevator. Sampling shall be at an inspection level of S-2 with an AQL of 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 202610-26T08:57Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-139-8338	KNIFE-ELEVATOR, Paparella, Duckbill, 6-1/2 Inch (16.5 cm), Each

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

PGC 53359

Project No. 6515-4566

Source: https://assist.dla.mil -- Downloaded: 202610-26T08:57Z
Check the source to verify that this is the current version before use.

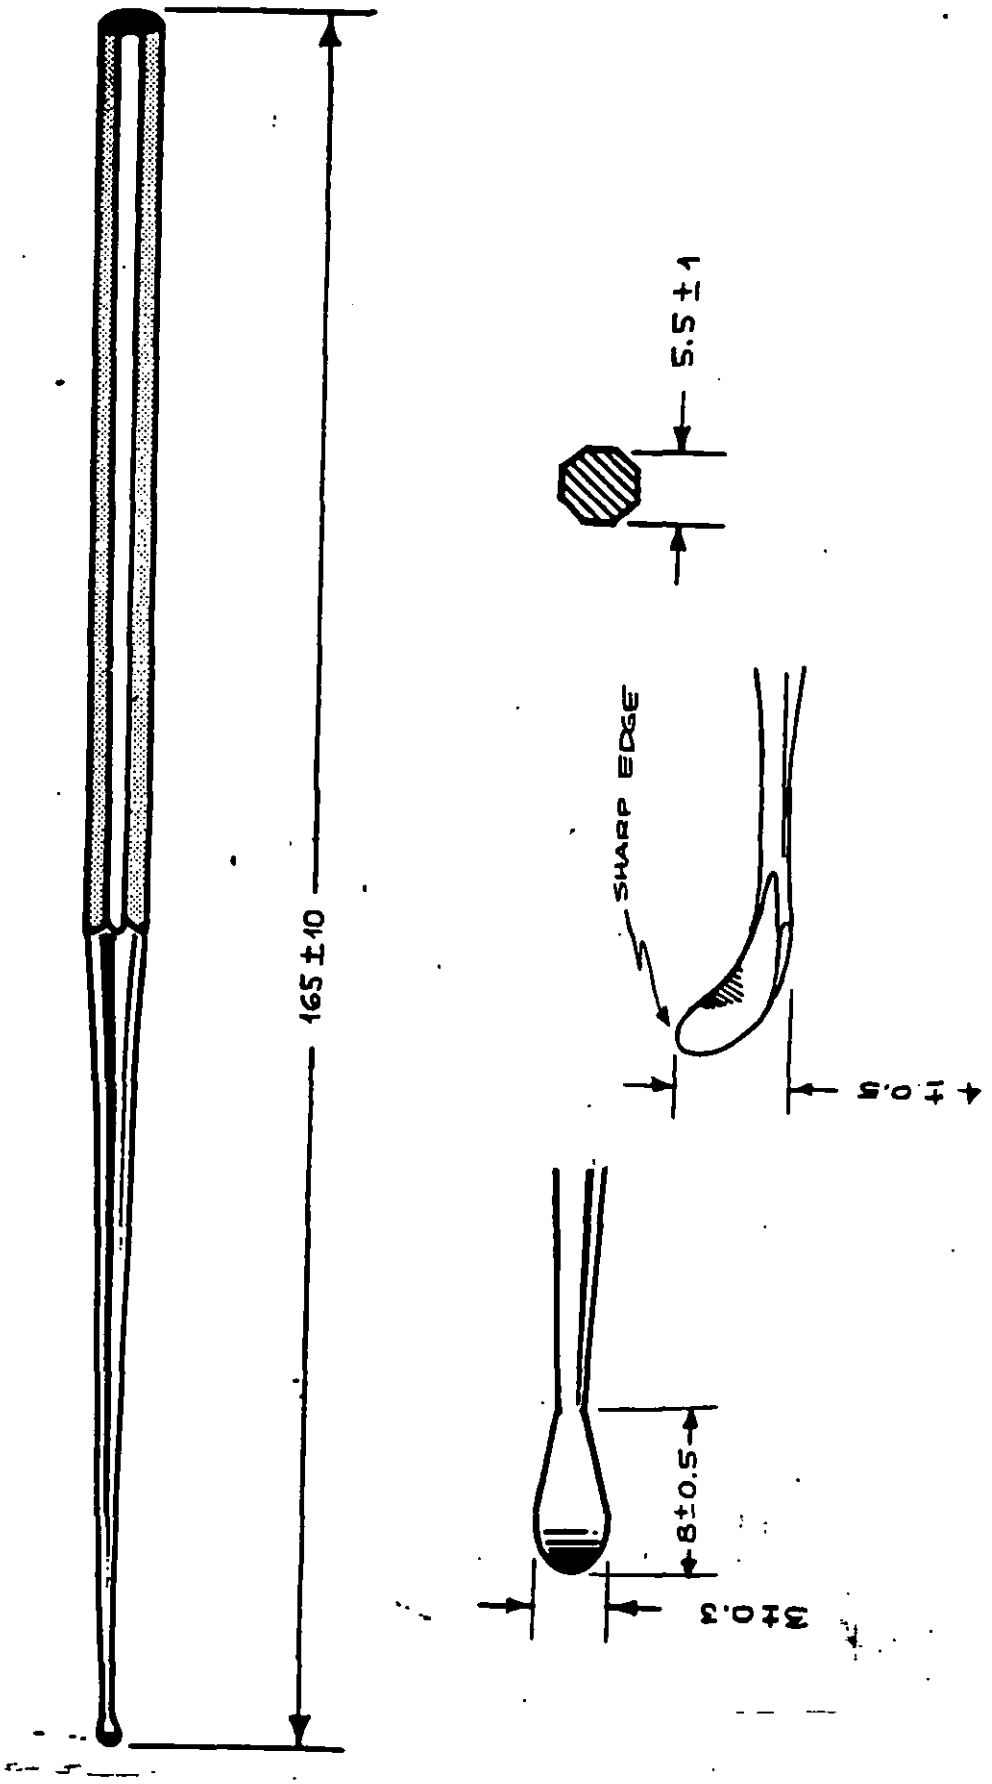


FIGURE 1.

KNIFE-ELEVATOR
PAPARELLA

DIMENSIONS IN MILLIMETERS

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:57Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-51557A	KNIFE-ELEVATOR (Paparella)

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
	☐ USER
3b. ADDRESS *(Street, City, State, ZIP Code)*	☐ MANUFACTURER
	☐ OTHER *(Specify)*: _____

5. PROBLEM AREAS

a. Paragraph Number and Wording:

b. Recommended Wording:

c. Reason/Rationale for Recommendation:

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

DD FORM 1426 PREVIOUS EDITION IS OBSOLETE.

Source: https://assist.dla.mil – Downloaded: 2026-10-26T09:57Z
Check the source to verify that this is the current version before use.