ARTICLE

PRISM: a modular system for glioma progression surveillance on MRI

[PENDING: first author's full name][a] and Jessica Zhang[b]

[a]Department of Biomedical Engineering, Carnegie Mellon University, Pittsburgh, PA, USA; [b]Department of Mechanical Engineering, Carnegie Mellon University, Pittsburgh, PA, USA

ARTICLE HISTORY

Compiled October 26, 2026

ABSTRACT

[PROPOSED, awaiting approval] Treatment effects can mimic glioma progression on MRI; most surveillance datasets lack treatment dates, centres document progression differently and the hardest scans are few. We built PRISM, which scores each scan through separate treatment-timeline and image pathways, so the clinician sees what each score uses, and adds a confidence and a report from a local language model. On MU-Glioma-Post both pathways detected the scan where progression was called; the timeline pathway reached an AUC of 0.82. The combined model, applied unchanged, reached 0.77 on LUMIERE; on UCSF-ALPTDG, single-scan measurements reached 0.80 and the image pathway, with change between scans, 0.73, against 0.86 when trained there. An audit found the models used mainly the timeline at MU-Glioma-Post and enhancing tumour volume at UCSF-ALPTDG. Conformal sets for the combined score met their planned coverage on point estimates at every centre, and after one revision every report passed a check against its record.

KEYWORDS

glioma surveillance; external validation; clinical decision support

1. Introduction

After surgery and chemoradiotherapy, patients with glioma are followed with MRI every few months, and at each scan the team must decide whether the tumour has progressed. The decision is hardest in the months after radiotherapy, when treatment can increase contrast enhancement without tumour growth. This pseudoprogression is most common in the first weeks after chemoradiotherapy and more frequent when the promoter of MGMT, a DNA-repair gene, is methylated (Taal et al. 2008; Brandes et al. 2008). In routine care, progression is therefore documented from the images together with symptoms and the course of treatment, and the date on which it is recorded depends on when the patient was scanned, so a model trained on such records can learn from the schedule as well as from the images.

Surveillance data set five challenges for a model of this task. First, most public surveillance datasets hold images but few treatment dates. Second, centres document progression differently, from dated clinical decisions to expert ratings of each scan, so a model can score well at two centres

CONTACT [PENDING: first author. Email: ...; ORCID: ...]

for different reasons. Third, cohorts are small, and one test split can move the area under the receiver operating characteristic curve (AUC) by more than a change of model (An et al. 2021; Varoquaux 2018). Fourth, the situations in which the decision is hardest, early after radiotherapy or when enhancement grows, hold few cases in any one cohort. Fifth, segmented volumes are noisy, so the clinician needs to see what was measured; and patient records often cannot leave the hospital, so the report has to be written there. Repeated cross-validation addresses the third challenge and external tests the second, which 3 of 20 studies in a recent systematic review of automated response assessment included (Shi et al. 2025); we planned two.

We asked whether a system could give the clinician, at each post-treatment scan, the image evidence and the treatment-timeline evidence separately, transfer to other centres without refitting, and say how far each can be trusted there. We also wanted it to explain each score in a short report written inside the hospital.

We present PRISM, a modular system that scores each post-treatment scan through two pathways, one from clinical data and the treatment timeline and one from measurements of the segmented tumour, and shows a combined score beside them. The confidence has three parts, a conformal prediction set, a statement of whether the pathways agree and a reliability card; a local language model writes the report, and a checker tests it against the scan's record.

We developed PRISM on MU-Glioma-Post (MU) and tested it on LUMIERE and UCSF-ALPTDG (UCSF) with models fitted once and external tests planned in advance. On MU both pathways detected the scan at which progression was documented; the models fitted there transferred to LUMIERE, and the image measurements to UCSF. When we audited the scores, the models at MU used mainly the patient's position in treatment, and at UCSF mainly the enhancing tumour volume. The conformal sets for the combined score met their pre-specified coverage on point estimates at all three centres, at UCSF exactly at the threshold, and after one revision of the prompt every report passed a check against its record.

2. Methods

2.1. PRISM

PRISM handles each scan in five modules (Figure 1). The timeline pathway and the image pathway keep the two kinds of evidence apart, so that the image pathway can run where no treatment dates exist and the audit can show which evidence a score used. Segmentation masks supply the measurements and the images the clinician sees. The confidence gives the clinician a set of plausible outcomes and how many scans like this one the system has been tested on; the report is written inside the hospital, so the record never leaves it. We meet the third challenge, small cohorts, in how we evaluate PRISM (Section 2.3).

The timeline pathway scores a scan from clinical data and the patient's position in treatment. On MU its inputs are age, sex, IDH mutation and MGMT promoter methylation, which alone form the clinical-only reference model, together with the days since diagnosis and since surgery, the start, end and dose of radiotherapy, chemotherapy and the visit index, each taken as of the scan day. Where a cohort records no treatment dates, PRISM uses a reduced timeline that keeps the clinical inputs, the days since surgery and a flag for the first weeks after radiotherapy. The flag comes from the rater's note at LUMIERE and is approximated from the start of radiotherapy at UCSF. Both

pathways are ridge logistic regressions; scaling and any selection were fitted on the training data only.

The image pathway scores a scan from simple measurements of the segmented tumour. On MU it uses 27 inputs: the volumes, shape and relative intensity of the segmented compartments at the scan, their change from the previous scan, and the enhancing and total lesion volumes relative to the smallest in the patient's history ([Supplementary section: image pathway inputs and their harmonisation at LUMIERE and UCSF]). It holds no dates, intervals or treatment flags. A single-scan version keeps only the 19 measurements of the current scan. We defined these inputs after finding that the planned imaging model contained three inputs that encode the scan schedule (Section 3.3). Such inputs belong to the timeline pathway, because they carry when a scan was taken, which the timeline already holds, and the image pathway has to run where no dates exist.

The combined score is one ridge model fitted on both sets of inputs and is shown beside the two pathways. At LUMIERE and UCSF its inputs are the reduced timeline, the harmonised volumes and their change, and the interval since the previous scan, its one schedule input.

The measurements come from the segmentation masks supplied with each cohort: the automatic masks released with MU (Mahmoud et al. 2025), the DeepBraTumIA masks of LUMIERE (Suter et al. 2022) and the masks provided with UCSF (Fields et al. 2024). PRISM renders the report's figure from the same masks by code, and the language model receives only the record, not the image.

Each scan's confidence has three parts, a conformal set, a pathway-agreement statement and a reliability card (Mitchell et al. 2019). The conformal set is a patient-level split conformal prediction set at the 80% level (Angelopoulos and Bates 2023), built to contain the true outcome for at least 80% of scans; it holds one outcome when the score is clear and both when it is not. It comes from the combined model refitted on 70% of the MU patients and calibrated on the remaining 30%; on MU this split is made inside each training fold, and for the external cohorts one MU-calibrated set was applied unchanged, which assumes that their scans are exchangeable with MU's. Because of the refit, the set's model ranks scans slightly differently from the displayed combined score ([Supplementary section: system results]). The two pathways agree when both scores lie on the same side of that pathway's median score over the cohort's evaluation scans; the rule uses scores only, never labels, but as evaluated it needs the scores of a whole cohort ([round 4: agreement rule with medians fixed on MU and applied unchanged externally; NUMBERS.md 12A]). The reliability card looks up the scan's situation, its phase of care crossed with the change in enhancing tumour since the previous scan, in a table of results measured in each cohort. It states the situation's tier: tested, with AUCs and intervals, when the situation holds at least 10 progression and 10 non-progression scans; few cases, with counts only, when it holds fewer; and not tested when it holds none.

A local language model writes the report from the scan's record, and a deterministic checker tests the report against that record. The model (Qwen3.8-27B) runs offline at temperature 0 and receives only the record; the checker rejects any number, flag or confidence statement that is not in the record, any omission of required content, and any wording that offers a diagnosis, advice or a probability (Supplementary Section S19).

2.2. Cohorts and the task

PRISM was developed on MU and tested on LUMIERE and UCSF, in each case on grade 4 glioma as the primary population, with models fitted once on MU and applied unchanged, which we call locked (Table 1). MU records the dates of surgery, radiotherapy and chemotherapy (Mahmoud et al. 2025). LUMIERE records no treatment dates, and the rater notes whether the scan falls within three months of radiotherapy (Suter et al. 2022). UCSF holds one pair of consecutive post-treatment scans per patient, with the start of radiotherapy (Fields et al. 2024). Progression is documented in each cohort's own record (Table 1): as a dated clinical decision at MU, as an expert rating of response at each scan at LUMIERE and as a progression date supplied with the dataset at UCSF. Because the first scan of each pair has no earlier scan, we evaluated the second scan only.

The task is to decide, at each scan, whether this is the scan at which progression is documented. On MU a positive is the first scan on or after the documented progression date, and a negative is a scan followed by at least 120 days without progression. At LUMIERE a positive is the first scan rated as progressive disease, and a negative is an earlier scan rated stable or responding. At UCSF a positive is a second scan with progression dated within 30 days of it and nearer to it than to the first scan; a negative is a second scan with progression at least 120 days later, or with at least 120 days of follow-up without progression. On MU the intended use is scans from the start of radiotherapy onwards, and unless stated MU results are for this population; LUMIERE and UCSF are evaluated on all scans in their detection sets. We divide the intended use into phases of care: during radiotherapy, early after radiotherapy (up to 84 days, 12 weeks, after its end) and later. Predicting progression within 120 days of a scan is reported as a secondary task.

2.3. Evaluation

On MU, every model was evaluated by repeated patient-grouped cross-validation. We used five repeats of five folds, with all scans of a patient in the same fold, and report the mean over repeats of the pooled held-out AUC with a 95% confidence interval (CI) from 1,000 patient-level bootstrap draws. In the analyses of Sections 3.1 to 3.4 no patient appears in more than one of fitting, calibration and testing. We chose this design because in cohorts of this size one split can move an AUC by more than a change of model. We saw this in our first evaluation, in which a radiomics model reached an AUC of 0.80 on one test split and averaged 0.72 when re-selected and re-tested over 500 splits of the same design (Supplementary Section S8 and Figure S2).

For the external tests, each model was fitted once on MU and applied once, under plans committed before any external label was read. The locked models were fitted on all grade 4 detection scans of MU, from every phase of care. The UCSF plan named all MU detection scans; fitting on all gliomas gave the same AUC at LUMIERE, and at UCSF the all-glioma models were tested on all-glioma scans ([Supplementary section: deviations from the plans]). External AUCs have 95% CIs from 1,000 patient-level bootstrap draws. As a reference, we also fitted each UCSF model on UCSF itself by repeated cross-validation. Table 2 lists the questions fixed in advance and their answers.

Some analyses were not planned, and we list them here once. They are the definition of the image pathway on MU (its use at UCSF and in the system tests was planned); the three-step comparison of image models; the clinical-only, image-only and timeline-only models at LUMIERE; the single-scan comparison with models trained at UCSF; the audits of what each score used; the agreement rule and the reliability card, both defined post hoc, after the cohort results had been seen; a

stricter flag rule; the second evaluation of the reports, which followed a failure seen in the first; and the comparison of report models ([round 4: add the new exploratory analyses: MU-fixed agreement, class-conditional coverage, enhancing-volume baselines, operating points, calibration]). In the Results each is marked "(exploratory)" once, where it first appears in a paragraph, and the figure and table notes mark exploratory panels and rows. Comparisons within a phase of care or within an enhancement category are diagnostics of what a score depends on; none of them is a decision rule.

3. Results

3.1. Both pathways detect the progression scan on MU

In the intended use on MU (146 scans; Table 1), the image pathway (exploratory) detected the progression scan with an AUC of 0.71 (95% CI 0.63–0.78), and the timeline pathway with 0.82 (0.75–0.90), mostly by separating phases of care, within which it did no better than the images (Section 3.3). Clinical data alone, without the timeline, scored 0.53, close to chance. The combined score also reached 0.82; on MU the images did not raise the timeline's AUC, and the planned imaging model fell short of the pre-specified gain of 0.03 (Table 2). Predicting progression within 120 days of a scan was harder; the model reached 0.60 (0.52–0.69) in the intended use (Supplementary Section S23). In one secondary evaluation set, all scans of all gliomas, the planned model did gain 0.04 (Table 2), which may reflect image inputs that encode the scan schedule (Section 3.3). A timeline pathway needs treatment dates, which the two external cohorts largely lack, so we next tested how each pathway transfers to them.

3.2. The models transfer to two external centres without refitting

The locked combined model reached 0.77 (0.68–0.86) on LUMIERE (Figure 2) and met its planned transfer rule (Table 2). At LUMIERE the combined score was above either pathway alone, images 0.65 and the reduced timeline 0.69 (exploratory; the gain over the timeline alone had an interval that included zero). Clinical data alone stayed close to chance in all three cohorts (Figure 2). [round 4: enhancing tumour volume alone as a reference at MU and LUMIERE (UCSF in Section 3.3), as a bar in Figure 2 (NUMBERS.md 12C); sensitivity and specificity at one MU-fixed threshold (12D) and calibration externally (12F), one sentence here and a supplementary table.]

At UCSF, both planned image models transferred. Measurements of the single scan reached 0.80 (0.69–0.89), and the image pathway, which adds change from the previous scan, reached 0.73 (0.60–0.84), meeting its planned transfer rule (Table 2). Training at UCSF raised the image pathway to 0.86 (difference 0.14, 0.03–0.26), while the single-scan model scored about the same when trained there (exploratory). The change inputs therefore transferred less well than the measurements of the scan itself. The reduced timeline, whose early-post-radiotherapy flag UCSF can only approximate (Section 2.1), transferred worst of the pathways, at 0.56. The combined score at UCSF scored above the image pathway (Figure 2), partly through the interval between the two scans, which was shorter before progression. Because similar AUCs at different centres can come from different evidence, we audited what each score used.

3.3. *What each score rests on depends on the cohort*

The audit (exploratory) shows that at MU the scores depend mainly on where the patient is in treatment, and at UCSF on how much the tumour enhances (Figure 3). At MU the scan schedule alone separates most progression scans from most non-progression scans, because most progression scans came more than 12 weeks after radiotherapy and most non-progression scans came within those 12 weeks (Table 1). Across phases of care, adding the timeline to clinical data and images gained 0.11 (0.04–0.20); within a phase it gained −0.02 (−0.13 to +0.11) (Figure 3A). Within a phase the images also gave about as much evidence as the timeline, 0.68 (0.58–0.77) against 0.64 (0.51–0.78).

We built the image model on MU in three steps (exploratory) to see which inputs raised its AUC (Figure 3C). Adding change from earlier scans to the current scan's measurements gave the image pathway, 0.05 higher ([round 4: bootstrap CI for this step; NUMBERS.md 12E]), and adding the three schedule inputs of the planned imaging model (the interval since the previous scan, a flag for whether there was one and the smallest volume counted from the end of radiotherapy) raised the AUC to 0.81 across phases of care but not within them (−0.01, −0.06 to +0.04).

At UCSF the progression calls follow enhancement closely. Enhancing tumour volume alone, the simplest baseline, gave an AUC of 0.88 (0.79–0.95), higher than the point estimates of the locked image models; UCSF rated enhancement as increased at 27 of the 29 progression scans, and progression was dated a median of 7 days after the evaluated scan (Figure 3B). Among the 37 scans rated as showing increased enhancement, the single-scan image model reached 0.65 (0.44–0.84), so beyond that rating the measurements added little. At UCSF an AUC therefore largely measures agreement with a progression call made from enhancement at the same scan, which the image pathway measures directly. Deep networks fine-tuned to score UCSF scans directly learned from the images, above a permuted-label control (Table 2), and their scores tracked enhancing volume (correlation about 0.8; [Supplementary section: deep networks at MU and UCSF]). Because the evidence behind a score differs by cohort and by situation, PRISM attaches a confidence to each score.

3.4. *The conformal sets of the combined score meet their coverage threshold on point estimates at all three centres*

At the 80% level, the conformal sets of the combined score covered between 0.78 and 0.87 of scans in the three cohorts, meeting on point estimates the threshold of 0.78 fixed in advance, a tolerance of 0.02 below the nominal level (Figure 4A). Most sets were informative, holding a single outcome for 62% to 75% of scans. At UCSF the point estimate sat at the threshold and its interval reached below it (0.68–0.87). Coverage fell short for the image pathway alone at LUMIERE and the timeline alone at UCSF, and it was uneven across situations within each cohort ([Supplementary section: system results]). [round 4: coverage by true class (progression and non-progression) in each cohort, with the single-outcome share by class; NUMBERS.md 12B.]

On MU, the warning that the two pathways disagree (exploratory) picked out the less accurate scans. The pathways disagreed on 40% of MU scans; the combined score's AUC was 0.90 where they agreed and 0.59 where they disagreed, and setting the disagreeing scans aside gained more than removing the same number matched for phase of care (Table 2; Figure 4B). At LUMIERE and UCSF disagreement did not pick out the less accurate scans. [round 4: restate with the MU-fixed agreement rule (NUMBERS.md 12A), whose LUMIERE result differs.] A stricter rule chosen after

these results, flagging a scan only when the pathways disagree and its set holds both outcomes, is described in the [Supplementary section: system results].

The reliability card (exploratory) states, for each scan, how many tested cases its situation holds, and this differs by cohort. Across the three cohorts only four situations held at least 10 progression and 10 non-progression scans, one at MU and three at LUMIERE; 35 of the 249 MU scans fell in a tested situation, most LUMIERE scans did, and every situation at UCSF had few cases (Figure 4C). At MU no situation in the first 12 weeks after radiotherapy held more than three progression scans. Tested situations had lower error than few-case situations at LUMIERE, with overlapping intervals (Table 2); at MU the order was reversed, with a Brier score of 0.222 in tested situations against 0.147 in few-case ones, because the few-case scans there were mostly non-progression scans early after radiotherapy, which the models score easily. The clinician reads these statements in the report, which we evaluated next.

3.5. Every report passes a check of its numbers, flags and wording against the record

Every evaluation report written by the local model passed a lexical check of its numbers, flags and wording against its record (114, 162 and 130 reports at MU, LUMIERE and UCSF; Figure 5); the check cannot judge emphasis, order or what a clinician would infer from the wording. These counts come from a second evaluation (exploratory), after one revision of the prompt; its records exclude the 10 LUMIERE and 10 UCSF patients used to develop the revision and are otherwise those of the first evaluation. The first evaluation had failed at LUMIERE (0 of 178) because one sentence quoted a number that was in no cited field; we corrected the prompt and left the checker unchanged. The reports stated the evidence tier wherever the card had few or no cases, and followed a changed field in 28 of 30 perturbed records (Table 2). The smallest open-weight model that passed in every cohort had 27 billion parameters and ran on one GPU ([Supplementary section: second report evaluation and model comparison]). The report therefore gives the clinician the volumes, the two scores and the confidence exactly as the record holds them.

4. Discussion

PRISM gives the clinician separate image and treatment-timeline evidence at each scan, transfers to two external centres without refitting, and states how far each score has been tested in the scan's situation, which for most scans at MU and UCSF is little. At the development centre the timeline provided most of the evidence, largely because of when patients were scanned, and within a phase of care the images provided about as much; at UCSF the image measurements provided the score, and training there raised it further; the locked results therefore measure transfer, and a model fitted at the centre can do better. Because the pathways were kept apart, we could measure these differences at each centre, and each report states them through the confidence and the card.

Because its modules are separate, PRISM runs where data are incomplete. The image pathway needs only the scans and their masks, which is what most public surveillance datasets hold; at LUMIERE and UCSF it ran without treatment dates. Where dates exist, the timeline is added as a second pathway, and the combined score, one ridge model on both sets of inputs, is shown beside both without changing the image model. A new cohort adds rows to the reliability card, so the tiers change as evidence accumulates and no confidence model has to be refitted.

Consider, as an illustration, a scan eight weeks after radiotherapy in which the enhancing tumour has grown. At MU, 1 of the 9 scans in this situation on the card (all grade 4 detection scans) was progression (exploratory). The timeline pathway scores such a scan low, because most scans at this point in treatment are not progression, and the image pathway scores it high, because enhancement has grown. PRISM's report would show both scores, state that they disagree, give a conformal set that holds both outcomes and record that the card has few cases for this situation. The clinician then sees that the system has no measured basis for a call at this scan, in the weeks when pseudoprogression is most common, and decides with information PRISM does not use, such as symptoms, steroid dose and the radiotherapy plan.

Each of PRISM's components has been described before, and we are not aware of a system that combines them. Automatic segmentation of post-treatment glioma with measurement of change between scans is established (Rudie et al. 2022), conformal prediction has been applied to glioma segmentation (Elyassirad et al. 2025), clinical and imaging data have been fused to separate pseudoprogression from progression (Gomaa et al. 2025), and model cards report performance by subgroup (Mitchell et al. 2019). The closest system we found combines treatment variables extracted by a language model with tumour volumes to assign a structured follow-up category at one centre, without an uncertainty attached to the output (Jabal et al. 2026). On MU, Christodoulou et al. (2026) predicted a label assigned at the patient level with a radiomics model, a different question from detection at the scan. On LUMIERE, [cite Tikhonov 2025, arXiv:2509.06511; full reference not yet verified] classified each scan into four response categories, and Chen et al. (2026) predicted recurrence risk from preoperative and postoperative MRI across centres; both address other labels.

PRISM was developed at one centre, with 126 grade 4 patients (80 in the intended-use detection set), and the two external tests are its only evidence of transfer. The label is progression as each centre documented it; no scan was re-read for this study, and at UCSF the label agrees closely with an enhancement call at the same scan. Subgroups are small, and UCSF contributes 29 progression scans. The coverage threshold was met on point estimates, and at UCSF the interval reached below it; the disagreement warning picked out less accurate scans only at MU. The exploratory analyses listed in Section 2.3 need testing on new data. The report checker is lexical, and no clinician has yet read the reports. PRISM forecast progression within 120 days less well than it detected it at the scan, so we present it as a detection system and report the forecast as a secondary task.

The next step is to pool the rare situations across cohorts and train on them. Early progression after radiotherapy and growing enhancement without progression are rare at any one centre. The Burdenko and UCSD-PTGBM datasets add radiotherapy detail and advanced sequences, and each new cohort adds cases to the card's thin situations, which is where models fine-tuned on these long-tail cases could be tested. A reader study in which clinicians use PRISM's reports at the scan would show whether separate evidence and a stated confidence change their decisions.

Conclusion

PRISM keeps image and treatment-timeline evidence apart, and its models held at two other centres without refitting. In our three cohorts the images and the timeline each contributed, in different proportions at each centre, and PRISM shows the clinician both scores at every scan, with how far each has been tested there.

Acknowledgements

[PENDING AUTHOR DECISION].

Disclosure statement

[PENDING AUTHOR DECISION: competing interests, or "The authors report there are no competing interests to declare."] If any author serves on the editorial or advisory board of this journal, state it here.

Declaration of generative AI use

[DRAFT, PENDING AUTHOR CONFIRMATION:] Generative AI is part of the system studied. PRISM's report generator uses a local language model (Qwen3.8-27B; six other open-weight models in a comparison); all ran offline on the authors' computing cluster and saw only derived system records. An AI assistant (Claude, Anthropic) was used to write and run analysis code and to draft and edit the manuscript under the authors' direction; it was given no patient-level data through any hosted service. The authors reviewed all code, results and text and take full responsibility for the content of this article.

Funding

[PENDING AUTHOR DECISION: "This work was supported by the [Funding Agency] under Grant [number]." If there was no funding: "No funding was obtained for this work."]

Ethics statement

[PENDING AUTHOR DECISION: secondary analysis of de-identified datasets (MU-Glioma-Post and LUMIERE, public; UCSF-ALPTDG under a data use agreement); state the institutional determination or waiver and cite the source datasets' approvals.] No registered protocol. Analysis plans were committed to the repository before each external test; their commits are listed in Table 2. Patient and public involvement: none.

Data availability statement

[PENDING AUTHOR DECISION: MU-Glioma-Post (TCIA, doi:10.7937/7K9K-3C83) and LUMIERE (figshare; Suter et al. 2022) are public; UCSF-ALPTDG is available from its provider under a data use agreement; state which derived tables, fold assignments and locked model files are released, with a DOI.] Code: [PENDING: public repository link and release tag.]

Supplemental material

Supplemental data for this article are provided as a separate file.

Notes on contributors

[PENDING: a short biographical note for each author (no more than 200 words each).]

References

An C et al. 2021. Radiomics machine learning study with a small sample size: Single random training-test set split may lead to unreliable results. PLOS ONE. 16(8):e0256152. https://doi.org/10.1371/journal.pone.0256152

Angelopoulos AN, Bates S. 2023. Conformal prediction: A gentle introduction. Found Trends Mach Learn. 16(4):494–591. https://doi.org/10.1561/2200000101

Brandes AA, Franceschi E, Tosoni A et al. 2008. MGMT promoter methylation status can predict the incidence and outcome of pseudoprogression after concomitant radiochemotherapy in newly diagnosed glioblastoma patients. J Clin Oncol. 26(13):2192–2197. https://doi.org/10.1200/JCO.2007.14.8163

Chen C, Guo F, Huang D et al. 2026. Predicting recurrence risk of glioblastoma based on preoperative-postoperative longitudinal MRI: A multicenter study. Bioengineering. 13(6):668. https://doi.org/10.3390/bioengineering13060668

Christodoulou RC, Vamvouras G, Pitsillos R, Solomou EE, Georgiou MF. 2026. Explainable radiomics with probability calibration for postoperative glioblastoma surveillance. Eur J Radiol Artif Intell. 5:100074. https://doi.org/10.1016/j.ejrai.2026.100074

Elyassirad D, Gheiji B, Vatanparast M, Ahmadzadeh AM, Faghani S. 2025. CONSeg: Voxelwise uncertainty quantification for glioma segmentation using conformal prediction. Am J Neuroradiol. 46(12):2553–2560. https://doi.org/10.3174/ajnr.A8914

Fields BKK et al. 2024. The University of California San Francisco adult longitudinal post-treatment diffuse glioma MRI dataset. Radiol Artif Intell. 6(4):e230182. https://doi.org/10.1148/ryai.230182

Gomaa A, Huang Y, Stephan P et al. 2025. A self-supervised multimodal deep learning approach to differentiate post-radiotherapy progression from pseudoprogression in glioblastoma. Sci Reports. 15:17133. https://doi.org/10.1038/s41598-025-02026-7

Jabal MS et al. 2026. Agentic automation of BT-RADS scoring: End-to-end multi-agent system for standardized brain tumor follow-up assessment. [Preprint, arXiv:2603.21494]. `https://arxiv.org/abs/2603.21494`

Mahmoud E, Gass J, Dhemesh Y et al. 2025. MU-Glioma Post: A comprehensive dataset of automated MR multi-sequence segmentation and clinical features. Sci Data. 12(1):1847. https://doi.org/10.1038/s41597-025-06011-7

Mitchell M, Wu S, Zaldivar A et al. 2019. Model cards for model reporting. In: Proceedings of the Conference on Fairness, Accountability, and Transparency (FAT* '19). ACM. p 220–229

Rudie JD, Calabrese E, Saluja R et al. 2022. Longitudinal assessment of posttreatment diffuse glioma tissue volumes with three-dimensional convolutional neural networks. Radiol Artif Intell. 4(5):e210243. https://doi.org/10.1148/ryai.210243

Shi T, Kujawa A, Linares C, Vercauteren T, Booth TC. 2025. Automated longitudinal treatment

response assessment of brain tumors: A systematic review. Neuro-Oncology. 27(8):1946–1971. https://doi.org/10.1093/neuonc/noaf037

Suter Y, Knecht U, Valenzuela W et al. 2022. The LUMIERE dataset: Longitudinal glioblastoma MRI with expert RANO evaluation. Sci Data. 9(1):768. https://doi.org/10.1038/s41597-022-01881-7

Taal W, Brandsma D, de Bruin HG et al. 2008. Incidence of early pseudo-progression in a cohort of malignant glioma patients treated with chemoirradiation with temozolomide. Cancer. 113(2):405–410. https://doi.org/10.1002/cncr.23562

Varoquaux G. 2018. Cross-validation failure: Small sample sizes lead to large error bars. NeuroImage. 180:68–77. https://doi.org/10.1016/j.neuroimage.2017.06.061

Tables

Table 1. The three cohorts. What each cohort records, and the scans in the detection task. Grade 4 glioma is the primary population.

	MU-Glioma-Post	LUMIERE	UCSF-ALPTDG
Role	Development (repeated cross-validation)	External, locked	External, locked
Access	Public	Public	Data use agreement
Scans per patient	Up to 6 index scans (median 2)	Up to 10 index scans (median 2)	One consecutive pair
Treatment dates	Surgery, radiotherapy start and end, dose, chemotherapy	None; rater flag for scans within three months of radiotherapy	Days from surgery; radiotherapy start only
Documented progression (the label)	Documented date in the clinical record	Expert response rating of each scan	Progression date supplied with the dataset
Segmentation masks	Automatic masks released with the dataset	DeepBraTumIA (three labels)	Masks provided with the dataset
Patients[a]	126	61	140
Age, median	62.5 (IQR 53–70)	62 (IQR 53–70)	57.5
Male	66 (52%)	32 (52%)	81 (58%)
IDH wildtype / mutant / unknown	112 / 8 / 6	38 / 1 / 22	81 / 13 / 46
MGMT methylated / unmethylated / unknown	45 / 62 / 19	26 / 28 / 7	71 / 43 / 26
Detection task[b]: progression / non-progression scans (patients)	62 / 84 (80) in the intended use; 64 / 117 (92) over all scans	73 / 105 (79)	29 / 40 (69), second scan only
Phase of care in the detection set	Progression: 56 of 62 later after radiotherapy; non-progression: 51 of 84 early after radiotherapy	Not recorded	65 of 69 later after radiotherapy[c]

[a] Patient characteristics describe the cohorts of the secondary 120-day task at MU-Glioma-Post (grade 4) and LUMIERE, and all grade 4 patients at UCSF-ALPTDG. Age is at diagnosis at MU-Glioma-Post and at surgery at LUMIERE.

[b] Positives are the scan at which progression was documented; negatives are defined per cohort in Section 2.2. The LUMIERE detection set has more patients than the 120-day cohort because it includes patients who contribute only a progression scan. At MU-Glioma-Post, 47 progression scans of patients with no index scan (no scan with a 120-day label) are excluded.

[c] UCSF-ALPTDG gives only the first radiotherapy start; the phase assumes a six-week course. Two scans were early after radiotherapy and two had no radiotherapy date.

Table 2. Questions fixed in advance and their answers. Each rule was committed to the repository before the analysis it governs. AUC differences with 95% CIs.

Question	Rule fixed in advance	Result	Met
Detection on MU-Glioma-Post			
Do image measurements add to the timeline?	Planned model ≥ 0.75 (lower bound ≥ 0.65) and gain ≥ 0.03 with CI above 0	Model 0.837 (0.763–0.904); gain +0.015 (−0.032 to +0.063)	No
Do fine-tuned deep networks add?	Gain ≥ 0.03 with CI above 0; permuted-label control covers 0.5	No network added; control 0.483 (0.436–0.527)	No (control valid)
Does the locked model transport to LUMIERE?	External AUC ≥ 0.65 (below: transport failure)	AUC above 0.65 (Section 3.2); no transport failure	Yes
UCSF-ALPTDG			
Q1. Does the image pathway transport?	AUC ≥ 0.65, lower bound > 0.5	Both conditions met (Section 3.2)	Yes
Q2. Do images add to clinical data without a timeline?	Gain with CI above 0	+0.248 (+0.096 to +0.392)	Yes
Q3. Does training at UCSF-ALPTDG do better than the locked model?	Descriptive	Higher when trained there (Section 3.2)	Descriptive
Q4. Do deep networks learn at UCSF-ALPTDG?	Above the permuted-label control; control covers 0.5	+0.201 (+0.094 to +0.306) over a control of 0.541 (0.480–0.603)	Yes
The system (MU-Glioma-Post, LUMIERE, UCSF-ALPTDG)			
S1. Do conformal sets keep their coverage?	Coverage ≥ 0.78 at the 80% level in each cohort	Combined score met in all three (Section 3.4); images at LUMIERE 0.708 and timeline at UCSF-ALPTDG 0.696	Yes (combined)
S2. Do flags pick out less accurate scans?	AUC unflagged minus flagged > 0, CI above 0	Disagreement at MU-Glioma-Post +0.307 (+0.175 to +0.432); per-cohort results in the supplement[a]	Both at MU-Glioma-Post; set at LUMIERE; none at UCSF-ALPTDG
S3. Does setting flagged scans aside beat matched removal?	Retained AUC minus matched removal > 0, CI above 0	Disagreement met at MU-Glioma-Post (Section 3.4); per-cohort results in the supplement[a]	MU-Glioma-Post (disagreement); UCSF-ALPTDG (set)
S4. Do the card's tiers mean something?	Descriptive: tested below few cases in Brier score and error	Brier 0.187 vs 0.258 at LUMIERE; reversed at MU-Glioma-Post (Section 3.4)	Descriptive
S5. Are reports faithful to the record?	≥ 95% pass the checker in each cohort	First evaluation failed at LUMIERE; second evaluation: all passed (Section 3.5)	No, then yes

Figure legends

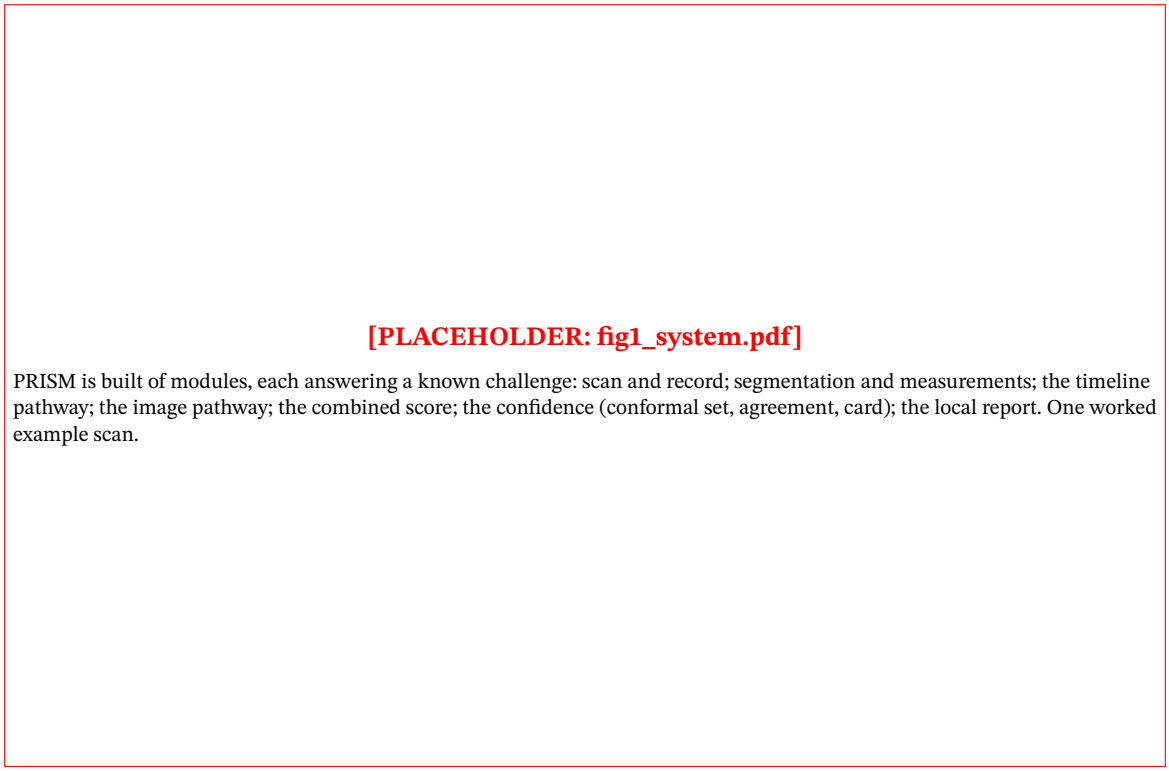


Figure 1. PRISM is built of modules, each answering a known challenge. A scan and its record enter two pathways: the timeline pathway (clinical data and the patient's position in treatment) and the image pathway (measurements from the segmentation masks supplied with each cohort). The combined score, one ridge model on both sets of inputs, is shown beside them. The confidence has three parts: a conformal prediction set at the 80% level, a statement of whether the two pathways agree, and the reliability card's tier for the scan's situation. A local language model writes the report from the record, and a deterministic checker tests its numbers, flags and confidence statements against the record. One example scan is followed through each module.

[PLACEHOLDER: fig2_transport.pdf]

AUC by pathway (clinical alone, timeline, images, combined) and cohort (MU internal; LUMIERE and UCSF locked; UCSF-trained as a reference).

Figure 2. The models transfer to two external centres without refitting. AUC for detecting the scan at which progression was documented, by pathway (clinical data alone, timeline, images, combined) and cohort: MU-Glioma-Post (repeated cross-validation, intended use); LUMIERE and UCSF-ALPTDG (models fitted once on MU-Glioma-Post and applied unchanged); and UCSF-ALPTDG with models trained there, as a reference. At LUMIERE and UCSF-ALPTDG the timeline is the reduced version, and the clinical-only model at LUMIERE is exploratory. At UCSF-ALPTDG the images are shown for the single-scan model and for the image pathway with change features, which is the system's image pathway; the combined score there includes the interval between the two scans. [round 4: enhancing tumour volume alone as a reference bar in each cohort; NUMBERS.md 12C.] Bars are 95% patient-bootstrap CIs.

[PLACEHOLDER: fig3_evidence.pdf]

(A) MU: the timeline's gain lies between phases of care. (B) UCSF: enhancing volume alone scores above the image models. (C) The image-model ladder (exploratory).

Figure 3. What each score rests on depends on the cohort. (A) MU-Glioma-Post: the gain from adding the timeline to clinical data and images, across phases of care and within them. (B) UCSF-ALPTDG: AUC of enhancing tumour volume alone beside the locked image models, and the share of progression and non-progression scans that UCSF rated as showing increased enhancement. (C) The image model on MU-Glioma-Post built in three steps (current scan; with change from earlier scans; with schedule inputs), across and within phases of care. All panels are exploratory. Bars are 95% patient-bootstrap CIs.

[PLACEHOLDER: fig4_confidence.pdf]

(A) Conformal coverage at the 80% level by cohort and pathway. (B) AUC with and without the disagreement warning. (C) The reliability card: situations by cohort with their evidence tier.

Figure 4. The conformal sets of the combined score meet their coverage threshold on point estimates, and at MU-Glioma-Post disagreement marks the less accurate scans. (A) Coverage of the 80% conformal sets by cohort and pathway; the dashed line is the threshold fixed in advance, met by the combined score on point estimates in all three cohorts. (B) AUC of the combined score where the pathways agree and where they disagree, and after the disagreeing scans are set aside, compared with removal matched for phase of care, at MU-Glioma-Post; at LUMIERE and UCSF-ALPTDG disagreement did not pick out the less accurate scans. (C) The reliability card: situations (phase of care by change in enhancing tumour) in each cohort, shaded by tier (tested, few cases, not tested). The agreement rule and the card are exploratory.

[PLACEHOLDER: fig5_report.pdf]

One rendered report (segmentation figure, pathways, combined score, confidence) and faithfulness by cohort.

Figure 5. The report states the evidence and passes a check against the record. Left: one report as the clinician receives it, with the segmentation figure and its volumes, the two pathway scores, the combined score, the conformal set, the agreement statement and the card's tier. Right: share of reports passing the lexical check of numbers, flags and wording, by cohort, in the second evaluation, after one revision of the prompt following a failure at LUMIERE (Section 3.5).