

Tele Sensor Client Result

Sarah Jones

Date: February 12, 2024

Heart Rate: 90


Metric: Bpm

RMS Value: 100.73

RMS Accuracy: 72%

RMS Error: 5%

Graph Metric

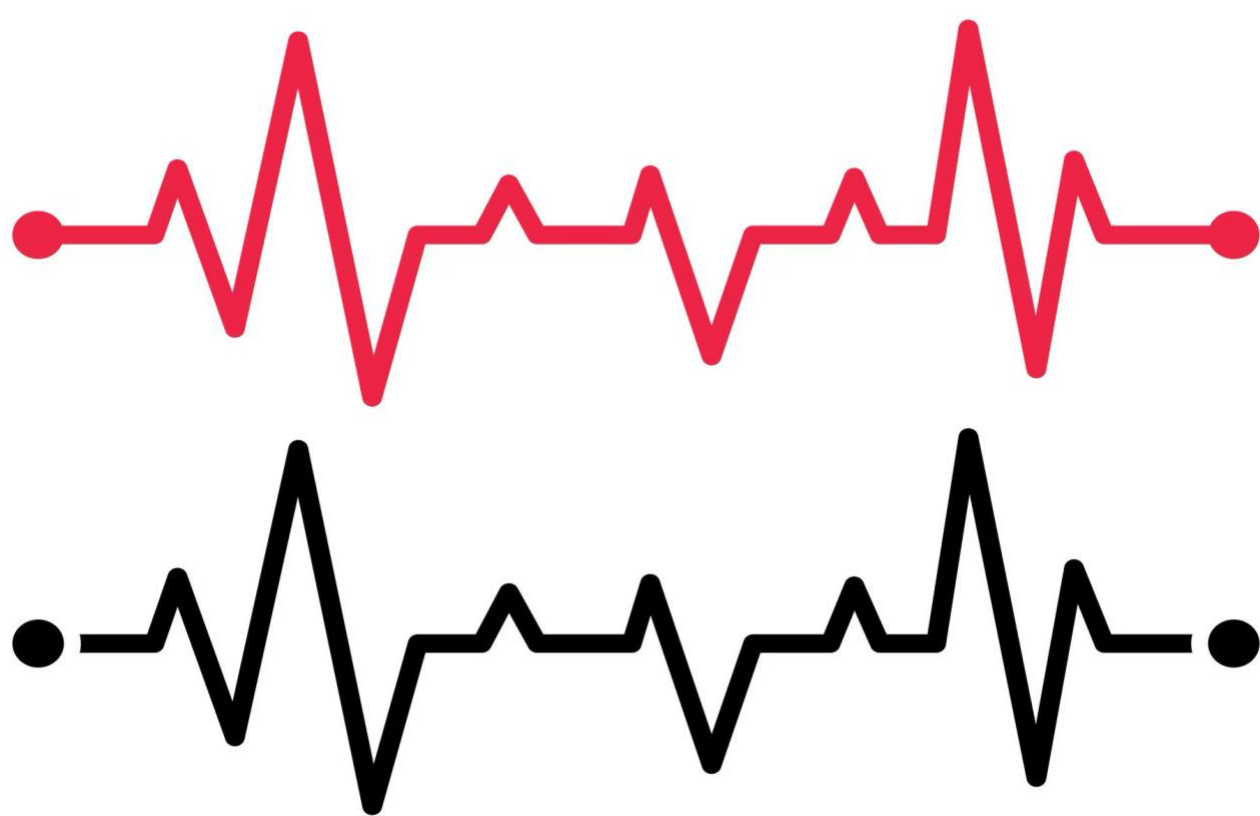

Note: this is a made result for system tests not real, this note can be used to display some information about the result or patient.