
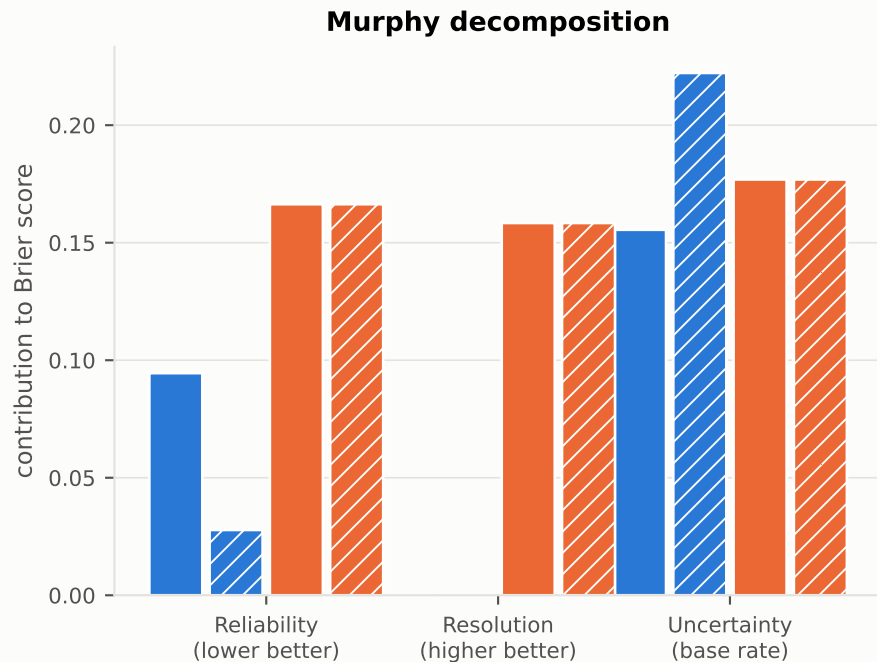


Figure 6 Calibration: Brier score decomposed into reliability, resolution and irreducible uncertainty

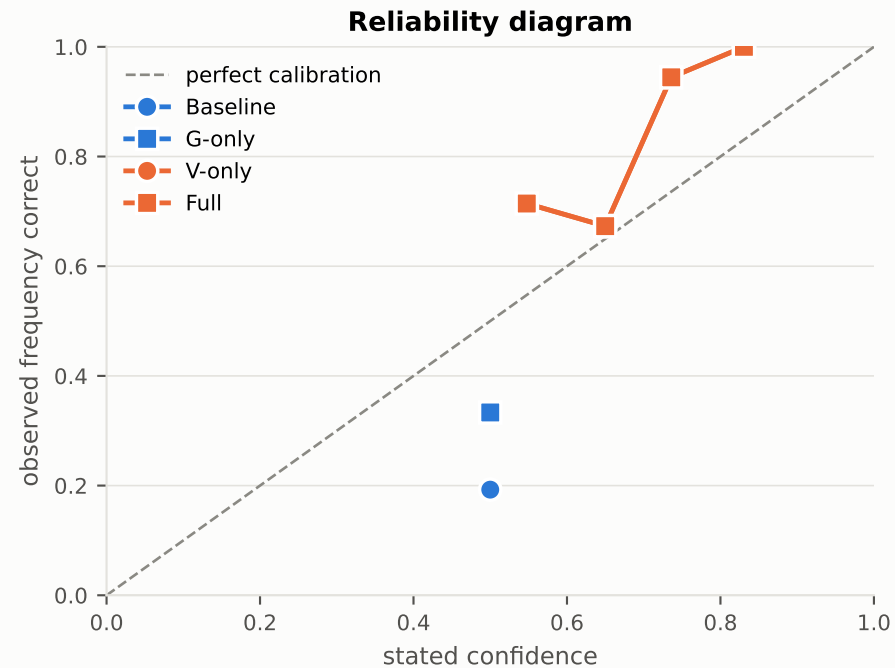

Baseline (V0 G0) G-only (V0 G1) V-only (V1 G0) Full GMAIS (V1 G1)