
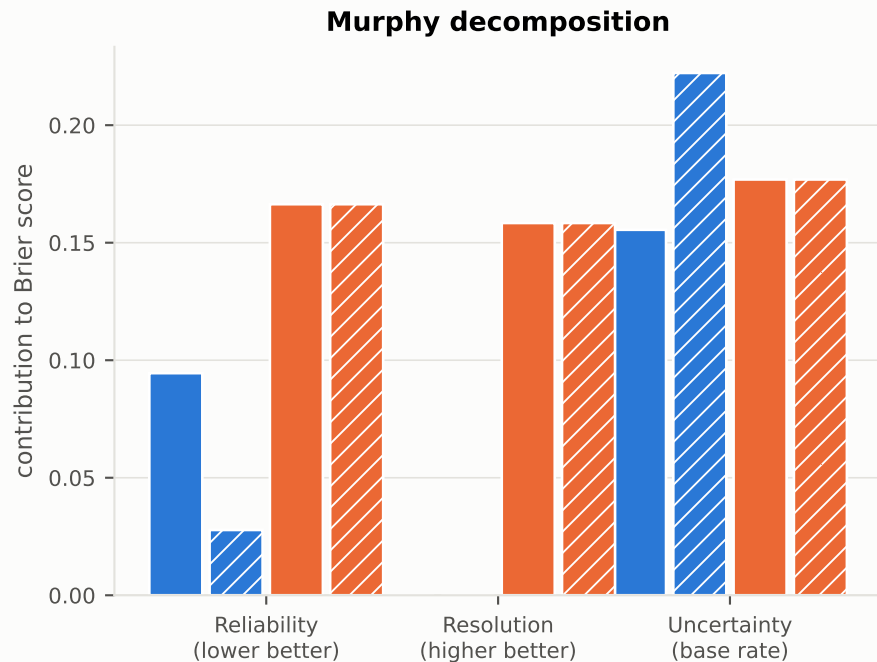


**Figure 6 Calibration: Brier score decomposed into reliability, resolution and irreducible uncertainty**

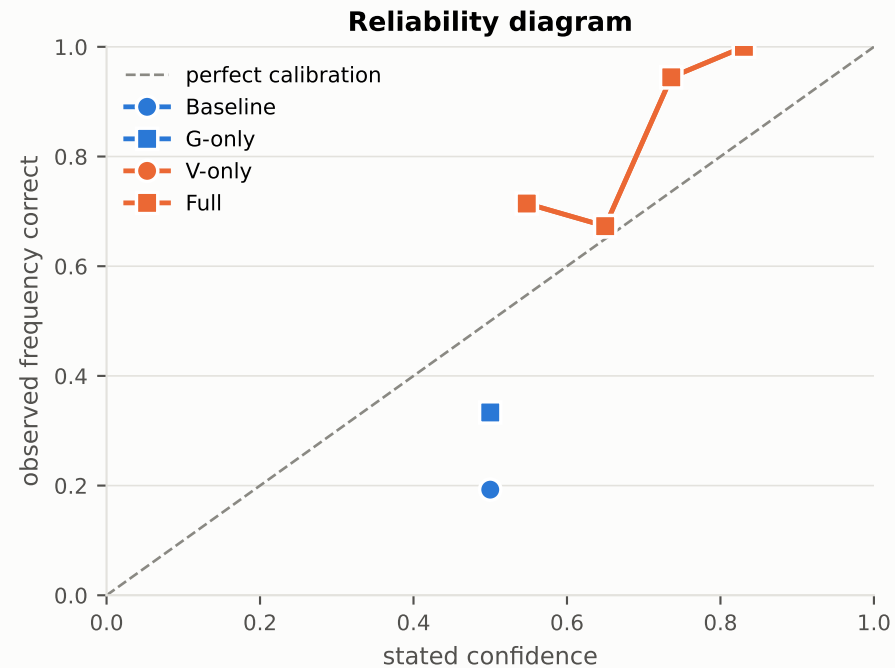

Baseline (V0 G0)    G-only (V0 G1)    V-only (V1 G0)    Full GMAIS (V1 G1)