




1-2. Implementation and normalisation

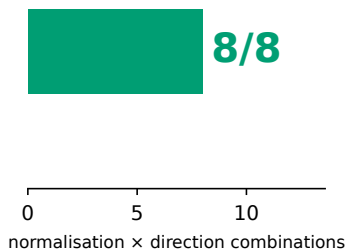


3. Platform suitability

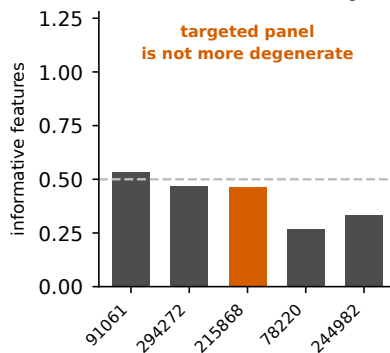


3. Score not degenerate

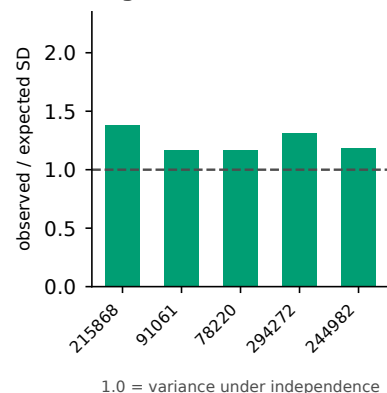


5. Biopsy timepoint

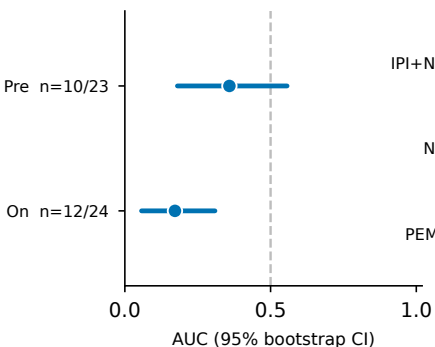

6. Treatment regimen

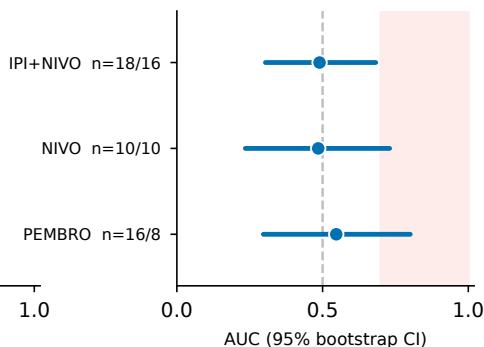

4. Sample size

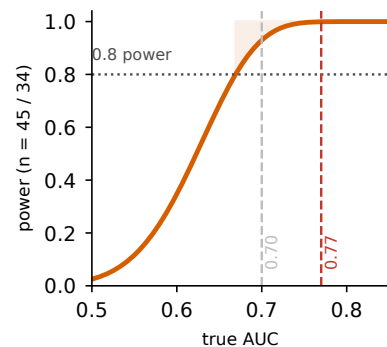

Excluded by design and data (7 of 9):

- 1 implementation error
- 2 normalisation
- 3 platform unsuitability
- 4 sample size
- 5 biopsy timepoint
- 6 treatment regimen
- 7 endpoint definition
- 8 population composition
- 9 weakness in the derivation cohorts

X = the available data cannot exclude this. Item 7 needed no data panel: the native endpoint of GSE215868 is 24-month long-term benefit (PFS-derived), not RECIST, so response was re-derived from best overall response to match the endpoint on which IMPRES was reported.