Calibration:

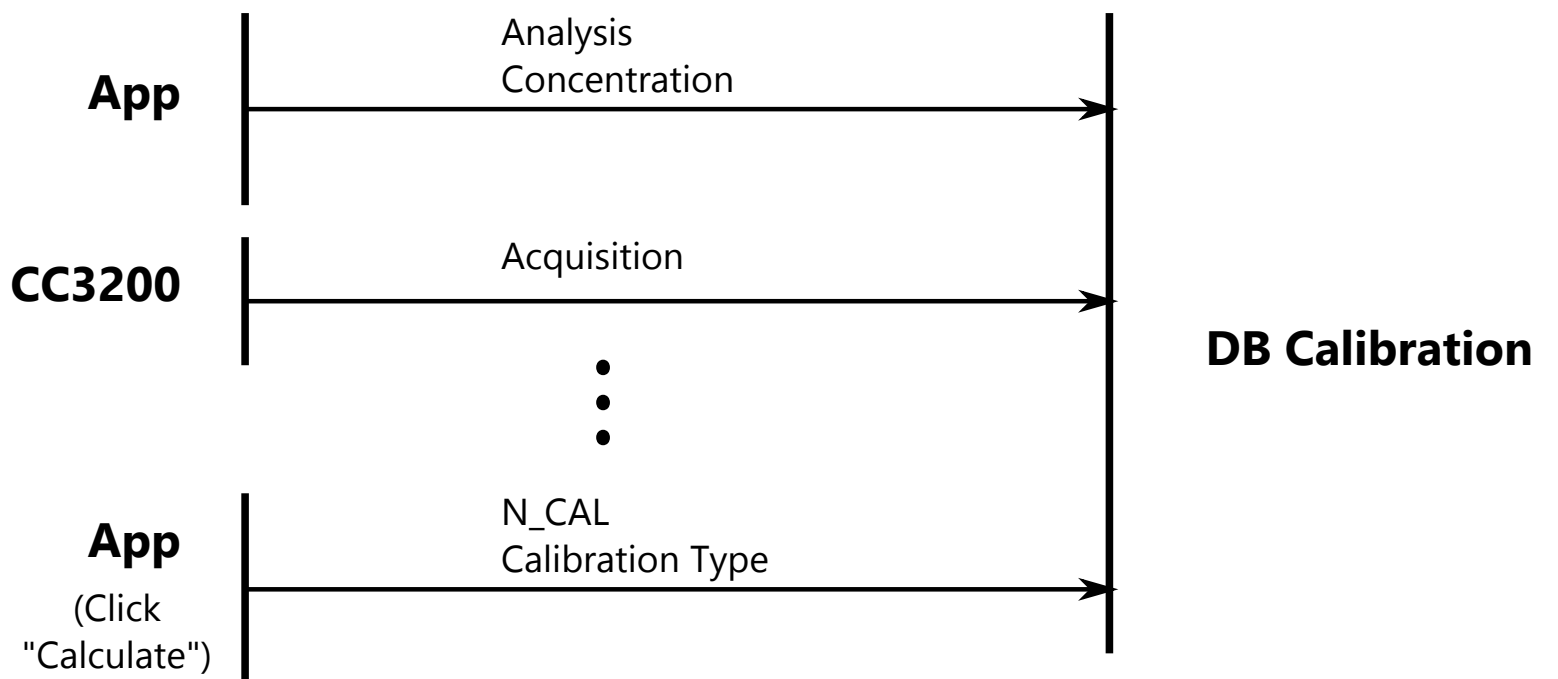|	
App	Analysis Concentration →
CC3200	Acquisition →
	⋮
App (Click "Calculate")	N_CAL Calibration Type →

DB Calibration

---- Pause >15 sec ----

App	runScript = true →
Script	runScript = true ←
	parameters →
App	parameters ←
	parameters →

DB Temp

DB Calibration

DB Analyses