


Boost — Parkes Error Grid (forecast accuracy)

Parkes Consensus Error Grid, **Type 1** (Pfützner 2013, Table 1). Window 14 days, 30-min horizon.
Anonymised. Generated by parkes_grid.py.

What this is

Reference (x) = the BG that actually occurred 30 min later; test (y) = Boost's predicted BG at that horizon (oref predBGs . IOB). So this grids Boost's forward-forecast accuracy — the prediction the dosing engine relies on. **Zone A** = clinically accurate; **A+B** = acceptable.

This is NOT the paper's two-version equivalence (that needs the replay harness / Method 2). It is a real Parkes grid on data we have, and the building block toward replay. IOB-only forecast: during meals the COB/UAM curves carry extra rise the IOB curve omits, so expect some legitimate under-prediction on meal climbs.

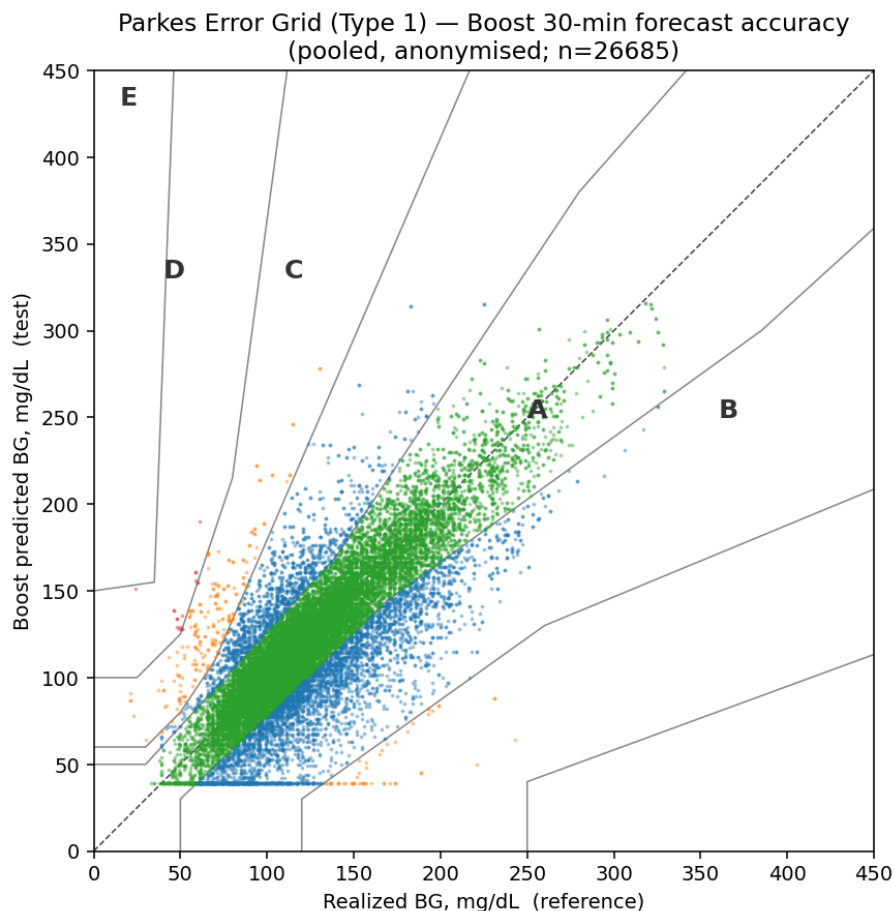

Zone distribution (30-min)

user	pairs	A	B	C	D	E	A+B
self	5908	69.6%	28.6%	1.7%	0.2%	0.0%	98.2%
A	4995	80.2%	19.3%	0.4%	0.1%	0.0%	99.5%
B	4825	78.4%	21.3%	0.4%	0.0%	0.0%	99.6%
C	5791	83.4%	15.9%	0.7%	0.0%	0.0%	99.3%
D	5166	79.6%	18.7%	1.6%	0.1%	0.0%	98.4%
ALL (pooled)	26685	78.1%	20.9%	1.0%	0.1%	0.0%	99.0%

A clinically-accurate predictor shows $\geq 95\%$ in A (regulatory bar for BG meters); A+B is the common "acceptable" threshold. Read these as forecast quality, not meter accuracy.