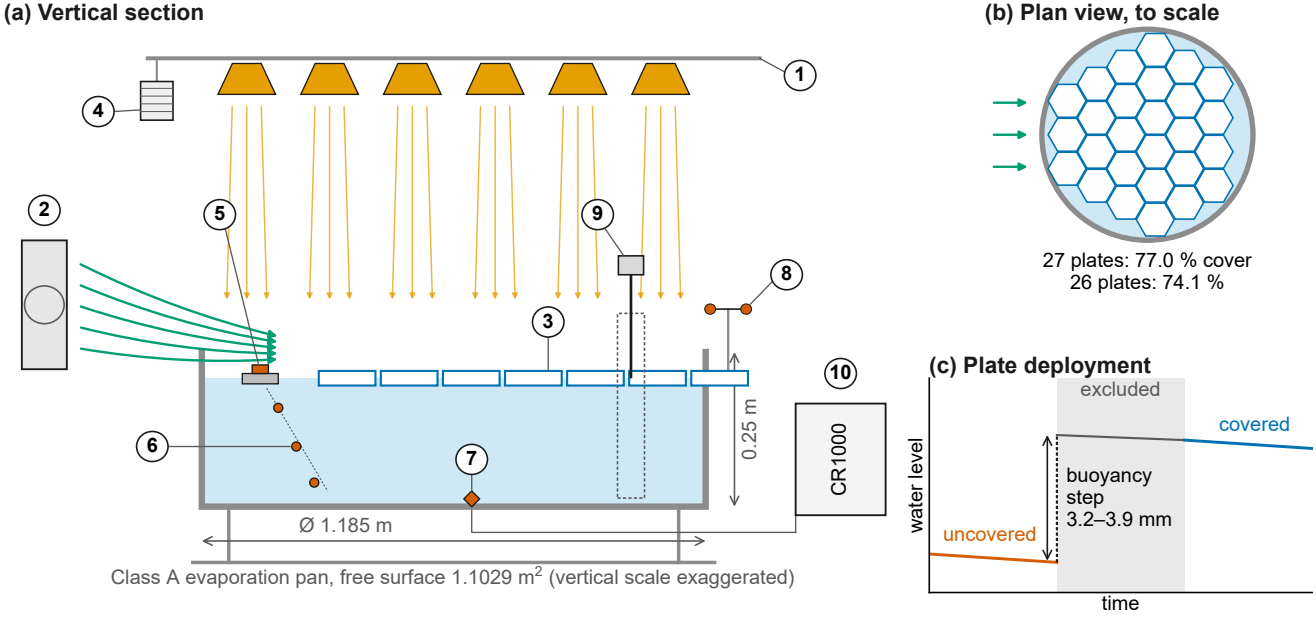


(1) Lamp array: 18 infrared lamps × 250 W, dimmer-controlled

(2) Fan: u = 0, ≈1.9–2.2 or 3.2–3.6 m s^{-1} over the pan

(3) Rigid floating hexagonal plates, 110 mm side

(4) Air temperature and humidity (HMP45C) on the lamp frame

(5) Pyranometer on a float at the surface (SP-LITE; LI200X)

(6) Water temperature, three thermistors (108)

(7) Water level, vented pressure transducer on the floor (QDY30A)

(8) Cup anemometer at the rim (034B)

(9) Micrometer on a stilling well (independent level check)

(10) CR1000 datalogger: 20 s scan, 1 min storage