


Calibration: M4
HL $\chi^2=103.2$, $p=0.000$



Calibration: M5
HL $\chi^2=121.6$, $p=0.000$

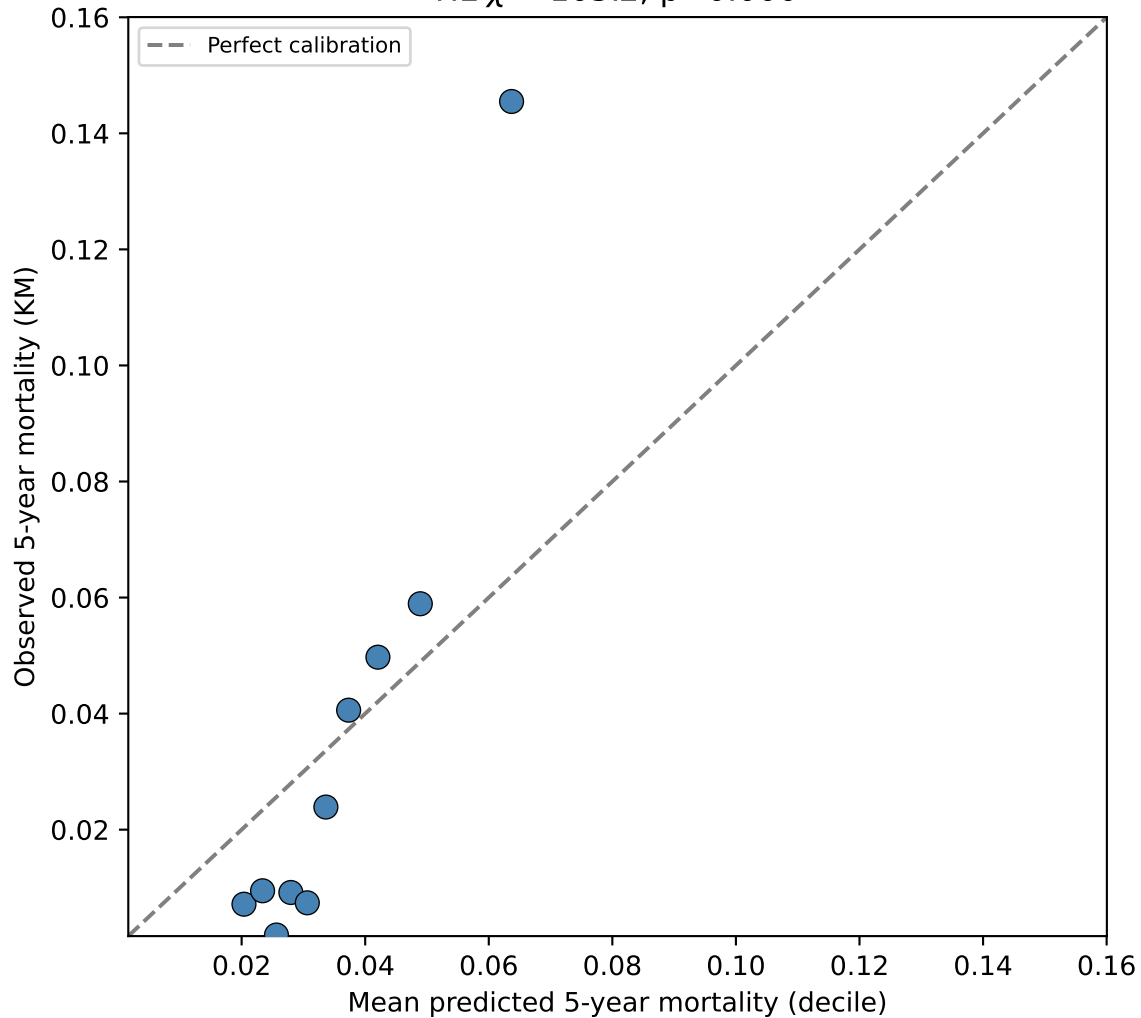