


Finding 7: Calibration and threshold transfer

Target FPR



PACC prevalence MAE

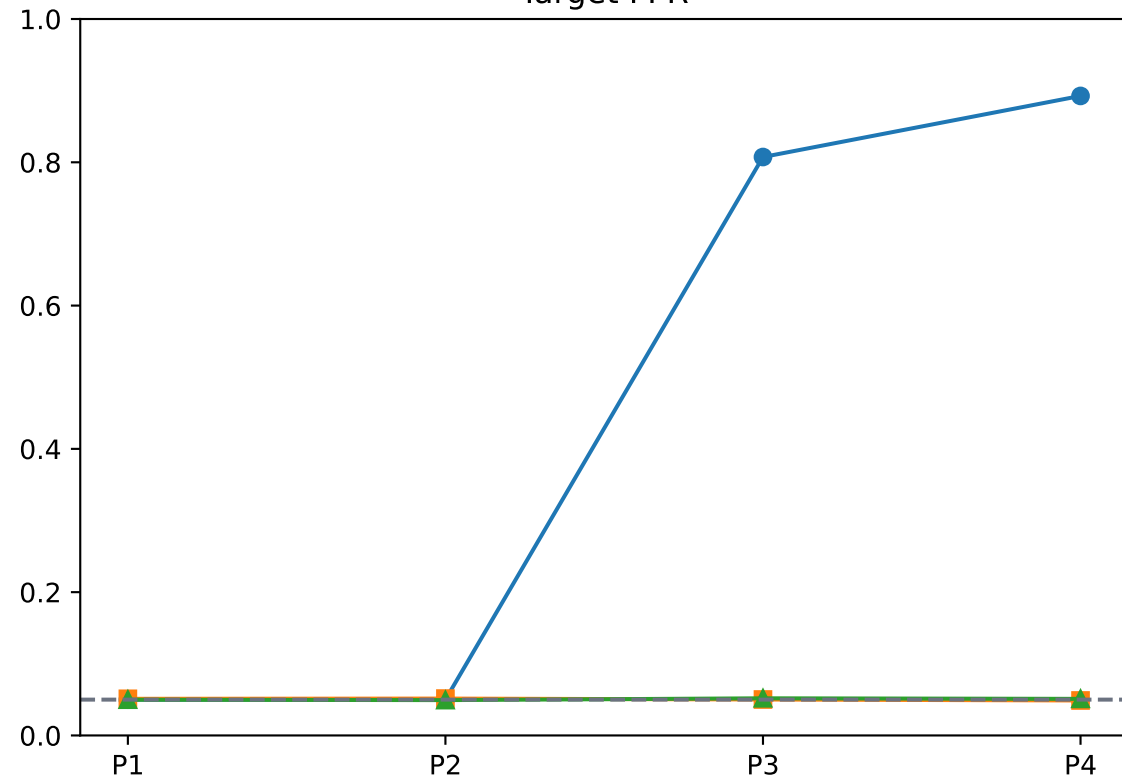