


Lab Notebook Entry from LeCroy DSO
DSO S/N: LCRY3561N17988
User: LeCroyUser
Time: 4/16/2023 12:15:30 AM

MyLabNotebook--00000



LabNotebook

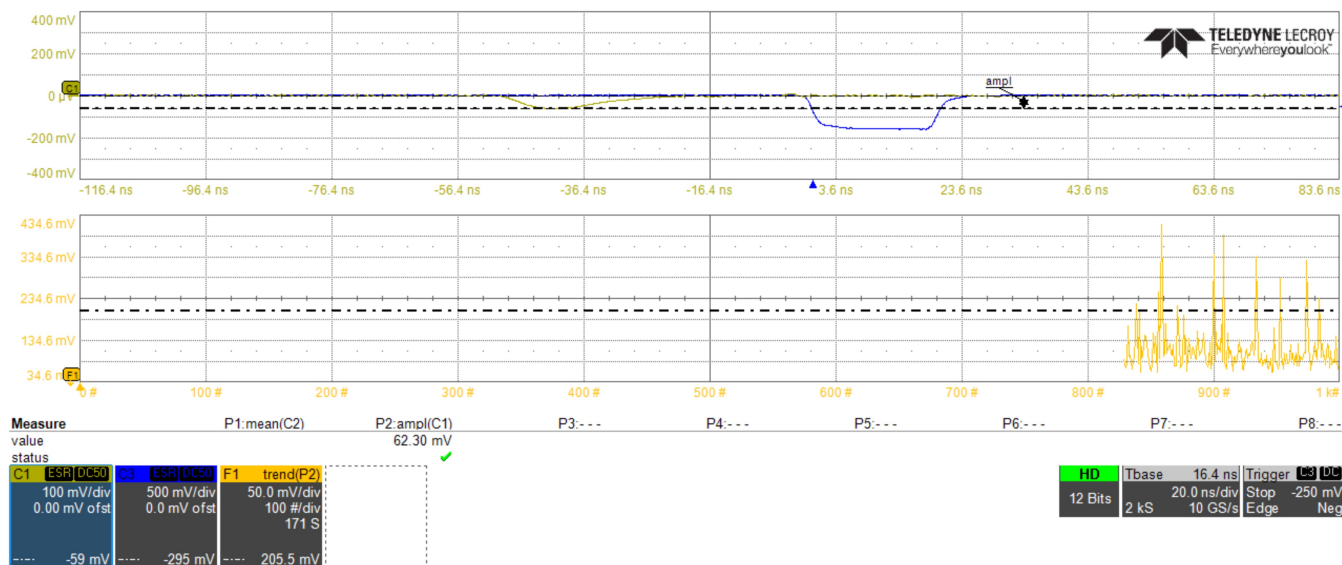

Channel Status

		C1		C3
Vertical	V / Div	100 mV		500 mV
	Offset	0.00 mV		0.0 mV
	Coupling	DC50Ω		DC50Ω
	BW-Limit	FULL		FULL
	Probe	1.000000		1.000000
	Sweeps	1 #		1 #

Acquisition Status

Horizontal	Time / Div	20.0 ns	Sampling Rate	10.000000000 GS/s
	Time / Pt	100.000e-12	Sampling Mode	RealTime
	Pts / Div	200.0 S	Trigger Delay	16.4 ns
Trigger	Mode	Stop	Slope	Negative
	Type	Edge	Level	-250 mV
	Source	C3	Coupling	DC