ВЕТЕРИНАРНА КЛИНИКА
Д-р Марин Величковски

Скопје, Македонија
мобилен: 070/340 846
info@doktormarin.com.mk

Test Report

Species:DOG	ID:123456789	Patient name:DOG-TEST-006
Owner:	Gender:мажјак	Age:0 Years
Analyzer Information: AUTO-GEN	Diagnosis note:	

Report

Item Name	Sample Type	Result(Ct)	Ranges	Indicator	Lot
CDV	oral_nasal_ocular swab	NoCt	>36 or NoCt	Negative(-)	250850
CPIV	oral_nasal_ocular swab	NoCt	>36 or NoCt	Negative(-)	250850
CAV-2	oral_nasal_ocular swab	NoCt	>36 or NoCt	Negative(-)	250850
Bb	oral_nasal_ocular swab	NoCt	>36 or NoCt	Negative(-)	250850
MC	oral_nasal_ocular swab	25.79	>36 or NoCt	Positive(+)	250850
IC	oral_nasal_ocular swab	24.71	>36 or NoCt	Positive(+)	250850

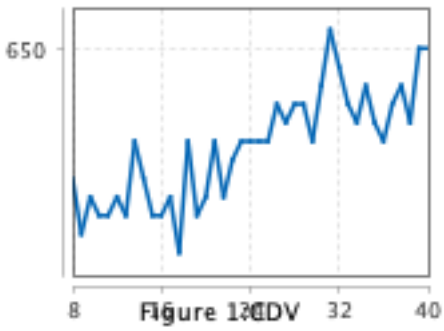

Figure 1:CDV

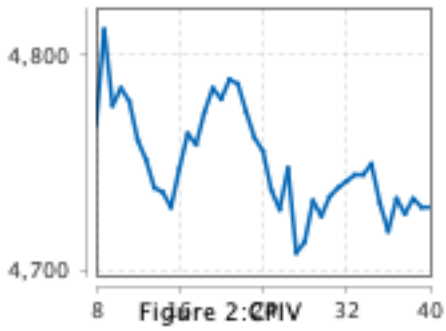

Figure 2:CPIV

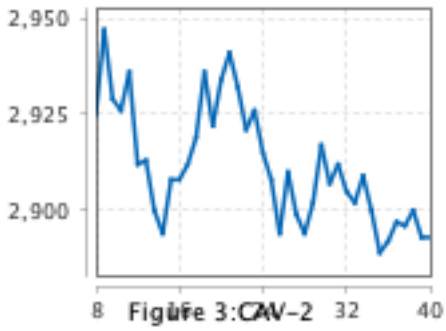

Figure 3:CAV-2

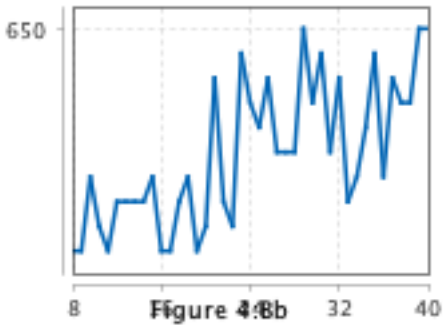

Figure 4:Bb

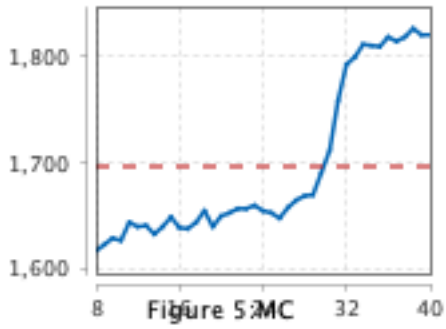

Figure 5:MC

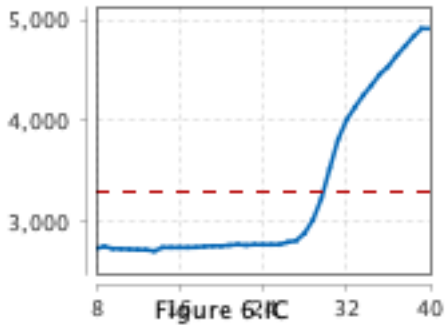

Figure 6:IC

rt Explanation:

': extremely high concentration of pathogens; 17<Ct<=27: high concentration of pathogens;
<=36: low concentration of pathogens; Ct>36: extremely low concentration of pathogens or no pathogens; NoCt: no pathogens;
when it reports Ct>36, there is possibility that the pathogen is not during detoxification period. Comprehensive consideration should be taken in combination with clinical symptoms and other test
:.

:

:est results of this kit are for clinical reference only. Comprehensive consideration should be given to the clinical diagnosis and treatment of patients in combination with pathogen spectrum and
nic status.
en the Ct value is <=36, the detection result is positive.
en the Ct value is > 36 or NoCt , the result is negative
e Ct value is >36. Retest is recommended. If the Ct value is > 36 or NoCt , the result is negative. If the Ct value is <=36, the detection result is positive.

it Datetime: Analysis Datetime:2026-03-03T12:26:26.930091+00:00 Print Datetime:03/03/2026