


DOxy: A Dissolved Oxygen Monitoring System

Navid Shaghghi  0000-0002-7142-827X, Frankie Fazlollahi, Tushar Shrivastav, Adam Graham, Jesse Mayer, Brian Liu, Naveen Govindaraju, Sparsh Garg, Katherine Dunigan, Gavin Jiang, and Peter Ferguson

Ethical, Pragmatic, and Intelligent Computing (EPIC) Research Laboratory
Department of Computer Science and Engineering (CSEN)
School of Engineering (SoE)
Santa Clara University (SCU)
Santa Clara, CA, USA
{nshaghghi, ffazlollahi, tshrivastav, ajgraham, bxliu, ngovindaraju, sgarg3, kdunigan, gyjiang}@scu.edu
{jdmayer, pferguson}@alumni.scu.edu
* Correspondence: nshaghghi@scu.edu;

Abstract: Dissolved Oxygen (DO) in water enables marine life. Measuring the prevalence of oxygen in a body of water is an important step in sustainability efforts because low oxygen levels are a primary sign of contamination and distress in bodies of water. Therefore, fish farms, aquariums, and other aquaculture are in need of near real-time dissolved oxygen monitoring and spend a lot of money on purchasing and maintaining DO meters that are either expensive, inefficient, or manually operated - in which case they also need to ensure that manual readings are taken frequently which is time consuming. Hence a cost-effective and sustainable automated Internet of Things (IoT) system for this task is necessary and long overdue. DOxy, is such an IoT system which utilizes cost-effective, accessible, and sustainable Sensing Units (SUs) for measuring the dissolved oxygen levels present in bodies of water which send their readings to a web based cloud infrastructure for storage, analysis, and visualization. DOxy's SUs are equipped with a High-sensitivity Pulse Oximeter meant for measuring dissolved oxygen levels in human blood, not water. Hence a number of parallel readings of water samples were gathered by both the High-sensitivity Pulse Oximeter and a standard dissolved oxygen meter. Then two approaches were investigated. One, in which various machine learning models were trained and tested to produce a dynamic mapping of sensor readings to actual DO values. And another in which curve-fitting models were used to produce successful conversion formula usable in the DOxy SUs offline. Both proved successful in producing accurate results.

Keywords: Aquaculture Technology; Dissolved Oxygen (DO) Monitoring; Internet of Things (IoT); Sustainable Automation; Water Quality Testing.

Citation: Shaghghi, N.; et al. DOxy: A Dissolved Oxygen Monitoring System. *Journal Not Specified* **2022**, *1*, 0.
<https://doi.org/>

Received:

Accepted:

Published:

Publisher's Note: MDPI stays neutral with regard to jurisdictional claims in published maps and institutional affiliations.

Copyright: © 2023 by the authors. Submitted to *Journal Not Specified* for possible open access publication under the terms and conditions of the Creative Commons Attribution (CC BY) license (<https://creativecommons.org/licenses/by/4.0/>).

1. Introduction

Oxygen from the atmosphere dissolves into rivers, lakes, and oceans and is consumed by aquatic animals for breathing [1]. Dissolved oxygen (DO) is hence considered to be the most important variable of water quality as marine life will suffocate if its levels are too low. Therefore, the aquaculture industry monitors the water circulating through their systems as even slight changes to the water quality can have severe effects on their crops. For instance, poor oxygen management in aquaculture systems can lead to physiological damage and substandard growth in the aquatic organisms being cultured [2] [3] [4] with most organisms sustaining damage when their ambient concentration of dissolved oxygen drops below 5% [5]. As such, proper management of DO levels is imperative and requires a diligent effort in taking DO measurements.

Another reason why DO is such a critical environmental variable is how dynamic it is: over a matter of hours or even only minutes, dissolved oxygen levels can change from optimum to lethal [6]. Therefore, since the response time for taking corrective measures is typically short, it is critical to have a rapid and reliable method of continuously monitoring

DO concentrations so that water facilitators can be proactive in improving the water's quality [6]. There are numerous issues with the current standard methods of measuring DO in water, including affordability, maintainability, and environmental safety - especially with chemical-based meters. Thus, research was conducted on the use of infrared technology as a means to measure DO in water and it was found that infrared sensors were capable of this task while addressing the lack of affordability, difficulty of maintenance, and potential environmental safety issues with the current standard of measuring methods. The preliminary findings were reported in a short 2020 paper with the same title that was presented at the 2020 IEEE Global Humanitarian Technology Conference (GHTC) and published as part of its proceedings [7]. This paper, in part, serves as an extended version of that paper but goes far beyond it.

Sections 2 and 3 detail existing methodologies for measuring dissolved oxygen sensing, and existing research and commercial products respectively. Section 4 delineates how DO was measured in this research as well as how the sensors were calibrated. Section 5 provides the technical setup of the DOxy hardware and software and section 6 reports on the results from DOxy's field testing. Finally, sections 7 and 8 respectively provide the current work in progress by the team and some closing remarks.

2. Methodologies for Dissolved Oxygen Sensing

Two general methodologies for measuring dissolved oxygen in water exist: Electrochemical and Optical.

2.1. Electrochemical

2.1.1. Methodology

There are two types of electrochemical dissolved oxygen sensors: galvanic and polarographic. Both methods utilize two polarized electrodes with differences in reactivity in an inert electrolyte solution that is not part of the reaction. A semi-permeable membrane separates the electrodes and the electrolyte solution from which oxygen diffuses across. dissolved oxygen is reduced at the cathode which causes an electrical current that is carried by the ions in the electrolyte to the anode. The measured electrical current provides information on the concentration of dissolved oxygen due to their direct relation [8]. Both methods work in a similar manner except for that in the galvanic method, there is no need to allocate warm-up time due to the self-polarization of the dissimilar metals used as the anode and cathode, such as zinc and silver. However, in the polarographic method, warm-up time is essential to polarize the electrodes as the metals used, such as gold and silver, do not have a large difference in reactivity [8].

2.1.2. Problems

Although both electrochemical methods have advantages and can return a result quickly, there are a number of inconveniences encountered. Since the electrodes employed in both methods consume oxygen the electrochemical method requires constant maintenance and thus recalibration every two to eight weeks and thus introduces a high maintenance cost and reduces efficiency and reliability- thus making them problematic to employ over sustained intervals [9]. For the polarographic electrochemical method specifically, the electrolyte needs to be replaced, and in the galvanic electrochemical method, the anode needs to be replaced as they are used up in the internal reactions [10]. Additionally, the consumption of the substances results in the sensors having a short lifespan and thus places a high replacement frequency and cost. In addition, the measurement accuracy may be lowered due to interference by certain chemical compounds such as hydrogen sulfide found in some bodies of water that may infiltrate the membrane.

2.2. Optical

2.2.1. Methodology

The optical sensor consists of a semi-permeable membrane, a sensing element, a light-emitting diode, and a photodetector. The sensing element contains a luminescent dye that is immobilized in sol-gel. The dye becomes excited and emits light when exposed to the blue light emitted by the LED in the presence of DO.[8] The intensity and luminescence of the dye when exposed to blue light and the wavelength of the emitted light is dependent on the amount of dissolved oxygen in the water sample. The intensity of the returned luminescence is measured by a photodetector and is used to calculate the dissolved oxygen concentration [8].

2.2.2. Problems

Optical dissolved oxygen sensors usually require more power and take 2-4 times longer to take a measurement than the electrochemical method [8]. These sensors are also heavily dependent on temperature because of the luminescent dye's sensitivity to temperature. The luminescent dye also will eventually degrade. To maintain this type of sensor, one or two calibrations per year and a replacement cap every 18 months is needed [11]. Although the optical sensor has a lower maintenance cost, it has a greater acquisition cost which fish farmers and others small producers in the aquaculture industry may not be able to afford.

3. Related Works

3.1. Academic Research

3.1.1. Utilization of Lightwaves for measuring DO in Water

Zhao et al. used light in fluorescence quenching to measure DO [12]. The team coated an optical fiber with a fluorophore, Trisaminomethane Ruthenium (II) Complex Dichloride, that quenched in the presence of DO. Light was sent down the fiber and the returning light was measured and used to derive the partial pressure of DO in the solution using the stern-volmer equation. To compensate for the brightness fluctuation inherent in the light source, the team coated the tip of the optic fiber with CdSe/ZnS quantum dots, allowing them to quantize the fluctuation and to calibrate their results. The collected data, when regressed onto the line predicted by the stern-volmer equation, was able to achieve an R^2 of 0.9957.

Yu et al. [13] created a quenching-based DO sensor specifically for the measurement of DO in the range of 1m and below. They were also concerned with the common use of transition metal complexes in DO sensing, since they cost a lot and are potentially toxic. For this reason Yu et al. chose to use metal-free organic phosphors, which, just like transition metal complexes, have long decay times. A challenge was the inundation of room temperature fluorescence in metal-free organic phosphors, since this requires particular conditions. The team ended up creating shell-core nanoparticles. The core was comprised of the metal-free phosphors embedded in a matrix of polystyrene (chosen because of its oxygen permeability). Poly(2-Methyl-2-Oxazoline) was chosen as the outer shell for its water solubility and biocompatibility. Upon testing, the nanoparticles were found to be particularly sensitive to the presence of oxygen. When dispersed within water containing DO and exposed to UV light, the nanoparticles exhibited very little fluorescence. As the water was sparged with nitrogen, the nanoparticles gradually became more fluorescent.

Miura et al. [14] studied the absorbance levels of DO for different wavelengths. Tests were conducted on both tap water and seawater, with samples from each type of water brought to 100% DO through aeration and 0% DO through reduction by sodium-sulfate. From the 108 samples of sea water and tap water tested on, they found that the greatest variance in absorbance occurred in the blue and infrared wavelengths of light and likely to be most detectable under blue light. The researchers then built a prototype sensor and conducted three tests on it. In the first test, both the LED and the photodiode were exposed to saline water. The researchers found that in this case, contact with the saline water

significantly effected experimental results. For the second and third tests, one component was kept dry while the other was exposed to saline water. In the second and third tests, where only the LED and only the photodiode were exposed to saline water respectively, only a small effect on the results was noted. The researchers thus concluded that it was important to separate the water being measured from touching the sensor.

3.1.2. Use of Machine learning in calibration of DO sensing

Zhang et al. [15] investigated the use of machine learning in the calibration of DO sensors. The team built an apparatus for sensor calibration, a chamber filled with ultrapure water in which an oxygen sensor, to be calibrated, and a reference sensor were suspended. The design of the apparatus allowed for the control of the DO concentration, the salinity, the temperature, and the pressure within the chamber. A small tube brings water from the chamber as an analyte for winkler iodometric titration analysis in order to allow for constant monitoring of the DO concentration. The collected data is then fed to a backpropagation neural network, which is run for a thousand iterations. When the calibrated model was finished, the team compared the accuracy of a quenching DO sensor to that of winkler analysis. The R^2 of the model was 0.99971, while the R^2 of traditional winkler analysis was 0.99839. When its performance was compared with that of an Anderaa sensor, the quenching DO sensor was found to produce results that were reliably similar.

Silva et al. [16], concerned with the use of nonrenewable transition metal complexes in quenching DO sensors, derived transition metal complexes from kale with chemical techniques. The extracted transition metal complexes, chlorophyll-zinc complexes, were immobilized in a thin film of sol-gel, as per standard procedure for the construction of quenching DO complexes. The thin film was put over the surface of a sample of water. An LED emitted blue light at it, and a photodiode received the light. The characteristic wavelength of chlorophyll-zinc complexes was determined to be 635 nm. When the DO concentration was made homogeneous across the analyte with a stirrer, the R^2 of the zinc chlorophyll complexes, when they were used for DO sensing, was 0.98282.

Michelucci et al. [17] modified quenching O_2 sensing with . Typically, the magnitude of the quenching is related to O_2 concentration with the stern-volmer equation, but the team trained an AI model to notice the correlation instead. The team utilized a commercial Pt-TFPP quenching-based sensor in a thermally controlled chamber in which the O_2 concentration could be varied and homogenized across the chamber. The authors used a feedforward neural network to relate several variables within the chamber to the O_2 concentration within it. Because of the paucity of extensive empirical datasets with respect to dissolved oxygen sensing, the team was forced to procedurally generate data with theoretical knowledge. The neural network was ran for three different network architectures and the mean absolute error (MAE) was calculated over each of them as they were given more layers and neurons, thus increasing in complexity. Two of the neural networks approached a minimum MAE of 0.012% on account of most of the data being theoretically generated. The third network stabilized at an MAE of 0.5%.

3.1.3. IoT DO sensing

Yunfeng et al. [18] noticed a trend in oxygen-controlling equipment for aquaculture: they were black boxes that did not transmit data to their users. To remedy this, the team developed an IoT platform to support the real-time monitoring of DO levels in fish ponds. The team deployed several sensors with each unit endowed with an electrochemical DO sensors, a temperature sensor, and a narrowband sending system. The device transmits data at intervals before returning to low-power mode.

Stine et al. [19] developed a system for gathering real-time data on the topology of oxygen distribution within a bioreactor. To achieve this they designed DO-measuring IoT sensors to be dispersed through the aqueous contents of a bioreactor. The sensors were designed to contain electrochemical DO detectors. Each sensor contained a potassium chloride electrolyte with a thin-film gold working electrode, a gold counter electrode,

and a silver reference electrode. The researchers communicated with the device network using a smartphone app, Silicon Labs, which allowed them to turn all the devices in the network to a low energy setting, calibrate the devices, and had the devices make intermittent measurements. A pod was placed in a 10 liter bioreactor filled with De-ionized (DI) water in order to test it. Oxygen and nitrogen gas were pumped into the DI water before it was stirred with an impeller. A cyclic voltammogram found that cathodic current was maximized when the potential was between -0.4 and -0.6V. Using a value in this range, -0.42V, the researchers used chronoamperometry to determine that there was an average difference of 2.5A in current between when the solution was diluted with gas and when it was sparged with nitrogen gas. Tethering the pod to a 3.3V power supply, the researchers calibrated the pod on -0.5V every 30 seconds at several different oxygen levels. Using this data, the researchers were able to obtain a calibration plot mapping the oxygen levels in the solution to the voltage outputted by the pod. The correlation between the two quantities was found to have an R^2 of 0.98, a sensitivity of 37.5 nA/DO%, and a limit of detection of 8.26DO%. Finally, the researchers tested the pod while the bioreactor ran a fermenter in order to more closely simulate a working environment. The voltage outputted by the pod was found to increase linearly and inversely proportionally with DO% concentration, showing that it had been successfully implemented. Some problems still remained, however. For the first 45 minutes of the test, the difference between measurements by the pod and a polarographic DO sensor, which had been introduced into the bioreactor as a control, was less than four percent. As the bioreactor continued to operate, however, the difference began to shift, which the researchers suspected was due to the degradation of the reference electrode after continual usage. In response the researchers fitted the sensors with several design improvements. Since the inaccuracy grew linearly with time, they applied a correction factor to multiply the pod output with to refactor the results back down to under the four percent range.

Hu et al. [20] observed that aquaculturists typically monitored DO levels by observing fish behavior, something that could only be done after fish had been affected by deleteriously low levels of DO. To remedy this, they engineered a Radial Basis Function Neural Network and trained it on data from aquaculture ponds in Zhenjiang, China. To optimize the Neural Network, a genetic algorithm was run on it. When compared with real data, the model showed high prediction accuracy.

3.2. Existing Products

Currently, the existing dissolved oxygen meters on the market are expensive, have high maintenance costs, or do not have wireless communication integrated into the device to enable continued remote monitoring of the dissolved oxygen levels.

For instance, Cole-Parmer which is a well known scientific and industrial instrument distributor has an array of costly dissolved oxygen Meters ranging from \$265 to \$2459 [21] at the time of this writing. Additionally, although their products have advantages such as features that allow calibration and measurement data to be stored with a timestamp, the meters have high maintenance costs due to replacements of the chemical solutions, membranes, and caps of the measurement probes. And most importantly, the devices offered are handheld and do not provide continuous monitoring in real time.

A similar company, Hanna Instruments, offers dissolved oxygen monitors with costs ranging from \$220 to \$1450 [22] at the time of this writing. Their products are also high maintenance as the solutions, membranes, and probe caps needed to be replaced. Because wireless communication is not offered, testing on site is required and the device can not provide continuous monitoring.

Such devices that do not include long range wireless communication, hinder fish farmers from having the ability to detect variations in oxygen levels instantly and continuously. Therefore the farmers need to manually measure the dissolved oxygen levels several times per day which increases the amount of manual labor and reduces efficiency. Manual measurements are not only time consuming, they may also be inaccurate especially

if the meters used are not calibrated and maintained correctly. Another advantage of an automated system would be the continues calibration and monitoring of individual sensors within the system which can also alert users to the malfunctioning of a sensor and or even diagnose the problem with the sensor(s) so that the technicians can repair or replace the faulty sensor(s).

4. Measuring Dissolved Oxygen (DO)

4.1. Data Collection

Various water solutions of differing dissolved oxygen levels were created and used to gather readings from the MAX30102, High-Sensitivity Pulse Oximeter sensor [23]. A Milwaukee MW600 Portable Dissolved Oxygen Meter [24] was used to measure the dissolved oxygen content of each water solution in parallel in order to equate the readings.

4.1.1. Water Sample Creation

At first, various local tap, bottled water, and deionized water supplies were used. After some experimentation, deionized water was determined to perform the best due to being free of any substances that could absorb the infrared wave of the Oximeter and thus result in inaccurate readings.

Samples were created to provide a sizable range of values between 0% and 100% dissolved oxygen in the water. A zero dissolved oxygen solution was created by mixing deionized water with sodium sulfite as it acts as an 'oxygen scavenger'. Sodium Sulfite reacts with the dissolved oxygen and forms sodium sulphate as seen in equation 1, which does not affect readings of the Infrared Sensor.



Thus, multiple different samples between 0% and 100% were created by simply using the ratio of 2 molecules of Sodium Sulfite to 1 molecule of dissolved oxygen. Furthermore, as the dissolved oxygen content of the solution increased gradually by being exposed to the open air over several days more readings were taken at various intervals by both the sensor and meter.

4.1.2. Data Gathering Process

The MAX30102, High-Sensitivity Pulse Oximeter sensor is not water proof. Hence, thin plexiglass [25] with a thickness of 1/32 of an inch was utilized to create a barrier between the sensor and water samples. To hold the sensor and plexiglass firmly together, a 3D printed apparatus was designed and utilized as can be seen in figure 1.

The sensor is attached to a threaded component that screws into the plexiglass component so that the sensor would not move while gathering readings, and to prevent any air from being trapped in between the sensor and the plexiglass. Then one of the water solutions was poured into the pale until the water completely submerged the plexiglass chamber, ensuring that the sensor's light would be solely transmitted through the plexiglass and water. Next the 2.5mm cap was screwed on the side of the plexiglass, to create a chamber with a set distance for the sensor's light to reflect back from. Screwing in the cap after the water was set ensured that there were no air bubbles in the chamber to interfere with readings. Then, the red LED and infrared readings that the sensor provided were collected. This method was used for each of the water solutions with differing dissolved oxygen content and compiled into a spreadsheet to be used for analysis and regression.

4.2. Data Analysis and Machine Learning

The data collected from testing the MAX30102 sensor in water samples of varying dissolved oxygen levels was compiled into a tabulated dataset to ease analysis and regression. The columns of the dataset consisted of the dissolved oxygen content, in mg/L obtained from the MW600 readings, the red LED reading from the MAX30102 sensor, and the infrared reading obtained from the same sensor. The size of the dataset was 800 samples,

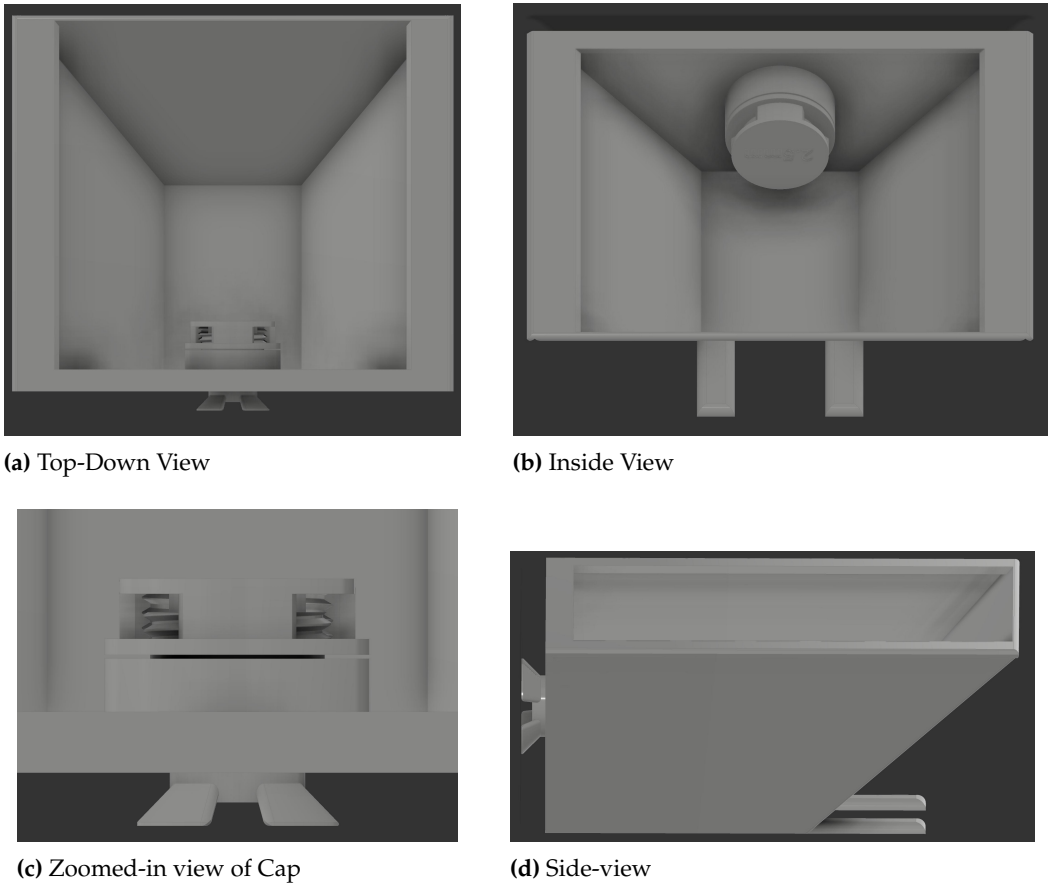


Figure 1. DOxy Testing Setup

comprising 100 readings from each of the water samples. Upon plotting the relationship between the red LED readings and DO levels, it was found that, generally, as the red LED value increased so did the DO level, as can be seen in figure 2. However, there was noticeable overlap between some of the red LED values that had differing DO levels.

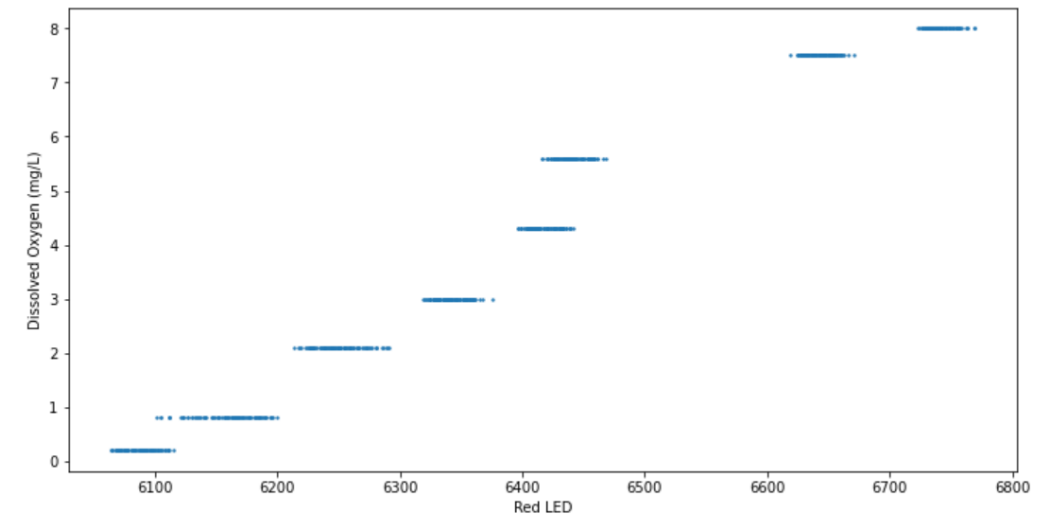


Figure 2. Scatter graph of Red LED data.

Plotting the relationship between the infrared readings and DO levels revealed a similar trend where as the infrared values increased, the DO levels also increased, with no samples

of the same infrared levels having different DO levels, as portrayed in figure 3. These results correlate with the findings of Miura et. al [14].

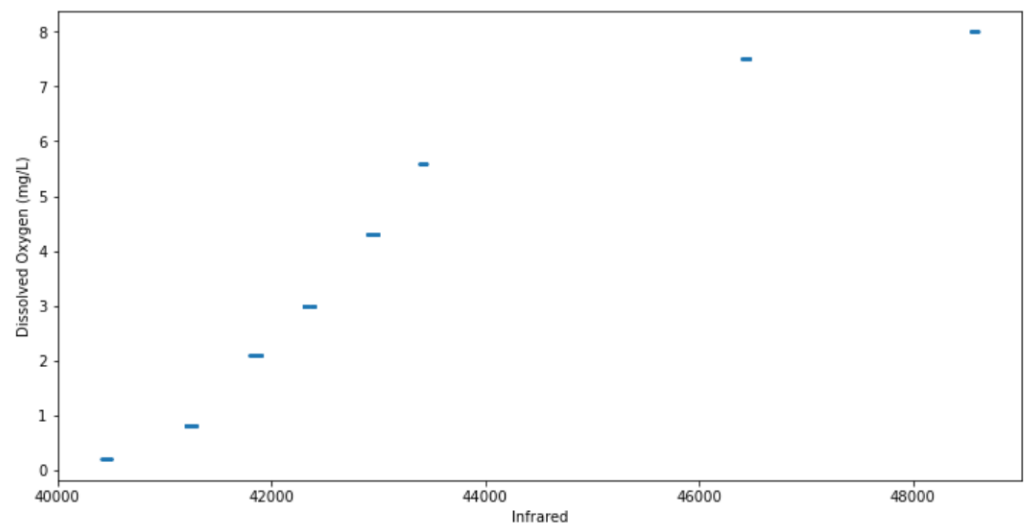


Figure 3. Scatter graph of Infrared data.

The dataset was then split into 70% for training and 30% for testing various machine learning regression models. The models used were sklearn's linear regression, and support vector machine regression (SVR) with a radial basis function (RBF) kernel. Each model was trained once with red LED data, once with the infrared data, and once with both red LED and infrared data, to determine which of the sensor data performs the best for converting to DO content. A 10-fold cross validation was used on the training data for both of the regression models. The SciPy library's curve_fit was also utilized with quadratic, cubic, and quartic equations in an attempt to obtain an equation that would be easily visualized, unlike SVM with an RBF kernel.

4.3. Formulation

Upon analysis from the 10-fold cross validation for the linear regression and SVM models, linear regression only outperformed the SVM model on the dataset using both red LED and infrared data, with a mean squared error (MSE) of 0.226, compared to SVM's poor MSE of 0.938, as depicted in figure 4a. Figure 4b shows the MSE on the solely red LED dataset, where linear regression and SVM performed decently having MSE of 0.247 and 0.097 respectively. The best performing model was however derived from the infrared dataset, shown in figure 4c, where linear regression performed poorly with a MSE of 0.818 but SVM had an outstanding MSE of 0.013.

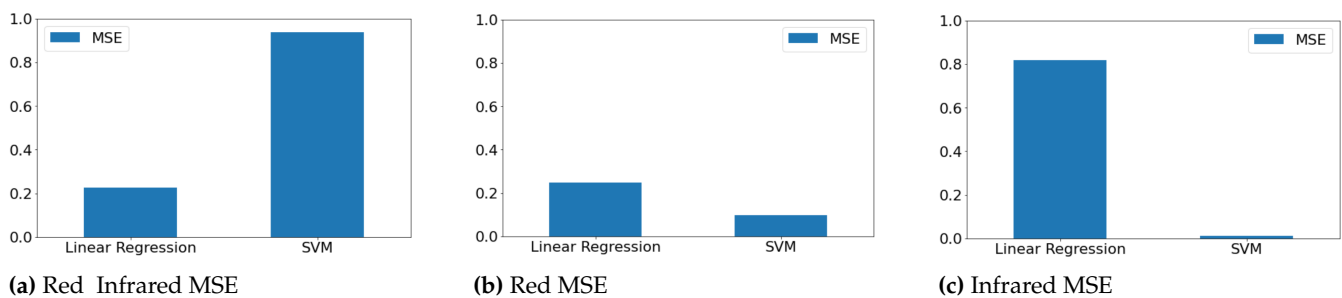


Figure 4. MSE Visualizations

For the curve_fit functions, as expected, the higher degree functions had a lower MSE and higher r^2 score. The quadratic, cubic, and quartic functions had MSE of 0.156, 0.148,

and 0.012, and r^2 scores of 0.979, 0.980, and 0.998 respectively. While the quartic function performs the best, it likely would not generalize well to outside data as its function likely overfits to the training dataset used here. It would be more practical to use the quadratic or cubic functions as they would likely generalize better to outside data. Each of the functions and their respective parameter values are shown in Figure 5.

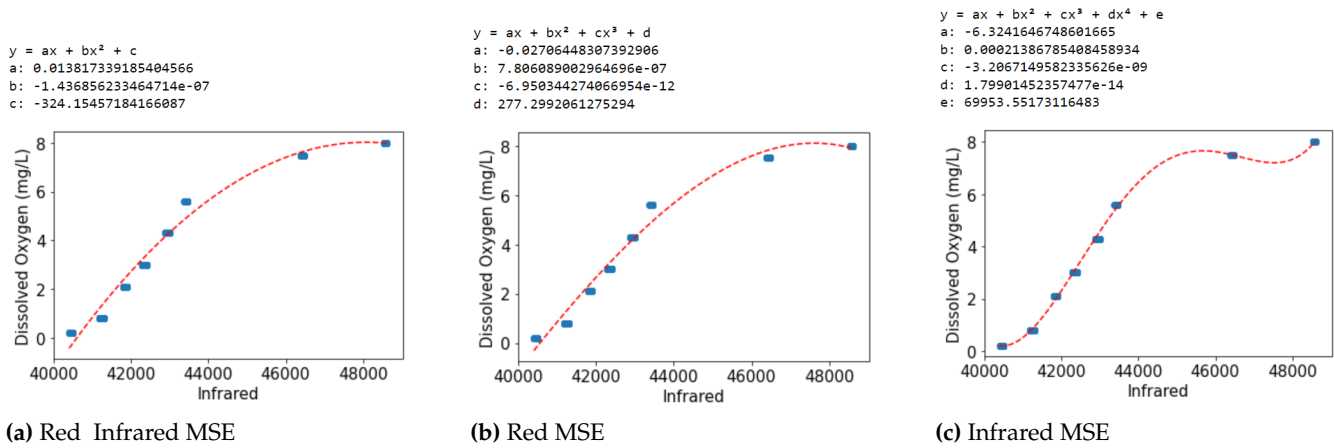


Figure 5. MSE Visualizations

5. DOxy Meter

Using the aforementioned derived formulas, an IoT meter named DOxy (short for Dissolved Oxygen) was constructed and tested in both the lab and real world settings. DOxy leverages the quenching effect that dissolved oxygen has on the fluorescence of a beam of light fired at water, an approach that allows DOxy's Sensing Units (SU)s to be small and cost-effective as well as passive with respect to observed systems, promoting its long-term deployment.


5.1. Electronics

DOxy was created in tandem with the Modular IOT Platform reported on in [26]. There are two versions of DOxy's electronics, one that can be used as a standalone product and the other that can be plugged into existing products. The standalone version is powered by a Wisen Whisper Node [27] micro-controller with an on-board LoRa (Long Range) [?] communication module [29] with 3DBI Omni-directional long range external antenna [30], a DHT11 Temperature and Humidity Sensor [31], a TP4056 battery charge controller [32], a 5W lithium battery pack, and a 5V 100 mAh solar panel. Using a solar panel makes the system more flexible in where it can be installed, as it does not require hard-lined power in order to work. The standalone version contains a MicroSD card adapter module [33] to enable local storage of data and resilience in the case of network failure or device failure. This also allows for storage of things like a device ID or other information about the system. A schematic of the standalone hardware can be seen in Figure 6.

The Plug and Play (PnP) version is similar to the standalone version, but instead is powered by a Arduino Nano micro-controller [34] and connects to the host device using a Cat-6 cable with an RJ45 Connector. There is no battery module or ambient temperature sensor included on the PnP version. A schematic of the PnP hardware can be seen in Figure 7.

5.2. 3D Printed Casing

The DOxy device is housed in a PolyEthylene Terephthalate Glycol-modified (PETG) [35] [36] [37] 3D printed casing prototyped and tested first in [7] and then enhanced as shown in Figure 8a, which keeps the device buoyant and waterproof utilizing the best



practices described in [38]. A primary gasket also 3D printed in PETG is used to waterproof the connection between the case's lid and main body. The hole in the top of the case's lid holds a cable gland for the communication and power cables that connect to the antenna and solar panel respectively. The next section under the lid is a specialized compartment that houses the PCB and waterproofs it with another gasket that connects it with the lid of the case. A secondary cable gland protrudes from the bottom of the PCB compartment to waterproof the sensor cable and direct it into the sensor housing.

The sensor housing consists of three main sections as shown in Figure 8b. The first section holds the sensor, with 3 small screw holes on the bottom to ensure the sensor is firmly secured. The sensor holder is then threaded into the plexiglass lens housing to ensure the sensor is completely parallel to the lens. The lens housing has the lens inserted at the very bottom where the threading ends internally. A gasket is inserted into a rim near the bottom of the lens housing to ensure the sensor assembly is waterproofed. And the final section provides a backdrop for the light from the sensor to reflect off of. This backdrop section is screwed on to the external threading of the lens housing and has large opening along three of its sides in order to ensure air bubbles are not present between the lens and the backdrop.

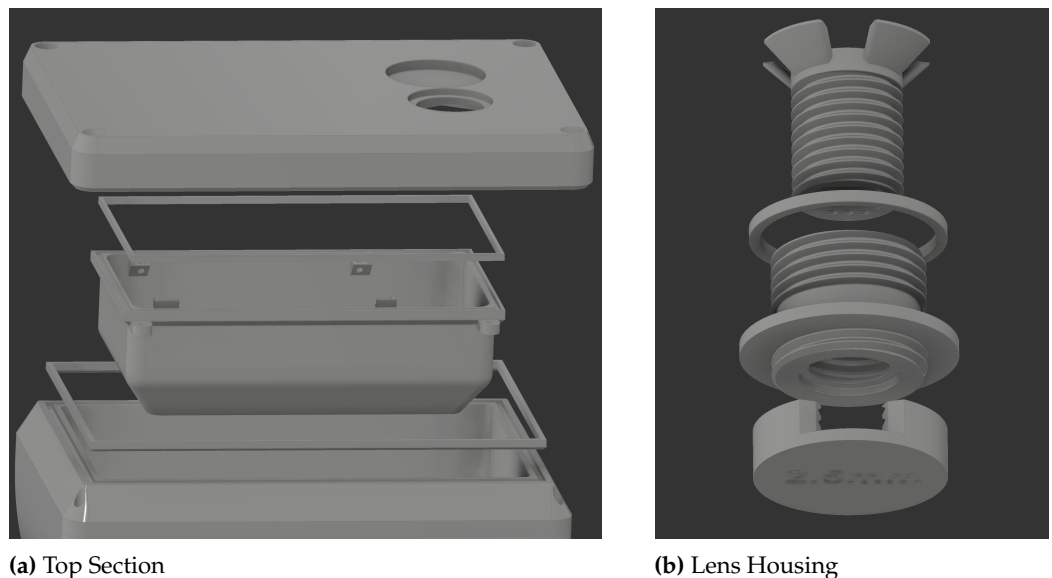


Figure 8. 3D Printed Casing

5.3. Communication

The standalone DOxy system SUs are capable of transmitting their measurements to the web based dashboard in several different ways which is dependent on the environment they are being set up in.

5.3.1. Single-hop communications

For instance, if they are set up in a facility with ample WiFi availability or in the backyard of home hydroponic system within the home WiFi signal range, then the SUs use an ESP8266-01 WiFi module [39] to send a POST request containing JSON sensor data to the web server through the internet. But if for instance the SUs are in a remote location where maybe only Cellphone service is available, then they can be quipped to utilize the GSM network instead.

5.3.2. Multi-hop communication

For bigger or more remote operations where WiFi and/or GSM are not available, the SUs could send data to a Base Station (BS) which could be responsible for compiling various

sensor data from multiple SUs in one site or several sites and relaying this information to the web dashboard and/or handling any actuation capabilities the system may be configured to perform given the various possible DO level readings. In this scenario, numerous wireless communication technology can be utilized between the SUs and the BS such as Zigbee, nrf, LoRa, or even WiFi based on their distance, line of site, and other environmental factors.

For handling this type of communication, the DOxy system uses an in house built Energy Aware Communication Protocol (EACP) named $\hat{A}b$ [40]. $\hat{A}b$ is a responsibility protocol which sits between layers 2 and 3 of the TCP-IP communication stack and thus provides layer 2 agnostic end-to-end communication capable of utilizing the low energy sleep mode of all the network hops and not only the initial transmitter and/or final receiver of the data packets. $\hat{A}b$ is currently in use in the Hydration Automation (HA) system [41] and Smart Tanks where LoRa is utilized to transmit the water level of water tanks in use for agricultural purposes to a pumping station; as well as in another implementation of DOxy in both a deeply forested areas necessitating many short range Zigbee hops from a river in Malaysia to a near by research lab at a school [42] and an ROV in a lake communicating to the shore and then a research facility using MQTT [43].

5.4. Web Based User Dashboard

In order to effectively collect and present data from DOxy SUs, a comprehensive dashboard system was developed. The dashboard is composed of a data access layer (backend) composed of a database and an Application Programming Interface (API) for posting/fetching values to/from the database, along with a presentation layer (frontend) Graphical User Interface (GUI). The SUs report their measurements to a base station, which then makes an HTTP request to the backend API in intervals configurable by the user. The various sensor readings are stored in the database. And the frontend allows for easy visualization and analysis of the data, with clear and concise graphs and charts.

5.4.1. Tech Stack: Data Access Layer (Backend)

The backend API is built using Node.js which is a popular and efficient JavaScript platform for building server-side applications. Node.js allows for fast and scalable network applications, making it an ideal choice for DOxy and IoT systems in general. The backend of the system is launched as multiple independently maintainable and expandable microservices using Docker [44] in order to add flexibility and scalability to the system. And in order to facilitate communication between the sensors or the base station, and the dashboard, the backend uses both an HTTP request and a WebSocket. The HTTP protocol allows for the transmission of data between the backend and frontend, while the WebSocket connection allows for live data display and receiving information from the base station.

The database used in the system is TimescaleDB [45], which is a time-series database optimized for storing and querying large amounts of time-stamped data. It is built on top of PostgreSQL and can handle high write and read loads, making it well-suited for storing data from IoT sensors that generate large amounts of data over time. The database consists of tables with user IDs that store sensor data for each user, with a schema for each type of sensor (DO, temperature, etc.). The schema defines the structure of the data stored in the table, including the names and data types of the columns, as well as any constraints or indexes on the data. By using a schema for each type of sensor, we can ensure that the data from each sensor is stored in a consistent and organized manner. The database is pseudo-schema-less though in that an external command-line interface (CLI) tool (built with Rust) is used to add new schemas to the database when new sensors (such as for measuring atmospheric pressure - as discussed in the work in progress section) are added to the system. This means that new sensors can be added to the system without having to modify the underlying database schema, which is a more flexible and scalable approach.


The backend service was deployed on an Amazon Web Services (AWS) EC2 instance as a Docker container, orchestrated by Docker Compose. EC2 is a cloud computing service offered by AWS that allows users to run applications on virtual machines in the cloud in

order to abstract away all of the setup and maintenance needs for the backend environment, and docker Compose is a tool that allows the definition and execution of multi-container Docker applications, making it easier to manage and deploy the service.


5.4.2. Tech Stack: Presentation Layer (Frontend)

For the frontend, the svelte [46] JavaScript web framework was utilized, along with Chart.js, in order to create a user-friendly interface for displaying sensor readings. Svelte is a modern framework that provides an efficient and reactive way to build user interfaces with responsive layouts, allowing for seamless use on various devices with various screen sizes. Chart.js is a powerful JavaScript library that allows for the creation of visually appealing and interactive charts, allowing users to easily analyze the data from the sensors. Technically though, Svelte has a Server-Side Renderer (SRR) which is set up as another microservice in the backend. SRR is a technique that renders the generated HTML on the server rather than in the client's browser which improves the performance of the web application, as the rendered HTML can be sent to the client faster than the client's browser could render the HTML code itself.

The authentication system supporting login functionalities with Google accounts as well as phone number login were added in order to separate and secure user data. When a user logs in with their Google account or phone number, the system verifies their identity and grants them access to the dashboard based on their credentials. Figure 9a shows an example of the post authentication welcome screen. The dashboard also allows for easy navigation and filtering of data, allowing users to focus on specific aspects of the data. For instance, the user can navigate to any of their sensors in order to see data from the sensors displayed in clear and concise graphs and charts as depicted in Figure 9b. Each sensor object on the dashboard has a set of instructions on how to display its data. For example, a sensor may display water oxygen levels as a line chart when in focus, and as a pie chart with a percentage when minimized. This allows for the customization of the visual representation of data based on the specific needs and characteristics of each sensor.

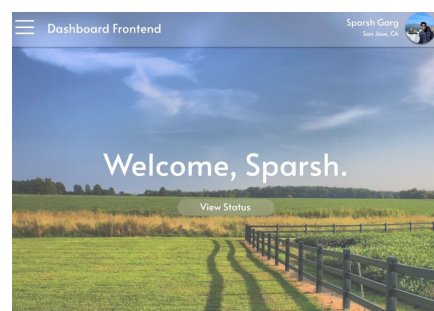

(a) Welcome Screen

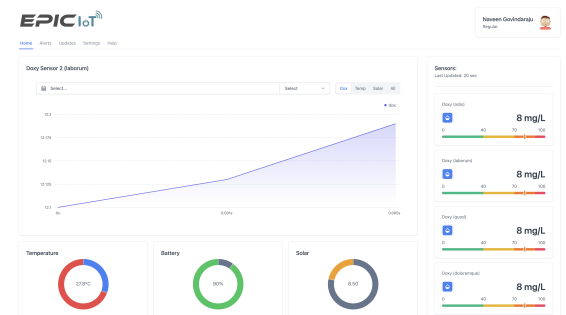

(b) Dashboard

Figure 9. Dashboard GUI

6. Results

Through a number of parallel readings of DO levels in water samples by both DOxy's High-sensitivity Pulse Oximeter and a standard dissolved oxygen meter, two approaches were investigated: One, in which various machine learning models were trained and tested to produce a dynamic mapping of sensor readings to actual DO values in the lab as discussed in section 4.3 in detail. And another in which curve-fitting models were used to find the best fitting curve for producing a successful conversion formula that was then programmed into the DOxy SUs to be used offline. The DOxy SUs were repeatedly tested in buckets filled with tap water, random water fountains on the Santa Clara University's main campus, and a nearby lake, all with accurate DO readings as confirmed with parallel readings with a DO meter.

In all cases, the sensor oscillated and then settled down on the correct reading once in the water for a few seconds. As an example, figure 10 shows the oscillation and subsequent settling down on the constant reading of 8 mg/L of DO when the SU was placed in one of the water fountains on the SCU campus.

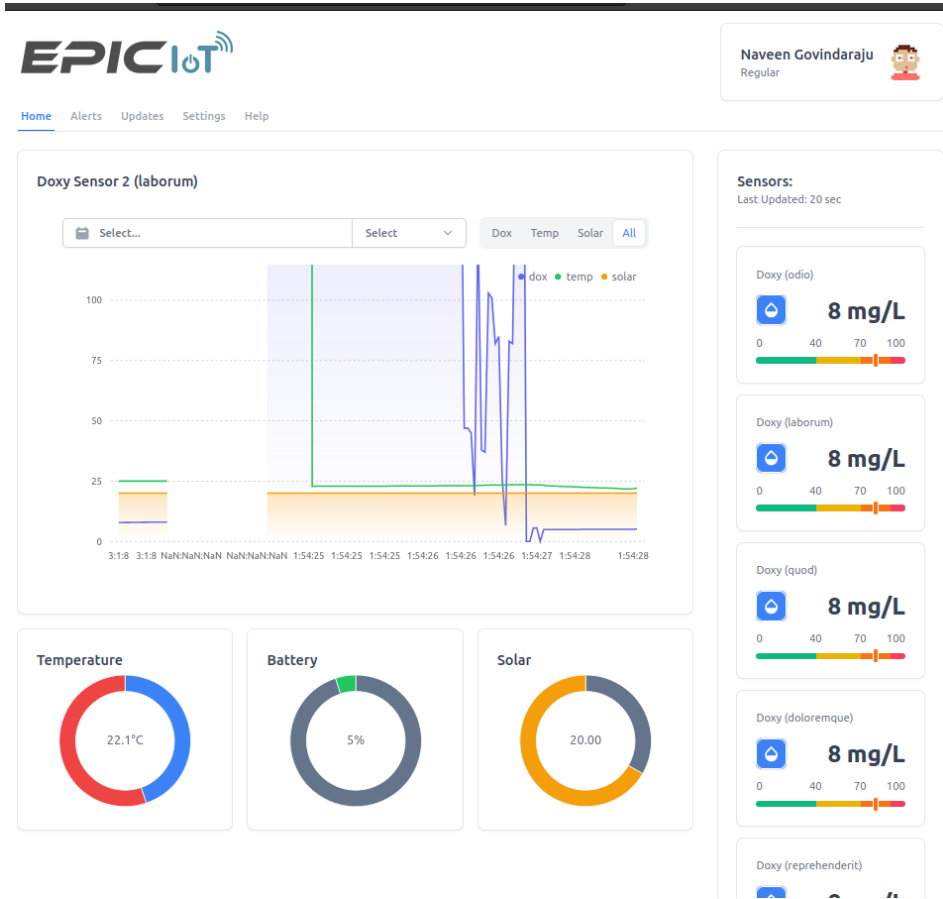


Figure 10. DOxy Results Displayed on the Dashboard

7. Work in Progress

Several theoretical and technical directions for improving measurements are under exploration and development as reported on in this section.

7.1. Effects of Temperature on DO measurements

Variance in temperature can effect the concentration of dissolved oxygen in water [47]. The colder the water is the higher concentration of dissolved oxygen it can hold [47] thus the temperature and dissolved oxygen concentration is inversely proportion. As displayed in figure 11 there is a significant drop of concentration of dissolved oxygen between colder months and warmer months.

Because the data collection performed to build the machine learning models used in DOxy was done at room temperature (20–22 °C), it is necessary to account for the temperature variation when applying the models to real-world scenarios. By understanding the relationship between temperature and dissolved oxygen concentration, the measurements can be adjusted in order to reflect the conditions of the surrounding environment.

To convert the room temperature DO measurement to the DO concentration at the surrounding temperature, an oxygen solubility chart can be utilized in order to supply the solubilities for the van't Hoff equation [48]. The van't Hoff equation 2 is a thermodynamic equation that relates the solubility of a gas in a solvent to temperature. It provides an approximation of how the solubility of a gas changes with temperature under certain

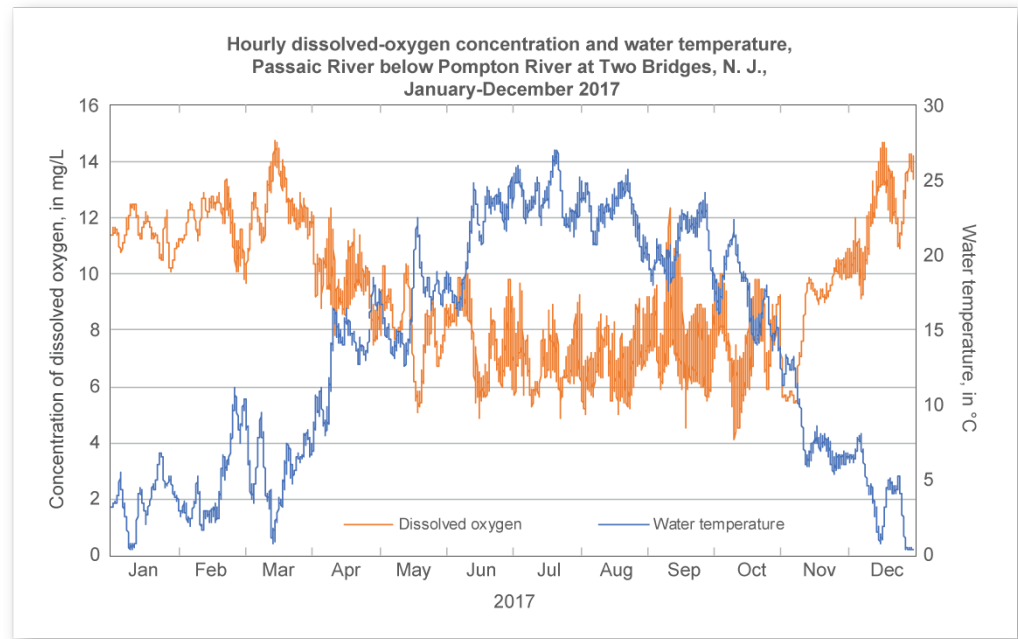


Figure 11. USGS Sample chart showing the effect of temperature on dissolved oxygen concentration in a body of water [47]

assumptions. In the context of dissolved oxygen in water, the van't Hoff equation can be used to estimate the change in solubility of oxygen as the temperature changes. The equation allows the calculation of a scaling factor that represents the relative change in solubility between two temperatures.

$$\ln\left(\frac{S_2}{S_1}\right) = \frac{\Delta H}{R} \left(\frac{1}{T_1} - \frac{1}{T_2} \right) \quad (2)$$

Where:

- S_1 is the solubility of oxygen at temperature T_1
- S_2 is the solubility of oxygen at temperature T_2
- ΔH is the heat of solution (usually a constant for a particular gas)
- R is the gas constant
- T_1 and T_2 are the respective temperatures in Kelvin

To scale the dissolved oxygen values from room temperature (T_1) to the desired temperature (T_2), a scaling factor can be calculated by isolating the solubility of oxygen at the two temperatures and multiplying it into the room temperature DO values in order to obtain the adjusted DO values for the desired temperature. The scaling factor can be calculated by isolating $\frac{S_2}{S_1}$ from equation 2 as seen in equation 3. Then plugged into equation 4, to obtain the final DO value.

$$\frac{S_2}{S_1} = e^{\left(\frac{\Delta H}{R}\right)\left(\frac{1}{T_1} - \frac{1}{T_2}\right)} \quad (3)$$

$$\text{Adjusted DO values} = \text{Room temperature DO values} \times \text{scaling factor} \quad (4)$$

7.2. Effects of Atmospheric Pressure on DO Measurements

Atmospheric Pressure can effect the concentration of dissolved oxygen in water. The calculation for the concentration after taking atmospheric pressure into account can be done by using Henry's law [49]. The dissolved oxygen concentration is proportional to the percent of oxygen in the air above it as can be seen in equation 5. Where C is the scaled

concentration of dissolved oxygen in water, k is Henry's law constant, and P is the percent of oxygen in the air above the water.

$$C = k \cdot P \quad (5)$$

There are two ways the scaling of the DO concentration value according to the atmospheric pressure can be accommodated for within the DOxy system: Either an additional atmospheric pressure sensor can be added to the DOxy SUs, or public API's of atmospheric pressure data can be used to perform the calculations within the dashboard's backend once the sensor readings have been received.

7.3. Sensor Enhancement

As the present research has shown, using purely the infrared data from the MAX30102 sensor, the dissolved oxygen content in water was accurately measured. Which is in line with, the findings of Miura et. al [14] which shows that the greatest variance in absorbance occurred in the blue and infrared light wavelengths in water. Wibowo et al. however, set up a fluorescence-quenching dissolved oxygen sensor, running it first with a red LED and then with a blue LED, finding that a blue light was more sensitive to dissolved oxygen levels [50]. Hence, for future implementation, research is being conducted on the effectiveness of the blue light for measuring dissolved oxygen in water both by itself, and in combination with data from infrared light. Based on those results, the sensor used in DOxy SUs may change or maybe even a completely new sensor is developed.

7.4. Actuation

Without loss of generality, it can be seen that a DOxy sensor can be used to control various environmental factors in an aquaculture setup. For instance, if the measured level of dissolved oxygen falls below a set certain level in a tank, the DOxy sensor readings could trigger the opening of oxygen valves or even the turning on of oxygen pumps that push more oxygen into the water until the DOxy readings show a restoration of the DO levels.

8. Conclusions

Measuring dissolved oxygen levels in water is achievable with use of none chemical based optical sensors. However, most current work in this area is academic and not market-ready. DOxy is a low-cost, accessible, and sustainable optical DO metering system which will transform the aquaculture industry in this respect. Given the importance of monitoring DO levels, an IoT solution such as DOxy has the potential to reduce labor and thus improve the efficiency and productivity of aquaculture via automation. A strong correlation between values produced by DOxy and values produced by a DO meter show the viability and accuracy of DOxy's approach at measuring DO in water. Furthermore, DOxy utilizes a web-based user-friendly dashboard to help users effectively visualize and analyze the data collected from sensors in the field. But most importantly, such aquacultural automation allows for early detection of changing water conditions and hence increases the quality of life for marine life as well as those who care for or whose livelihood depends on marine life.

Acknowledgments: Many thanks are due to the Frugal Innovation Hub (FIH) [51] and the department of Computer Science and Engineering (CSE) of the School of Engineering (SoE) at Santa Clara University (SCU) for their continued support of the DOxy project as well as the Ethical, Pragmatic, and Intelligent Computing (EPIC) research laboratory in general. And also to past team members and now SCU Alumni Jayati Patel, Tiana Nguyen, and Arianne Soriano for their ground breaking work on the early iterations of the project as reported on at the 2020 IEEE GHTC conference.

References

1. Environment and Natural Resources. Dissolved Oxygen (DO). https://www.enr.gov.nt.ca/sites/enr/files/dissolved_oxygen.pdf.

2. Richards, J.G. Chapter 10 Metabolic and Molecular Responses of Fish to Hypoxia. In *Hypoxia*; Richards, J.G.; Farrell, A.P.; Brauner, C.J., Eds.; Academic Press, 2009; Vol. 27, *Fish Physiology*, pp. 443–485. [https://doi.org/https://doi.org/10.1016/S1546-5098\(08\)00010-1](https://doi.org/https://doi.org/10.1016/S1546-5098(08)00010-1). 555
3. Abdel-Tawwab, M.; Monier, M.N.; Hoseinifar, S.H.; Faggio, C. Fish response to hypoxia stress: growth, physiological, and immunological biomarkers. *Fish physiology and biochemistry* **2019**, *45*, 997–1013. 558
4. Samaras, A.; Tsoukali, P.; Katsika, L.; Pavlidis, M.; Papadakis, I.E. Chronic impact of exposure to low dissolved oxygen on the physiology of *Dicentrarchus labrax* and *Sparus aurata* and its effects on the acute stress response. *Aquaculture* **2023**, *562*, 738830. <https://doi.org/https://doi.org/10.1016/j.aquaculture.2022.738830>. 560
5. Solstorm, D.; Oldham, T.; Solstorm, F.; Klebert, P.; Stien, L.H.; Vågseth, T.; Oppedal, F. Dissolved oxygen variability in a commercial sea-cage exposes farmed Atlantic salmon to growth limiting conditions. *Aquaculture* **2018**, *486*, 122–129. <https://doi.org/https://doi.org/10.1016/j.aquaculture.2017.12.008>. 563
6. Hargreaves, J.A.; Tucker, C.S. Measuring Dissolved Oxygen Concentration in Aquaculture. <http://agrilife.org/fisheries/files/2013/09/SRAC-Publication-No.-4601-T1\textendash-Measuring-Dissolved-Oxygen-Concentration-in-Aquaculture.pdf>, 2002. 566
7. Shaghghi, N.; Nguyen, T.; Patel, J.; Soriano, A.; Mayer, J. DOxy: Dissolved Oxygen Monitoring. In Proceedings of the 2020 IEEE Global Humanitarian Technology Conference (GHTC). IEEE, 2020, pp. 1–4. 568
8. Fondriest Environmental, Inc.. Measuring Dissolved Oxygen. <https://www.fondriest.com/environmental-measurements/measurements/measuring-water-quality/dissolved-oxygen-sensors-and-methods>, 2014. 570
9. Trivellin, N.; Barbisan, D.; Badocco, D.; Pastore, P.; Meneghesso, G.; Meneghini, M.; Zanoni, E.; Belgioioso, G.; Cenedese, A. Study and Development of a Fluorescence Based Sensor System for Monitoring Oxygen in Wine Production: The WOW Project. *Sensors* **2018**, *18*. <https://doi.org/10.3390/s18041130>. 572
10. Suresh, S.; Srivastava, V.C.; Mishra, I. Techniques for oxygen transfer measurement in bioreactors: a review. *Journal of Chemical Technology & Biotechnology: International Research in Process, Environmental & Clean Technology* **2009**, *84*, 1091–1103. 575
11. Algae Lab System. Optical Vs. Electrochemical Dissolved Oxygen Sensors. <http://algaelabsystems.com/optical-vs-electrochemical-dissolved-oxygen-sensors>. 577
12. Zhao, Y.; Zhang, H.; Jin, Q.; Jia, D.; Liu, T. Ratiometric Optical Fiber Dissolved Oxygen Sensor Based on Fluorescence Quenching Principle. *Sensors* **2022**, *22*. <https://doi.org/10.3390/s22134811>. 579
13. Yu, Y.; Kwon, M.S.; Jung, J.; Zeng, Y.; Kim, M.; Chung, K.; Gierschner, J.; Youk, J.H.; Borisov, S.M.; Kim, J. Room-Temperature-Phosphorescence-Based Dissolved Oxygen Detection by Core-Shell Polymer Nanoparticles Containing Metal-Free Organic Phosphors. *Angewandte Chemie International Edition* **2017**, *56*, 16207–16211. 581
14. Silveira Miura, A.; Parra Boronat, M.; Lloret, J.; Rodilla, M. LED optical sensor prototype to determine dissolved oxygen saturation in water. In Proceedings of the 2021 Global Congress on Electrical Engineering (GC-ElecEng 2021). Mosharaka for Research and Studies, 2021, Vol. 2. 584
15. Zhang, Y.; Zhang, Y.; Yuan, D.; Zhang, Y.; Wu, B.; Feng, X. Calibration method of multi-parameter compensation for optical dissolved oxygen sensor in seawater based on machine learning algorithm. *Deep Sea Research Part I: Oceanographic Research Papers* **2022**, *188*, 103856. <https://doi.org/https://doi.org/10.1016/j.dsr.2022.103856>. 587
16. Silva, E.B.; Pinto, P.V.F.; Chretien, J.B.; ao Isaac Silva Miranda, J.; Pinho, H.A.; Átila Pereira Timbó; Fraga, W.B.; Menezes, J.W.M.; Silva, M.E.R.; de Freitas Guimarães, G. Green optical dissolved oxygen sensor based on a chlorophyll–zinc complex extracted from the plant *Brassica oleracea* L. *Appl. Opt.* **2017**, *56*, 9951–9956. <https://doi.org/10.1364/AO.56.009951>. 590
17. Michelucci, U.; Baumgartner, M.; Venturini, F. Optical Oxygen Sensing with Artificial Intelligence. *Sensors* **2019**, *19*. <https://doi.org/10.3390/s19040777>. 593
18. Yunfeng, L.; Tianpei, Z. A Design of Dissolved Oxygen Monitoring System Based on Nb-Iot. In Proceedings of the 2019 International Conference on Smart Grid and Electrical Automation (ICSGEA), 2019, pp. 98–101. <https://doi.org/10.1109/ICSGEA.2019.00030>. 595
19. Stine, J.M.; Beardslee, L.A.; Sathyam, R.M.; Bentley, W.E.; Ghodssi, R. Electrochemical Dissolved Oxygen Sensor-Integrated Platform for Wireless In Situ Bioprocess Monitoring. *Sensors and Actuators B: Chemical* **2020**, *320*, 128381. <https://doi.org/https://doi.org/10.1016/j.snb.2020.128381>. 599
20. Hu, X.; Hu, Y.; Yu, X. The Soft Measure Model of Dissolved Oxygen Based on RBF Network in Ponds. In Proceedings of the 2011 Fourth International Conference on Information and Computing, 2011, pp. 38–41. <https://doi.org/10.1109/ICIC.2011.134>. 601
21. Cole-Palmer. Dissolved Oxygen Meters. www.colepalmer.com/c/dissolved-oxygen-meters, 2020. 603
22. Hanna Instruments. Measuring Dissolved Oxygen Concentration in Aquaculture. <https://www.hannainst.com/hi9142-portable-dissolved-oxygen-meter.html>, 2020. 604
23. Maxim Integrated. MAX30102, High-Sensitivity Pulse Oximeter and Heart-Rate Sensor. <https://www.maximintegrated.com/en/products/interface/sensor-interface/MAX30102.html>, 2017. 606
24. Milwaukee. Milwaukee MW600 Dissolved Oxygen Meter. <https://milwaukeeinstruments.com/pro-do-meter>. 608
25. Zlazzr.com. THIN 5/8"x1/32" Clear CIRCLE Acrylic Plastic Plexiglass Geometric Craft. <https://shop.zlazzr.com/collections/acrylic-circles-0-holes-2/products/thin-5-8x1-32-clear-circle-acrylic-plastic-plexiglass-geometric-craft>. 609
26. Shaghghi, N.; Kniveton, N.; Mayer, J.; Tuttle, W.; Ferguson, P. SU 2.0: A Marketable Low-Power Wireless Sensing Unit for Hydration Automation. In Proceedings of the AMBIENT 2020, The Tenth International Conference on Ambient Computing, Applications, Services and Technologies (IARIA Ambient), 2020, pp. 33–39. 611

27. Wisen. Whisper Node - AVR LoRa. <https://wisen.com.au/store/products/whisper-node-avr>, 2018. 614
28. Semtech(2015)(@)(@)Lora Semtech. SX1276/77/78/79 - 137 MHz to 1020 MHz Low Power Long Range Transceiver. https://cdn-shop.adafruit.com/product-files/3179/sx1276_77_78_79.pdf, 2015. 615
29. Semtech. SX1276 Transceiver. https://www.semtech.com/uploads/documents/DS_SX1276-7-8-9_W_APP_V5.pdf, 2018. 616
30. Wisen Labs. Magnetic Omni-directional Antenna - 3dBi. <https://wisen.com.au/store/products/magnetic-omni-directional-antenna-3dbi/>, 2023. 617
31. Components101. DHT11-Temperature and Humidity Sensor. <https://components101.com/dht11-temperature-sensor>, 2020. 618
32. ASIC, N.T.P. TP4056 1A Standalone Linear Li-Ion Battery Charger with Thermal Regulation in SOP-8. <http://www.tp4056.com/d/tp4056.pdf>, 2020. 619
33. HiLetgo. HiLetgo Micro SD card reader module. <http://www.hiletgo.com/ProductDetail/2158021.html>, 2018. 620
34. Arduino. Arduino Nano. <https://docs.arduino.cc/static/12f5bdbb504fa7bf4901483241e92936/A000005-datasheet.pdf>, 2023. 621
35. 3D, A.T. PET Filament: Waterproof and Food-Safe Material Plastic for 3D Printing. <https://www.allthat3d.com/pet-filament>, 2019. 622
36. Prusa Research. TECHNICAL DATA SHEET Prusament PETG by Prusa Polymers, 2019. 623
37. Kuhn, B. Important Advantages of PETG Filament in 3D Printing, 2016. 624
38. Shaghaghi, N.; Mayer, J. A sustainable 3D-printed casing for hydro-system automation sensing units. In Proceedings of the 2019 IEEE Global Humanitarian Technology Conference (GHTC). IEEE, 2019, pp. 1–7. 625
39. Espressif Systems. ESPRESSIF SMART CONNECTIVITY PLATFORM: ESP8266. https://nurdspace.nl/images/e/e0/ESP8266_Specifications_English.pdf, 2013. 626
40. Shaghaghi, N.; Cameron, Z.; Kniveton, N.; Mayer, J.; Tuttle, W.; Ferguson, P. ÂB: An Energy Aware Communications Protocol (EACP) for the Internet of Things (IoT). In Proceedings of the Workshops of the International Conference on Advanced Information Networking and Applications. Springer, 2020, pp. 877–889. 627
41. Shaghaghi, N.; Ferguson, P.; Mayer, J.; Cameron, Z.; Dezfouli, B. A Low-power Wireless Sensing Unit for Hydro-System Automation. In Proceedings of the 2019 IEEE 9th Annual Computing and Communication Workshop and Conference (CCWC). IEEE, 2019, pp. 0659–0665. 628
42. Thamrin, N.; Liyana, N.; bin Misnan, F.; Shaghaghi, N. Long-Range Data Transmission for Online Water Quality Monitoring of the Tembling River in Rural Areas of Pahang, Malaysia. In Proceedings of the AMBIENT 2020, The Tenth International Conference on Ambient Computing, Applications, Services and Technologies (IARIA Ambient), 2020, pp. 28–32. 629
43. Ali, M.S.A.M.; Thamrin, N.M.; Misnan, M.F.; Ibrahim, N.N.N.; Shaghaghi, N. Sustainable surface water dissolved oxygen monitoring at lake 7/1F, Shah Alam, Selangor. *Journal of Mechanical Engineering (JMecE)* **2021**, *18*, 13–26. 630
44. Docker Inc.. Docker Docs. <https://docs.docker.com/>, 2023. 631
45. Timescale, I. Timescale Documentation. <https://docs.timescale.com>, 2023. 632
46. Svelte Core Team. Svelte Documentation. <https://svelte.dev/docs>, 2019. 633
47. U.S. Department of the Interior. Dissolved Oxygen and Water. <https://www.usgs.gov/special-topics/water-science-school/science/dissolved-oxygen-and-water>, 2018. 634
48. van't Hoff, J.H. *Etudes de dynamique chimique*; Frederik Muller & Co, 1884. 635
49. Fondriest Environmental, Inc.. Dissolved Oxygen. <https://www.fondriest.com/environmental-measurements/parameters/water-quality/dissolved-oxygen>, 2023. 636
50. Wibowo, M.; Puspita, I.; Hatta, A.; Sekartedjo, S. Wavelength Effect on Graphene Oxide-Coated Plastic Optical Fiber for Dissolved Oxygen Sensor. In Proceedings of the 2019 International Conference on Advanced Mechatronics, Intelligent Manufacture and Industrial Automation (ICAMIMIA), 2019, pp. 151–154. <https://doi.org/10.1109/ICAMIMIA47173.2019.9223349>. 637
51. Santa Clara University. Frugal Innovation Hub (FIH). <https://www.scu.edu/engineering/labs--research/labs/frugal-innovation-hub>, 2020. 638