Trigger Fine Time Analysis

- Fine time bins (phase) span from 0 to 10 ns. Bin size are not even. Therefore, need calibration to go from phase to time.

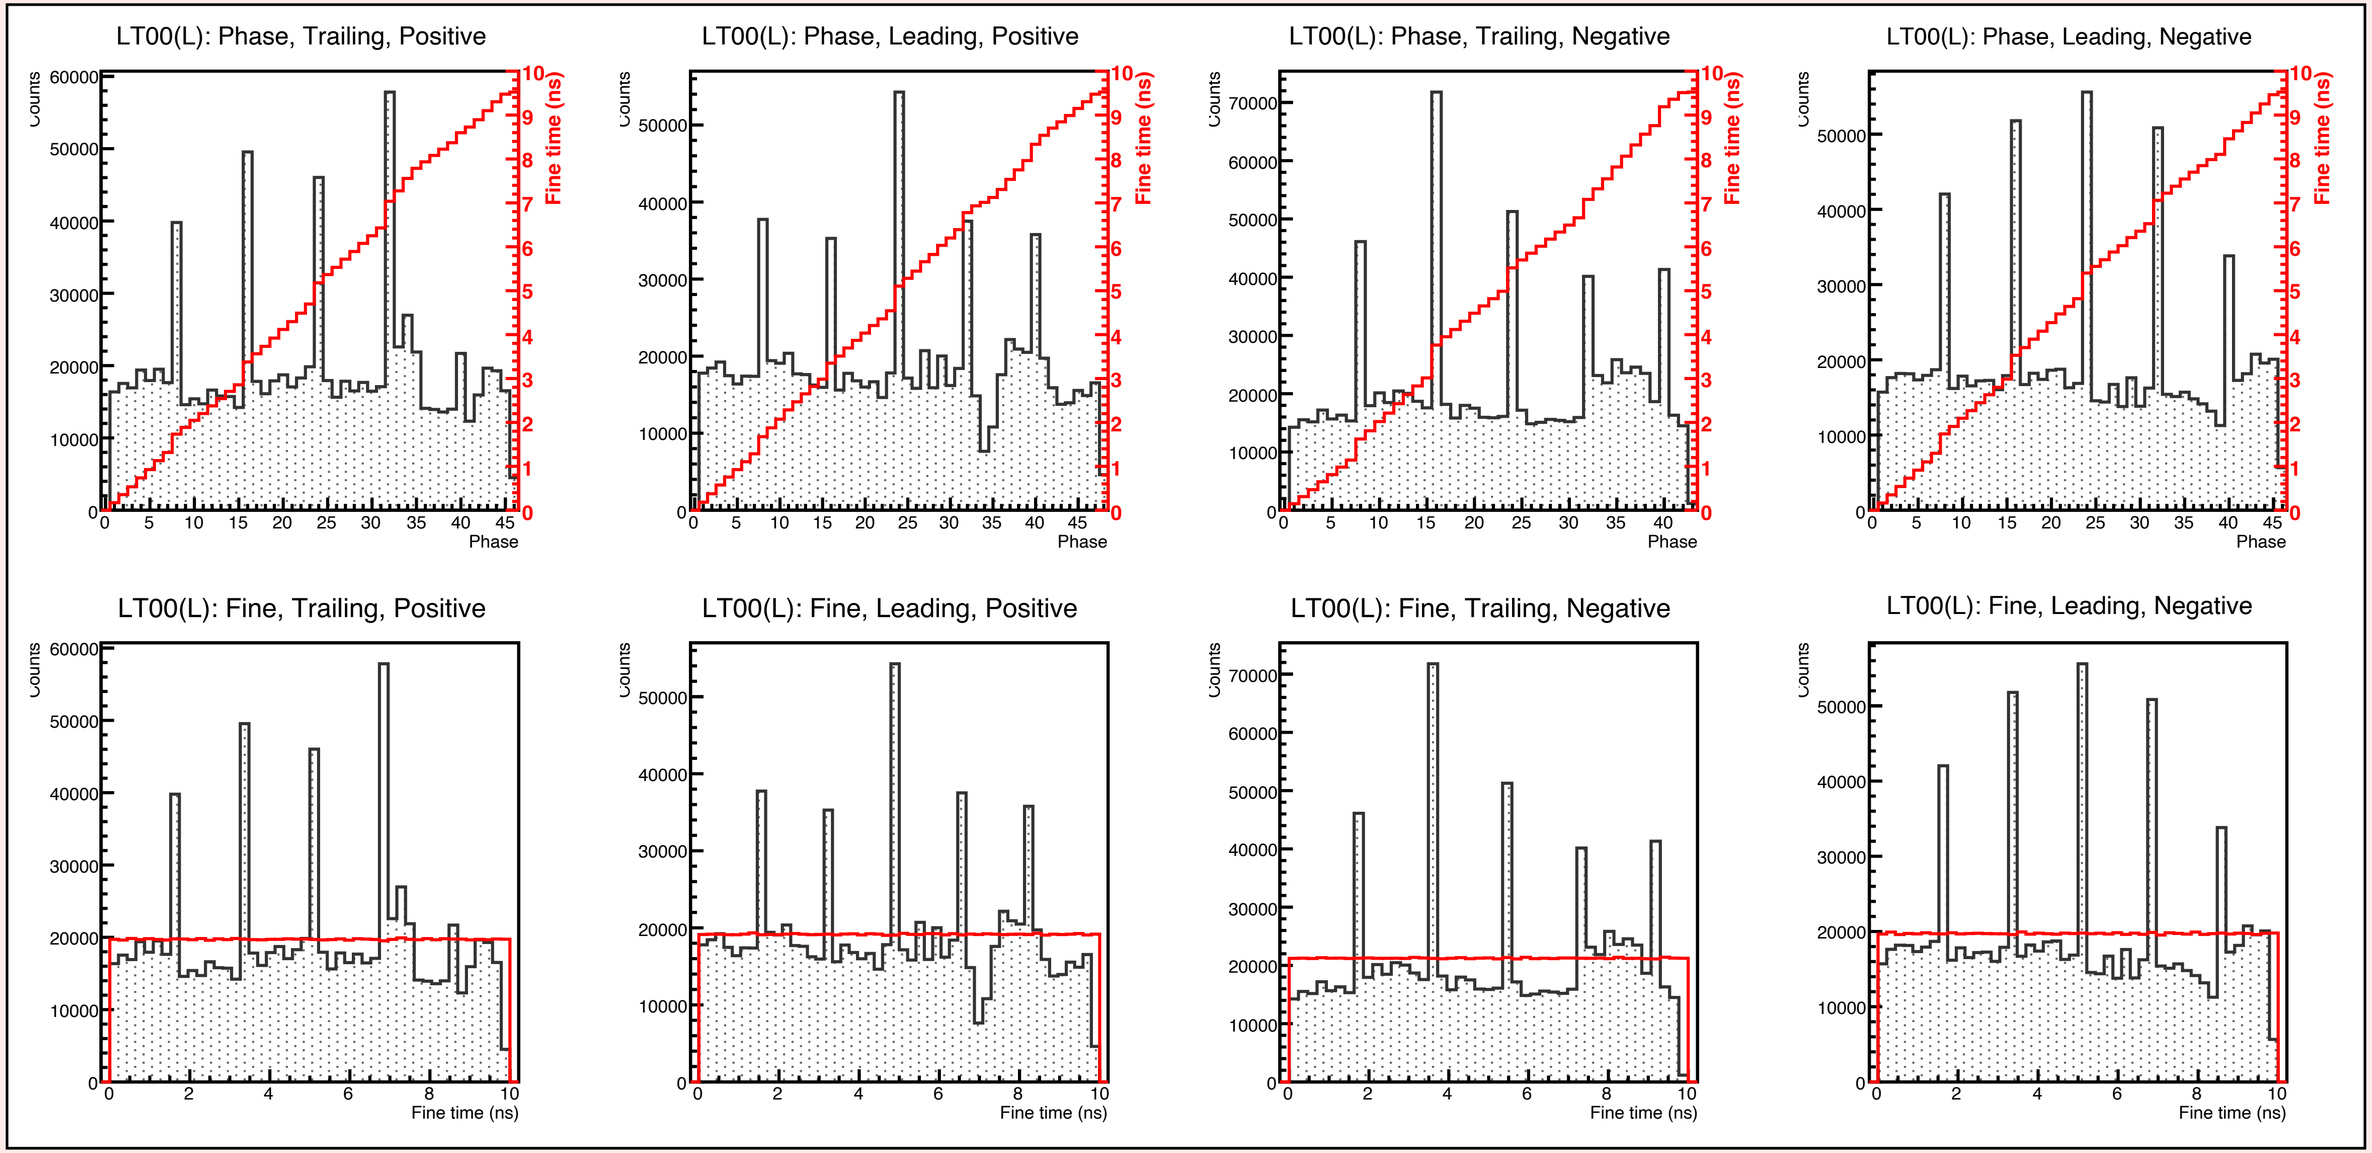

Trigger Fine Time Analysis

- Added new recipe: trs_online.xml. This loads the calibration .json file and skips the calibration process
- Original recipe: trs.xml. This perform fine time calibration during the first process loop

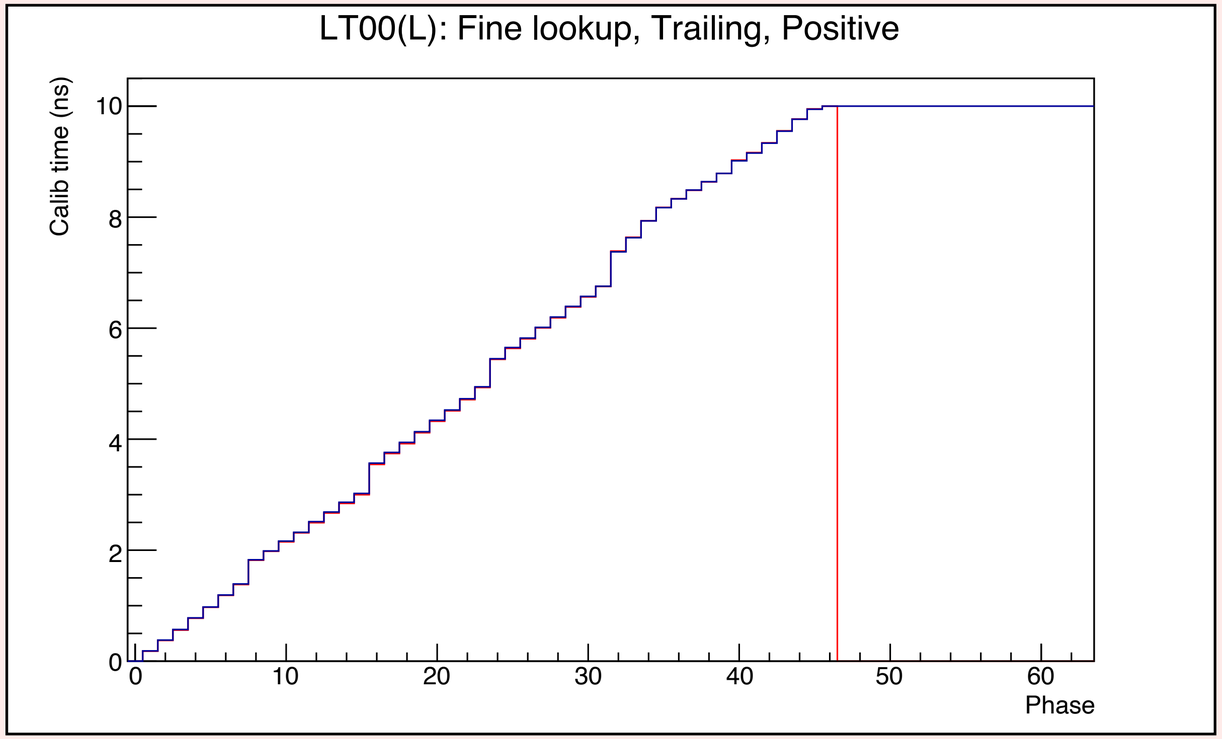

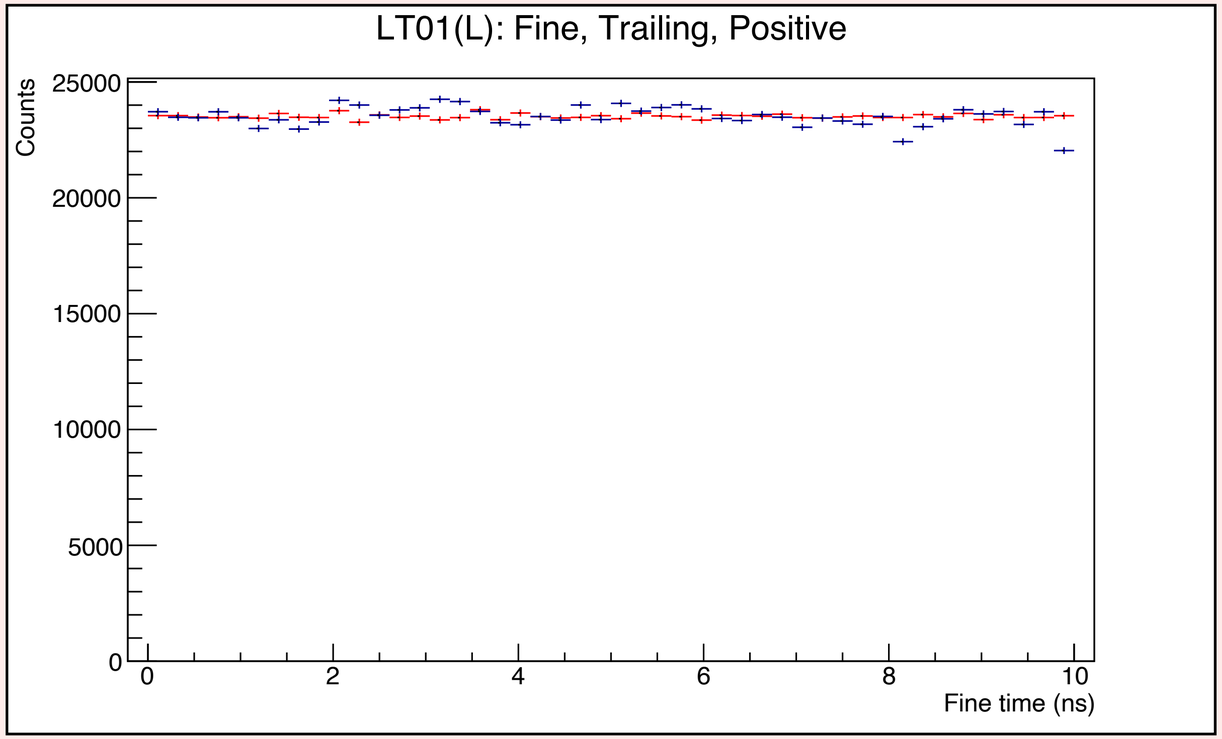

- trs.xml
- trs_online.xml

Trigger Fine Time Analysis

- 10 ns time structure from both recipes ..

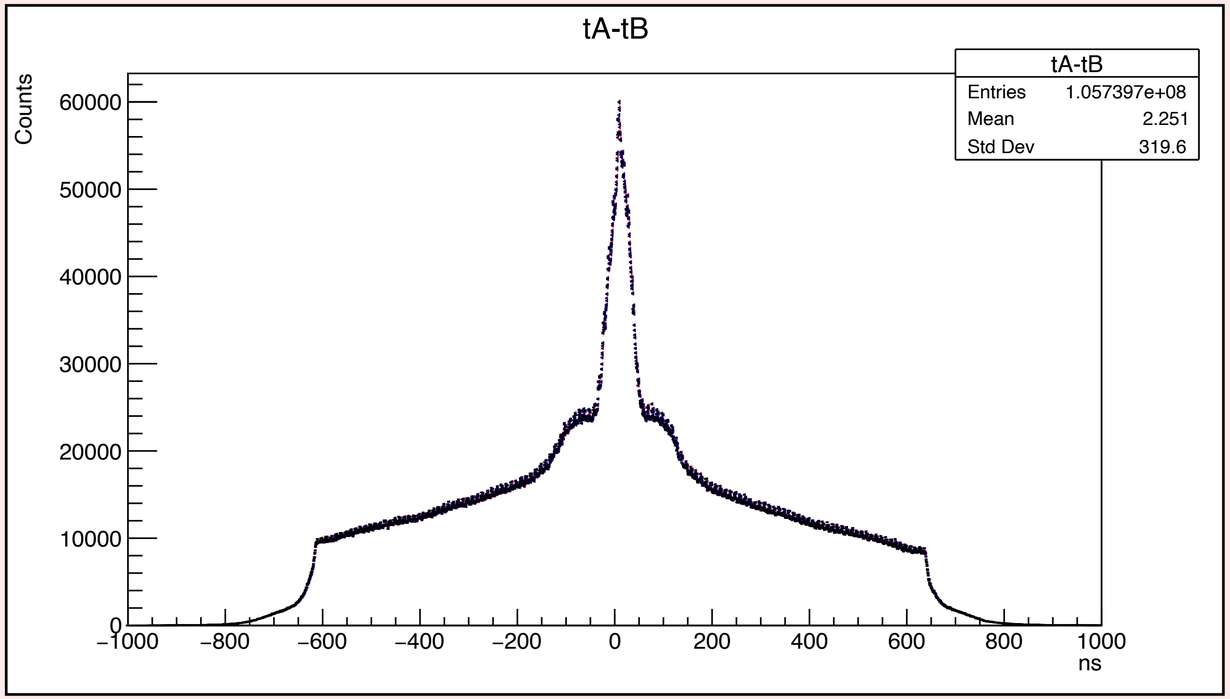

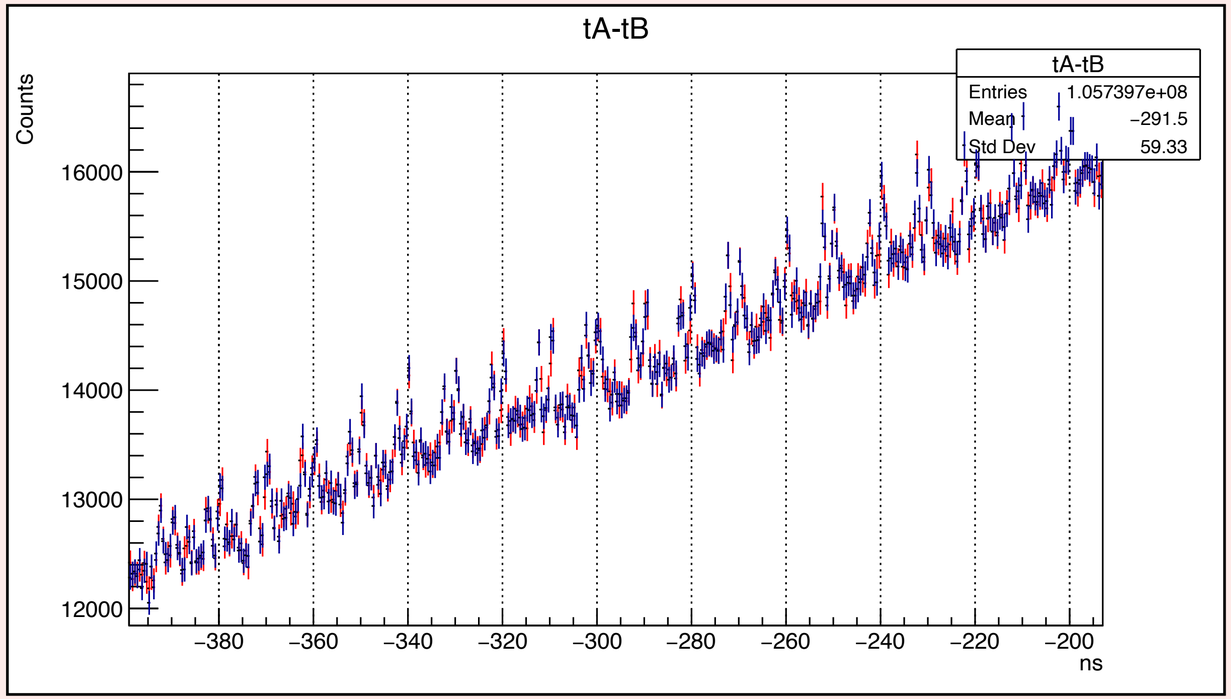

- trs.xml
- trs_online.xml

Trigger Fine Time Analysis

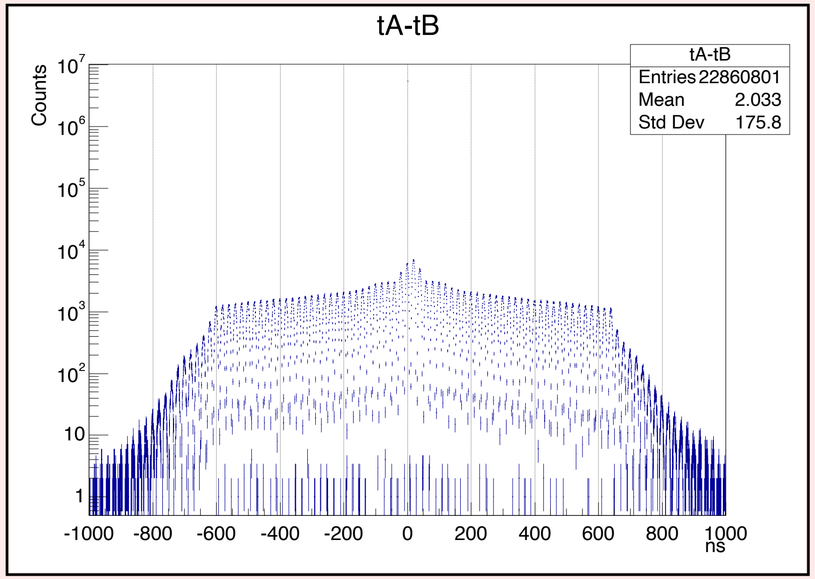

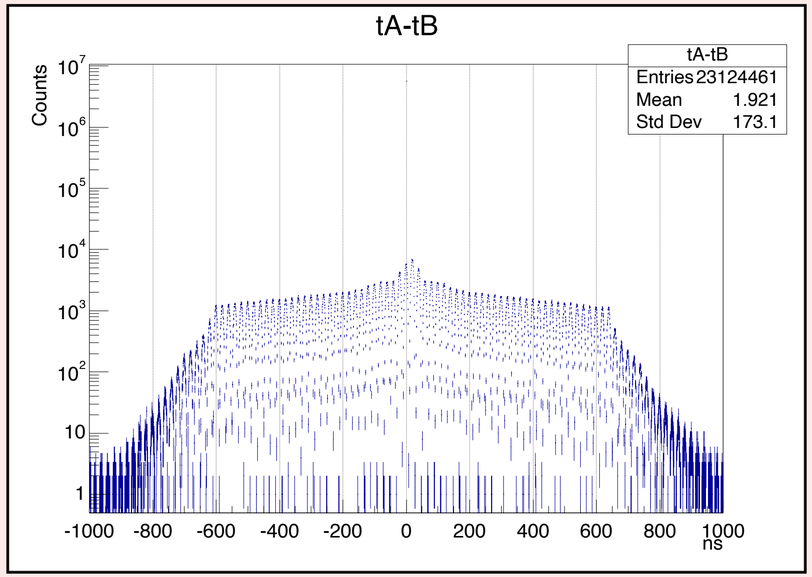

Phase 0 only

Phase 1 only

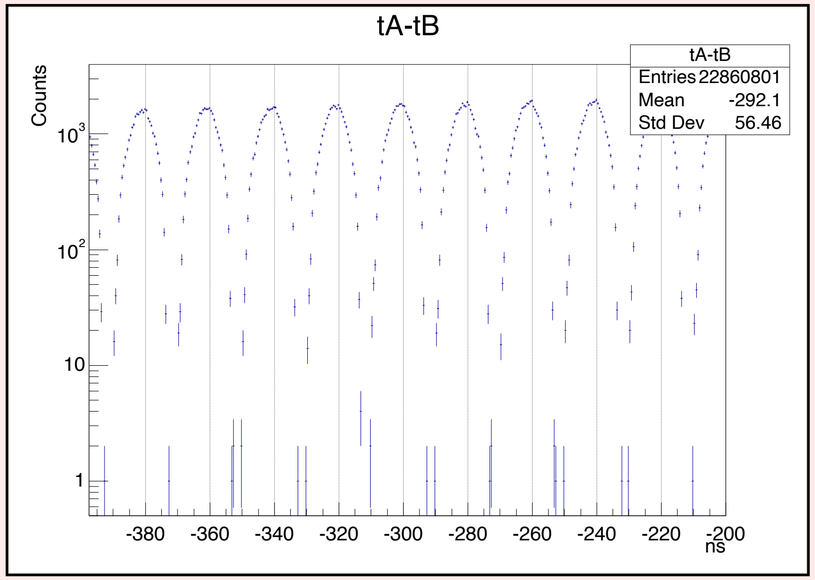

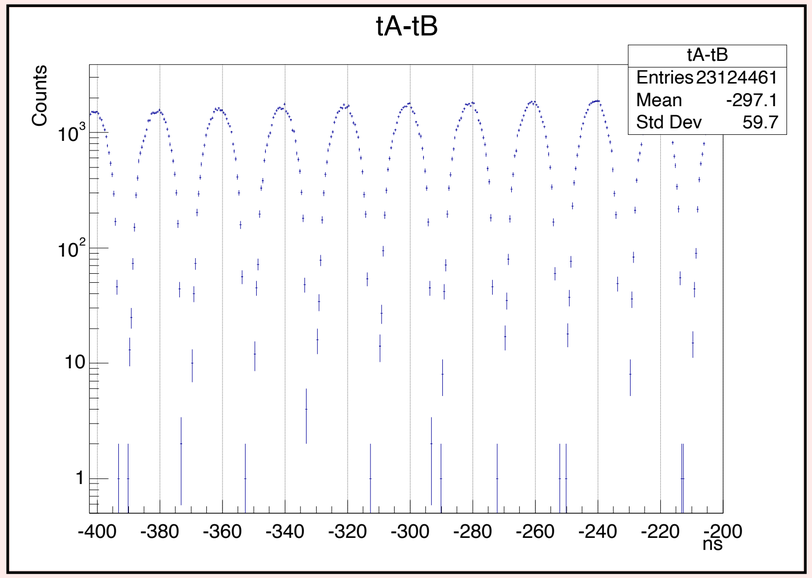

Reconstruction resolution with and without multiple scattering

Resolution of p, Θ, Φ with msc

	e^- spectrometer	e^+ spectrometer
p	76 keV	39 keV
Θ	0.486 deg	0.261 deg
Φ	2.472 deg	1.896 deg

Resolution of p, Θ, Φ without multiple scattering(msc) on focal planes

	e^- spectrometer	e^+ spectrometer
p	26 keV	36 keV
Θ	0.033 deg	0.032 deg
Φ	0.014 deg	0.014 deg