

# 12 Lead ECG Report

Date: 21 Feb 2026, 03:49 pm



|      |            |        |        |        |                  |
|------|------------|--------|--------|--------|------------------|
| NAME | AGE        | GENDER | HEIGHT | WEIGHT | REPORT ID        |
| Amit | 21 year(s) | Male   | 183 cm | 85 kg  | 1771669199672820 |

## ECG Parameters AI POWERED

| Parameter    | Observed Values | Standard Range   |
|--------------|-----------------|------------------|
| PR Interval  | 116 ms          | 100 ms - 200 ms  |
| QRS Interval | 87 ms           | 60 ms - 120 ms   |
| QT Interval  | 356 ms          | 300 ms - 450 ms  |
| QTc Interval | 401 ms          | 300 ms - 450 ms  |
| Heart Rate   | 76 bpm          | 60 bpm - 100 bpm |

## Result Details AI POWERED

Overall evaluation of test  
Abnormal ECG

Interpretation Details  
Borderline

Anomalies in test reports  
ST elevation in v4 (0.39mV),

Suggested Action  
If symptoms like chest pain, palpitations, shortness of breath and dizziness is felt,Intake a tablet of Aspirin 150mg and consult your physician.If ECG is abnormal without symptoms, closely monitor your ECG in every three hours,If abnormality persists, consult your physician.Recommended Evaluation Test,Echocardiogram/Exercise ECG.

## Risk Meter



This is a computer-generated ECG interpretation. Clinical validation by a licensed healthcare professional is required.

Disclaimer: NOT FOR COMMERCIAL USE | Medical advice asked and accepted on the internet (without physically examining the patient) is at patient's own risk. Visit a doctor in case of emergency.


# 12 Lead ECG Report

Date: 21 Feb 2026, 03:49 pm



| NAME | AGE        | GENDER | HEIGHT | WEIGHT | REPORT ID        |
|------|------------|--------|--------|--------|------------------|
| Amit | 21 year(s) | Male   | 183 cm | 85 kg  | 1771669199672820 |

Heart rate: 76 bpm

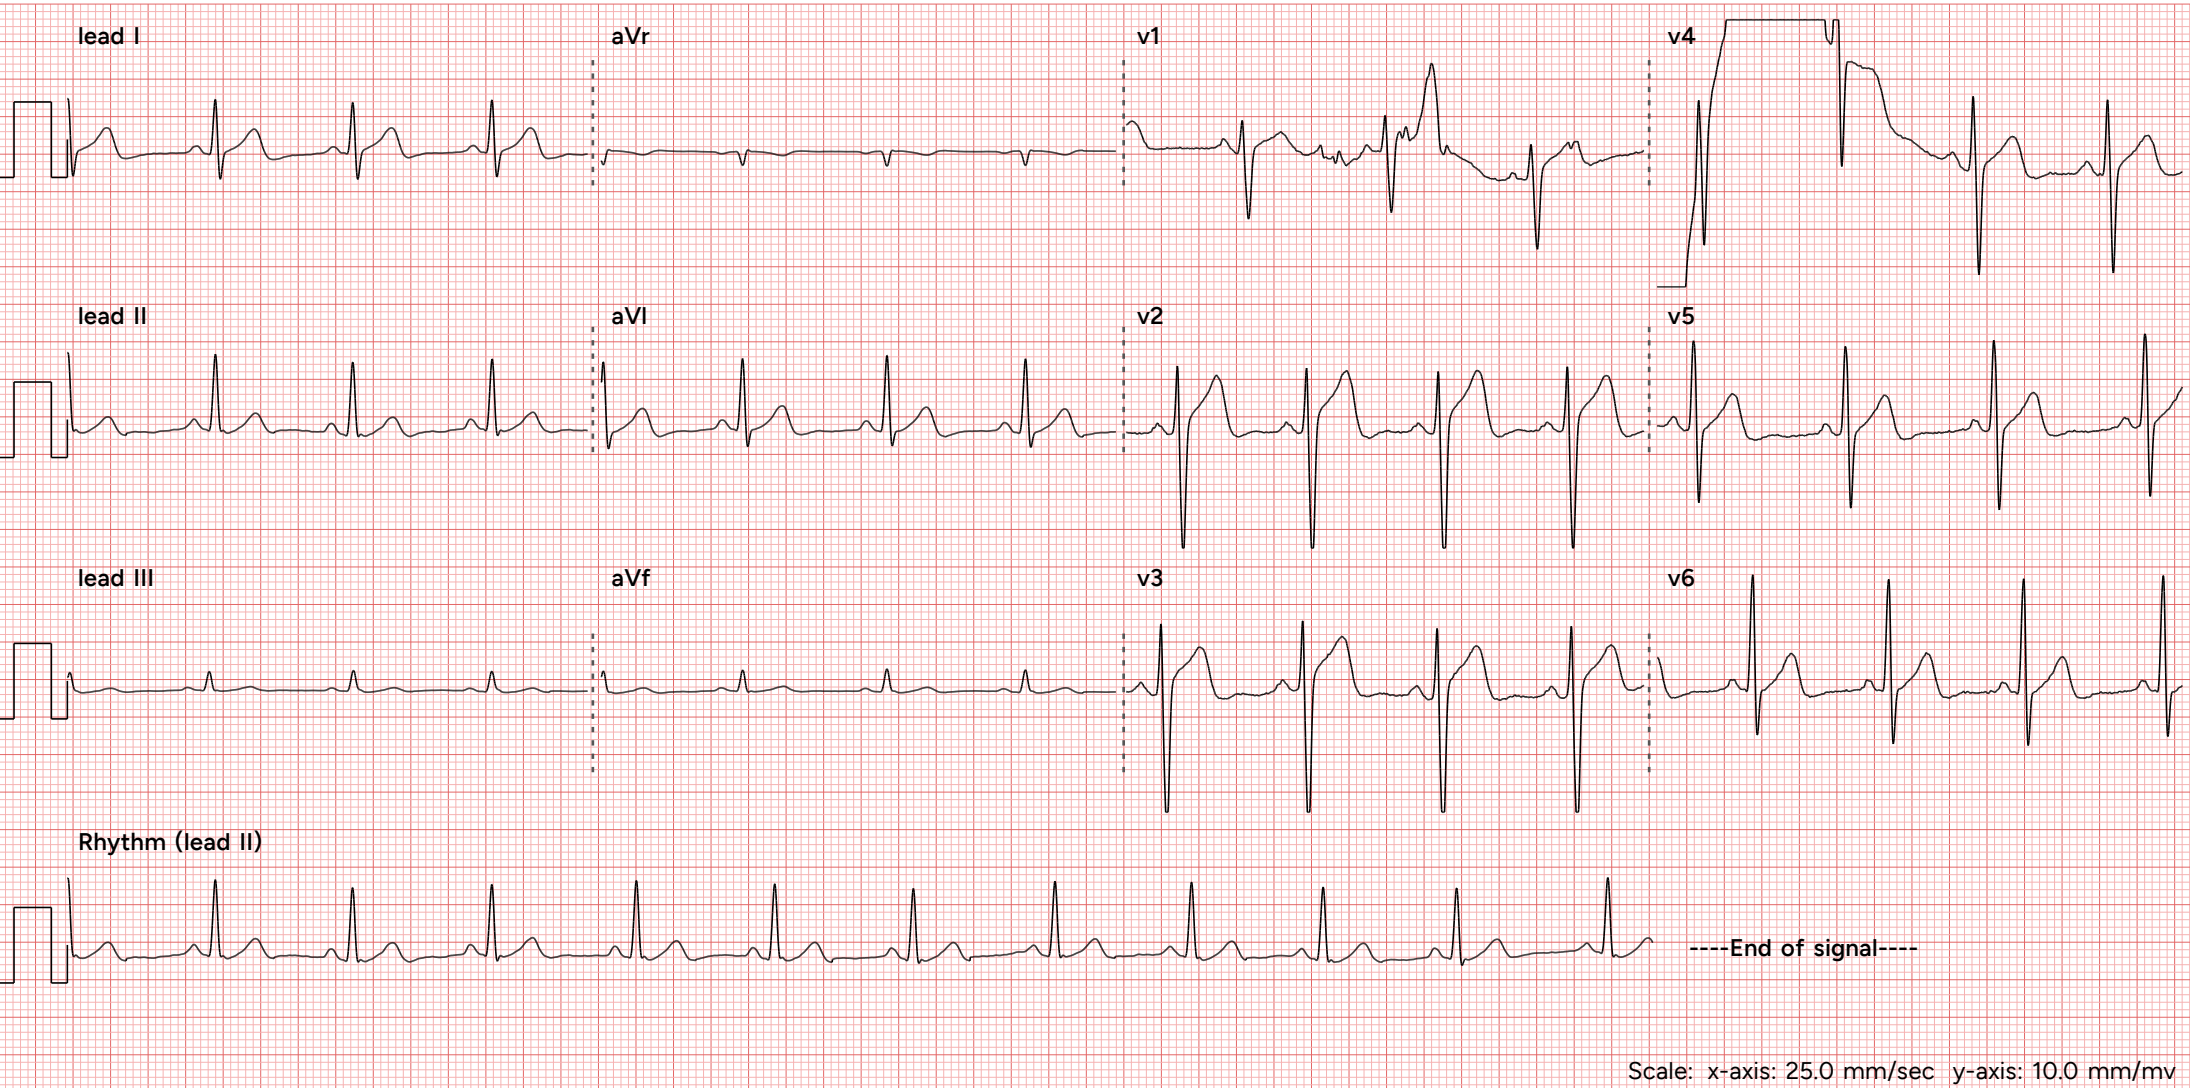

Note: This report is generated using **Spandan portable ECG device**. To know more about Spandan visit [www.sunfox.in/spandan](http://www.sunfox.in/spandan) or call at **(+91)7060000556**

Page: 2 of 2

Device Variant: **Spandan Pro**

Report Version: **1.0.18**

Source: **Spandan App v4.10.1**

ECG Processor Version: **2.0.40-beta6** Firmware Version: **001.03**

Device ID: **SPPR-DN01-2511260248**