CMS Preliminary Phase 2

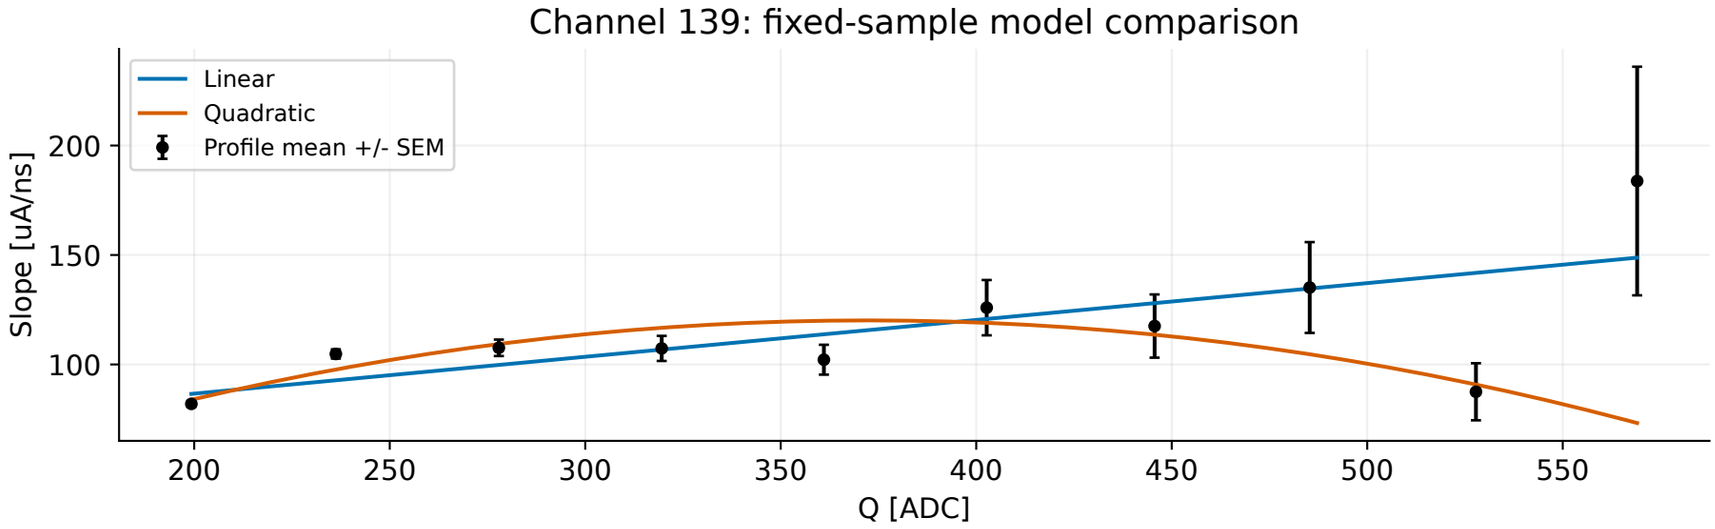

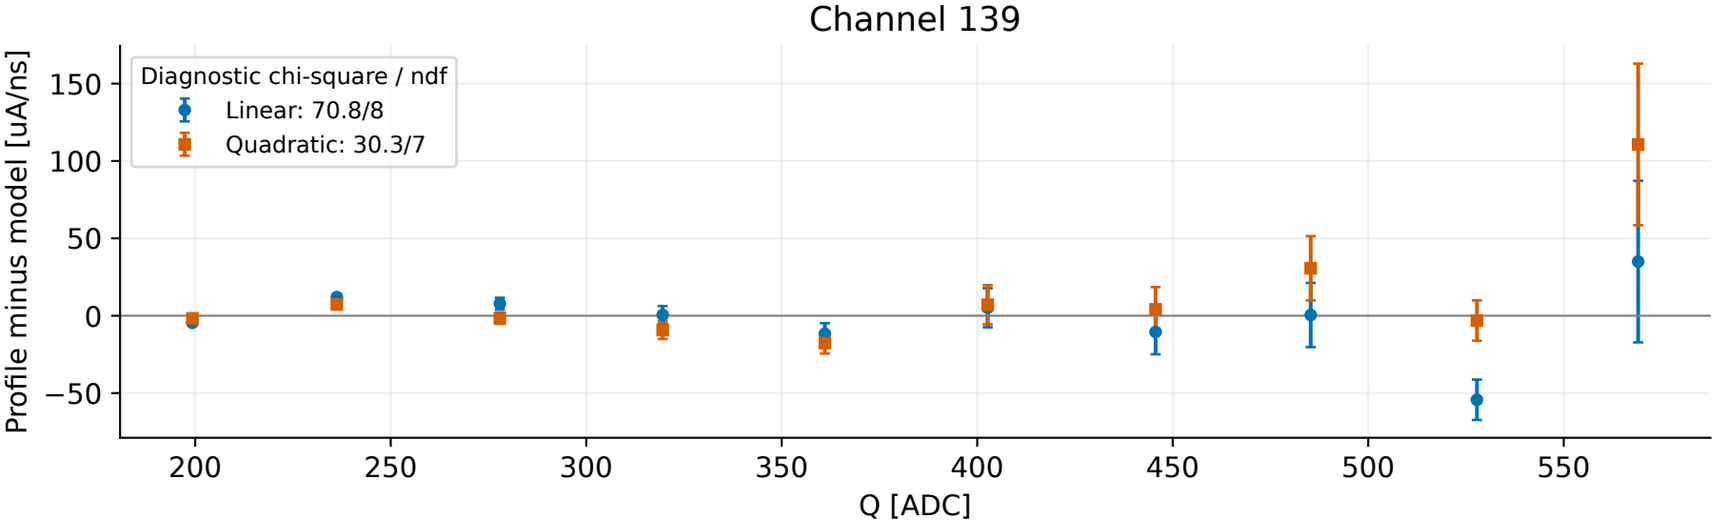

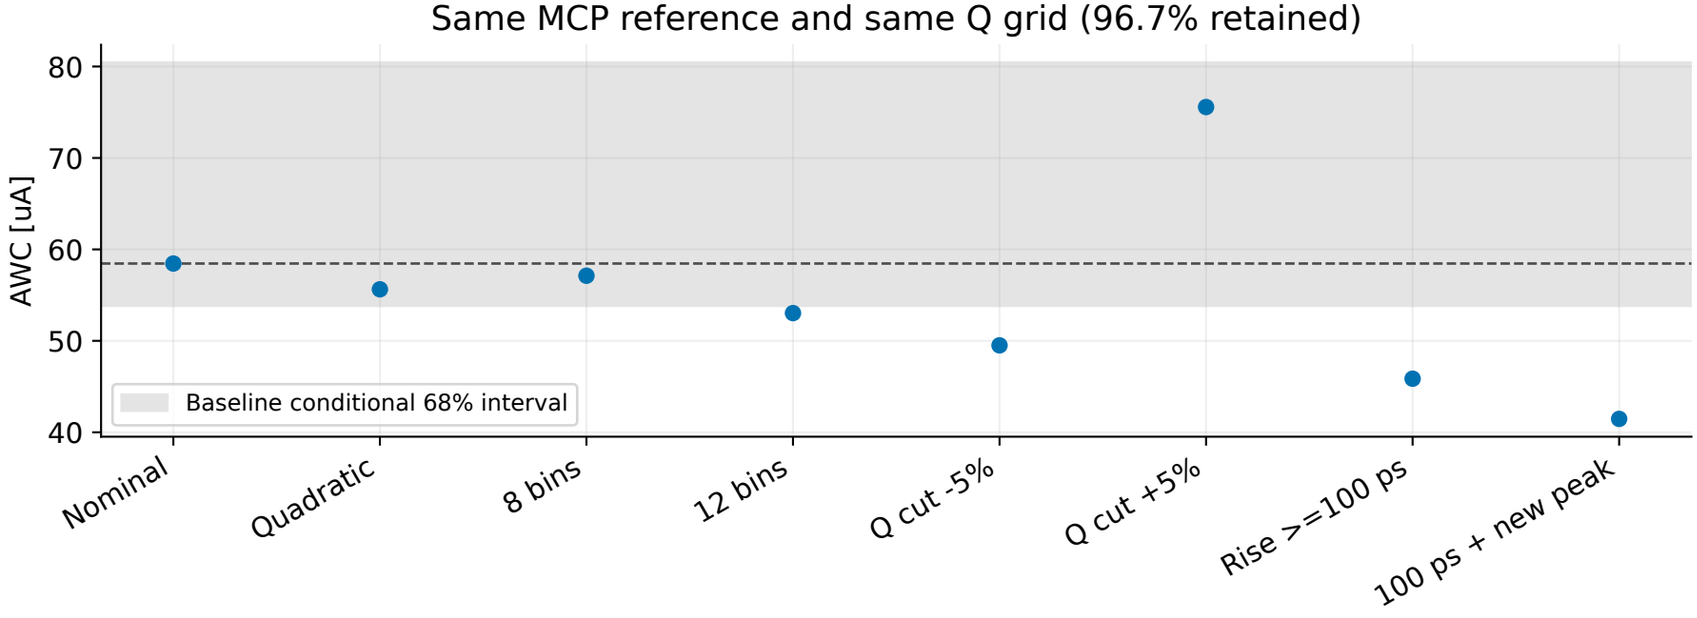

Sensitivity study only: no nominal calibration replaced. SEM errors condition on the reconstructed sample.