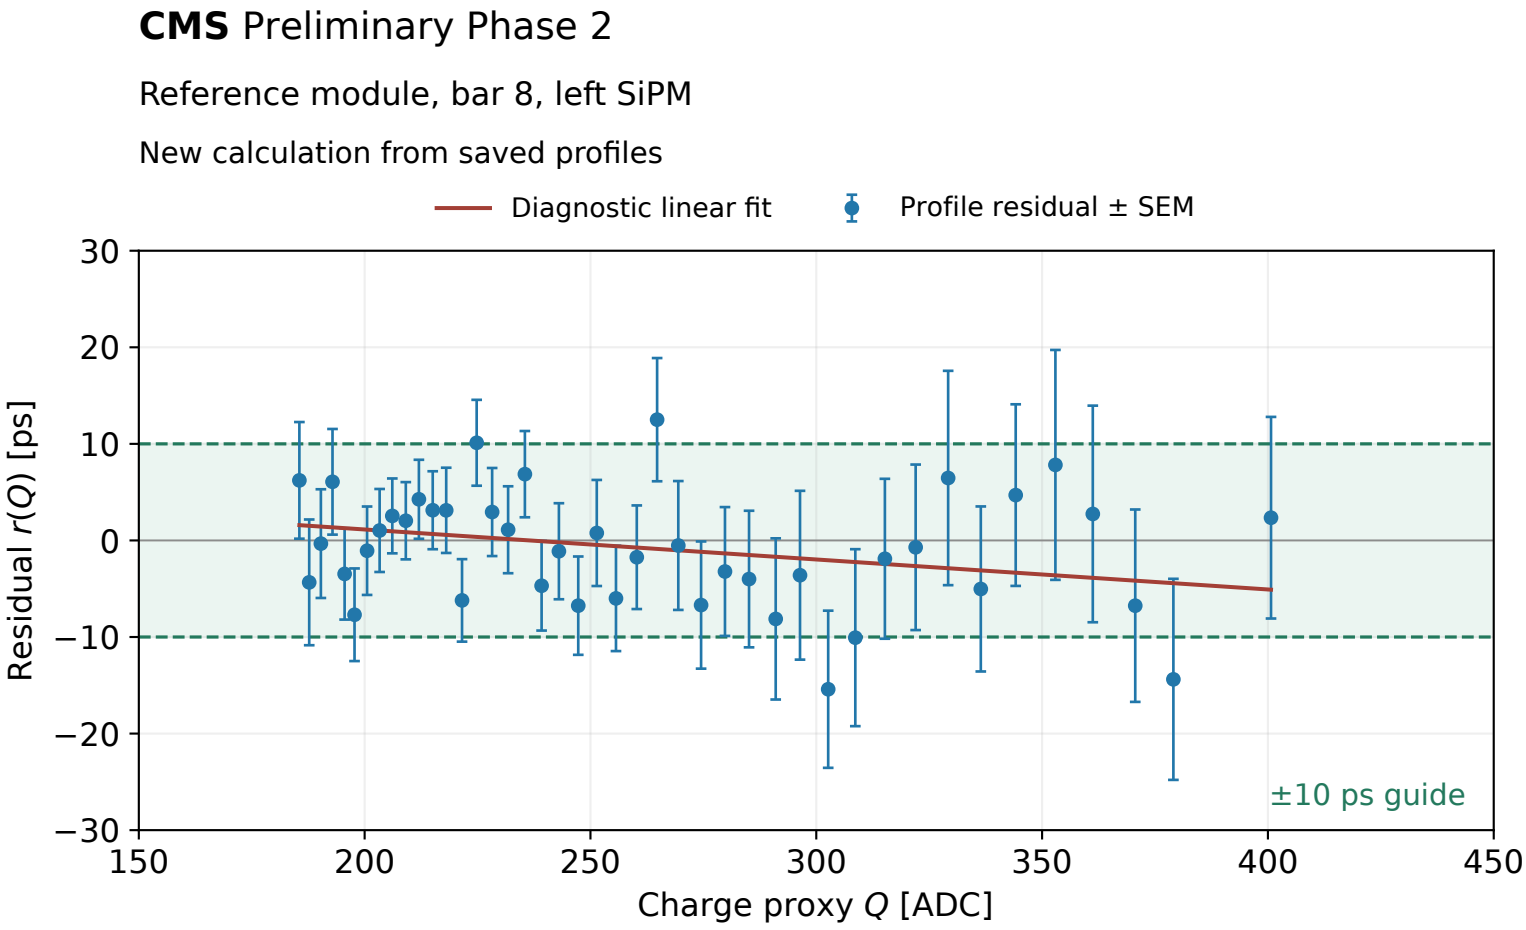
CMS Preliminary Phase 2
Reference module, bar 8, left SiPM
New calculation from saved profiles
Diagnostic linear fit
Profile residual ± SEM
Residual r(Q) [ps]
Charge proxy Q [ADC]
±10 ps guide
30
20
10
0
−10
−20
−30
150
200
250
300
350
400
450