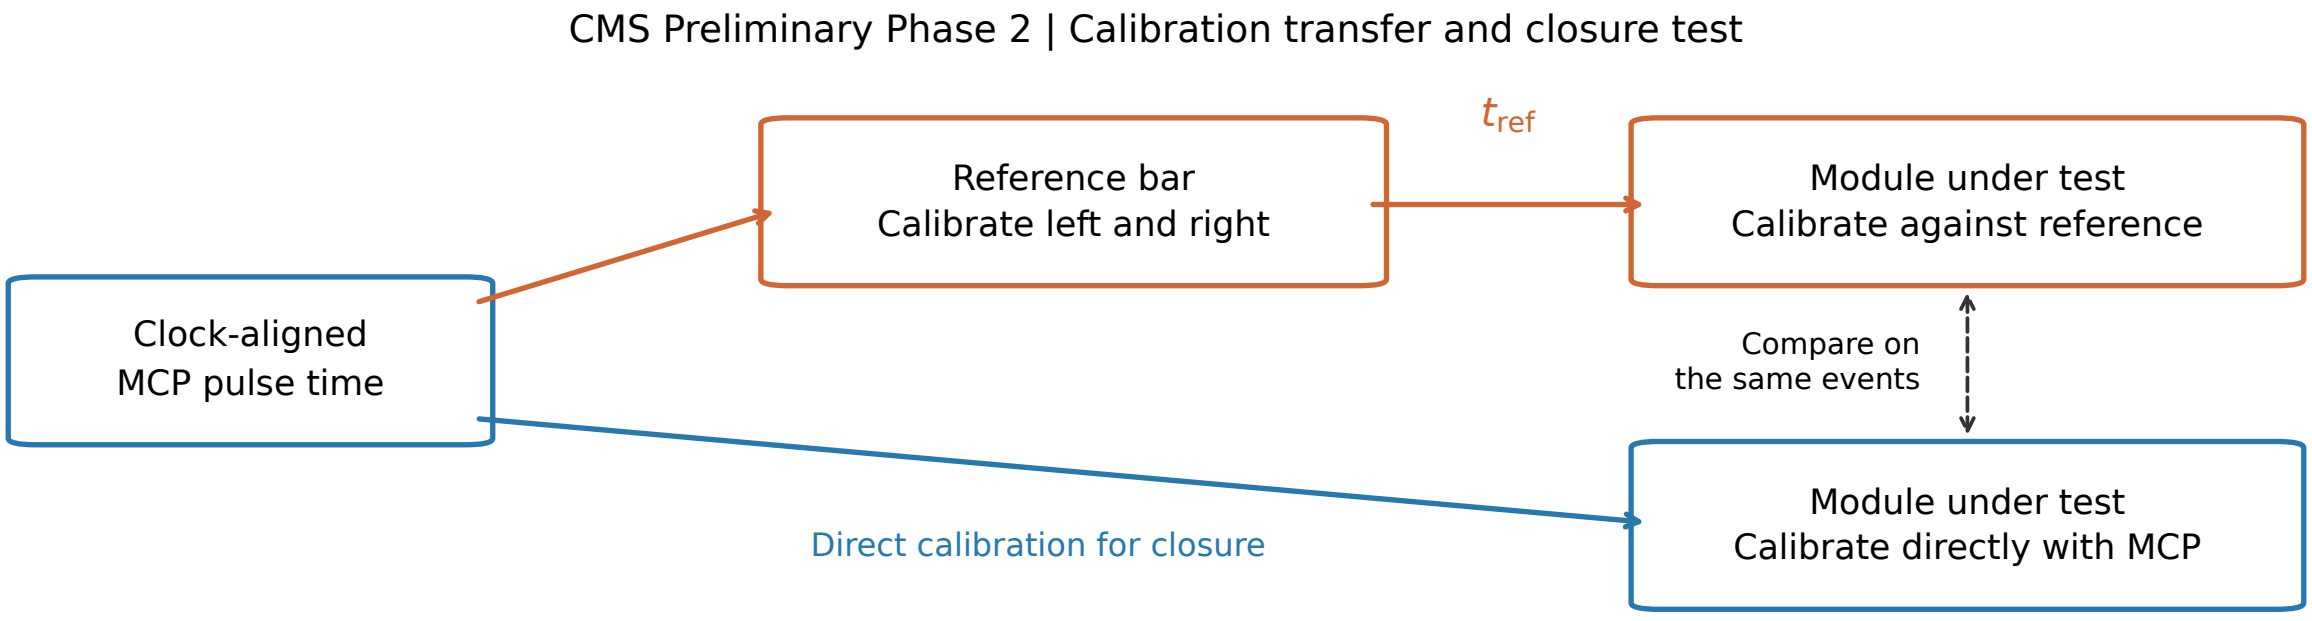
CMS Preliminary Phase 2 | Calibration transfer and closure test
Reference bar
Calibrate left and right
t_{ref}
Module under test
Calibrate against reference
Clock-aligned
MCP pulse time
Compare on
the same events
Module under test
Calibrate directly with MCP
Direct calibration for closure