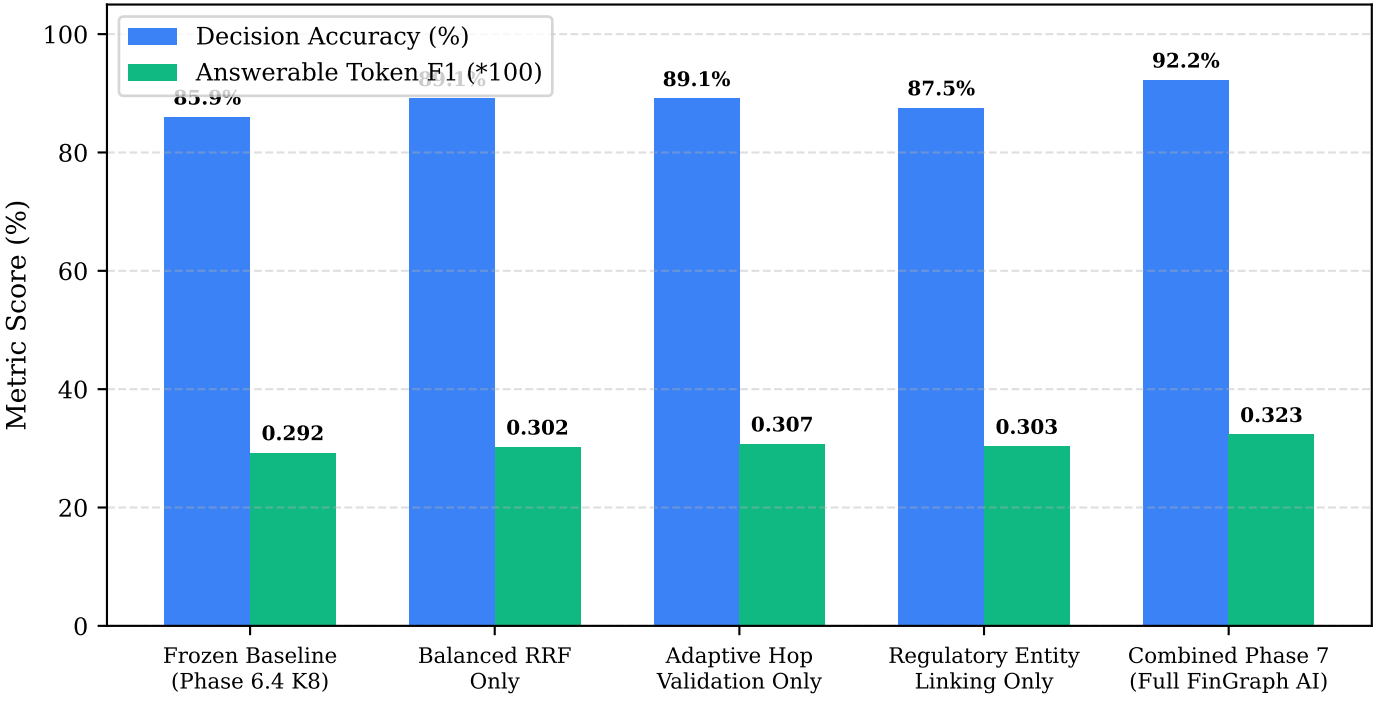Figure 11: FinGraph AI Phase 7 Component Ablation Performance