

## Patient Details

Name:	Ganesh	Age:	25	Gender:	Male
Date:	2026-01-23	Time:	12:08:55		

## Report Overview

Maximum Heart Rate:	100 bpm
Minimum Heart Rate:	100 bpm
Average Heart Rate:	100 bpm

## OBSERVATION

Interval Names	Observed Values	Standard Range
Heart Rate	100 bpm	60-100
PR Interval	174 ms	120 ms - 200 ms
QRS Complex	90 ms	70 ms - 120 ms
QT Interval	286 ms	300 ms - 450 ms
QTcB (Bazett)	369 ms	300 ms - 450 ms
QTcF (Fridericia)	0.339 s	300 ms - 450 ms
ST Deviation (J+60 ms)	0	Normal

## ECG Report Conclusion


S.No.	Conclusion
1	Measured Values:
2	Normal sinus rhythm (HR ≈ 100 bpm)
3	QTcB (Bazett): 369 ms (Normal); QTcF (Fridericia): 339 ms (0.339 s)
4	ST deviation: 0.00 mV (J+60ms); report only as deviation
5	Automated interpretation (conservative): Normal unless measurements suggest otherwise
6	Acquisition: Sampling rate 150 Hz; Gain 10.0 mm/mV; Paper speed 25.0 mm/s
7	This is an automated ECG analysis and must be reviewed by a qualified physician.

Name: Ganesh HR : 100 bpm P/QRS/T : -138/-/-165°  
Age: 25 PR : 174 ms RV5/SV1 : 0.083 mV/-1.127 mV  
Gender: Male QRS : 90 ms RV5+SV1 : 1.209 mV  
RR : 600 ms QTcf : 339 ms  
QT : 286 ms ST : 0 ms  
QTc : 369 ms 25.0 mm/s 0.5~35Hz AC : 50Hz 10.0 mm/mV

**DECK MOUNT**

Date: 2026-01-23

Time: 12:08:55

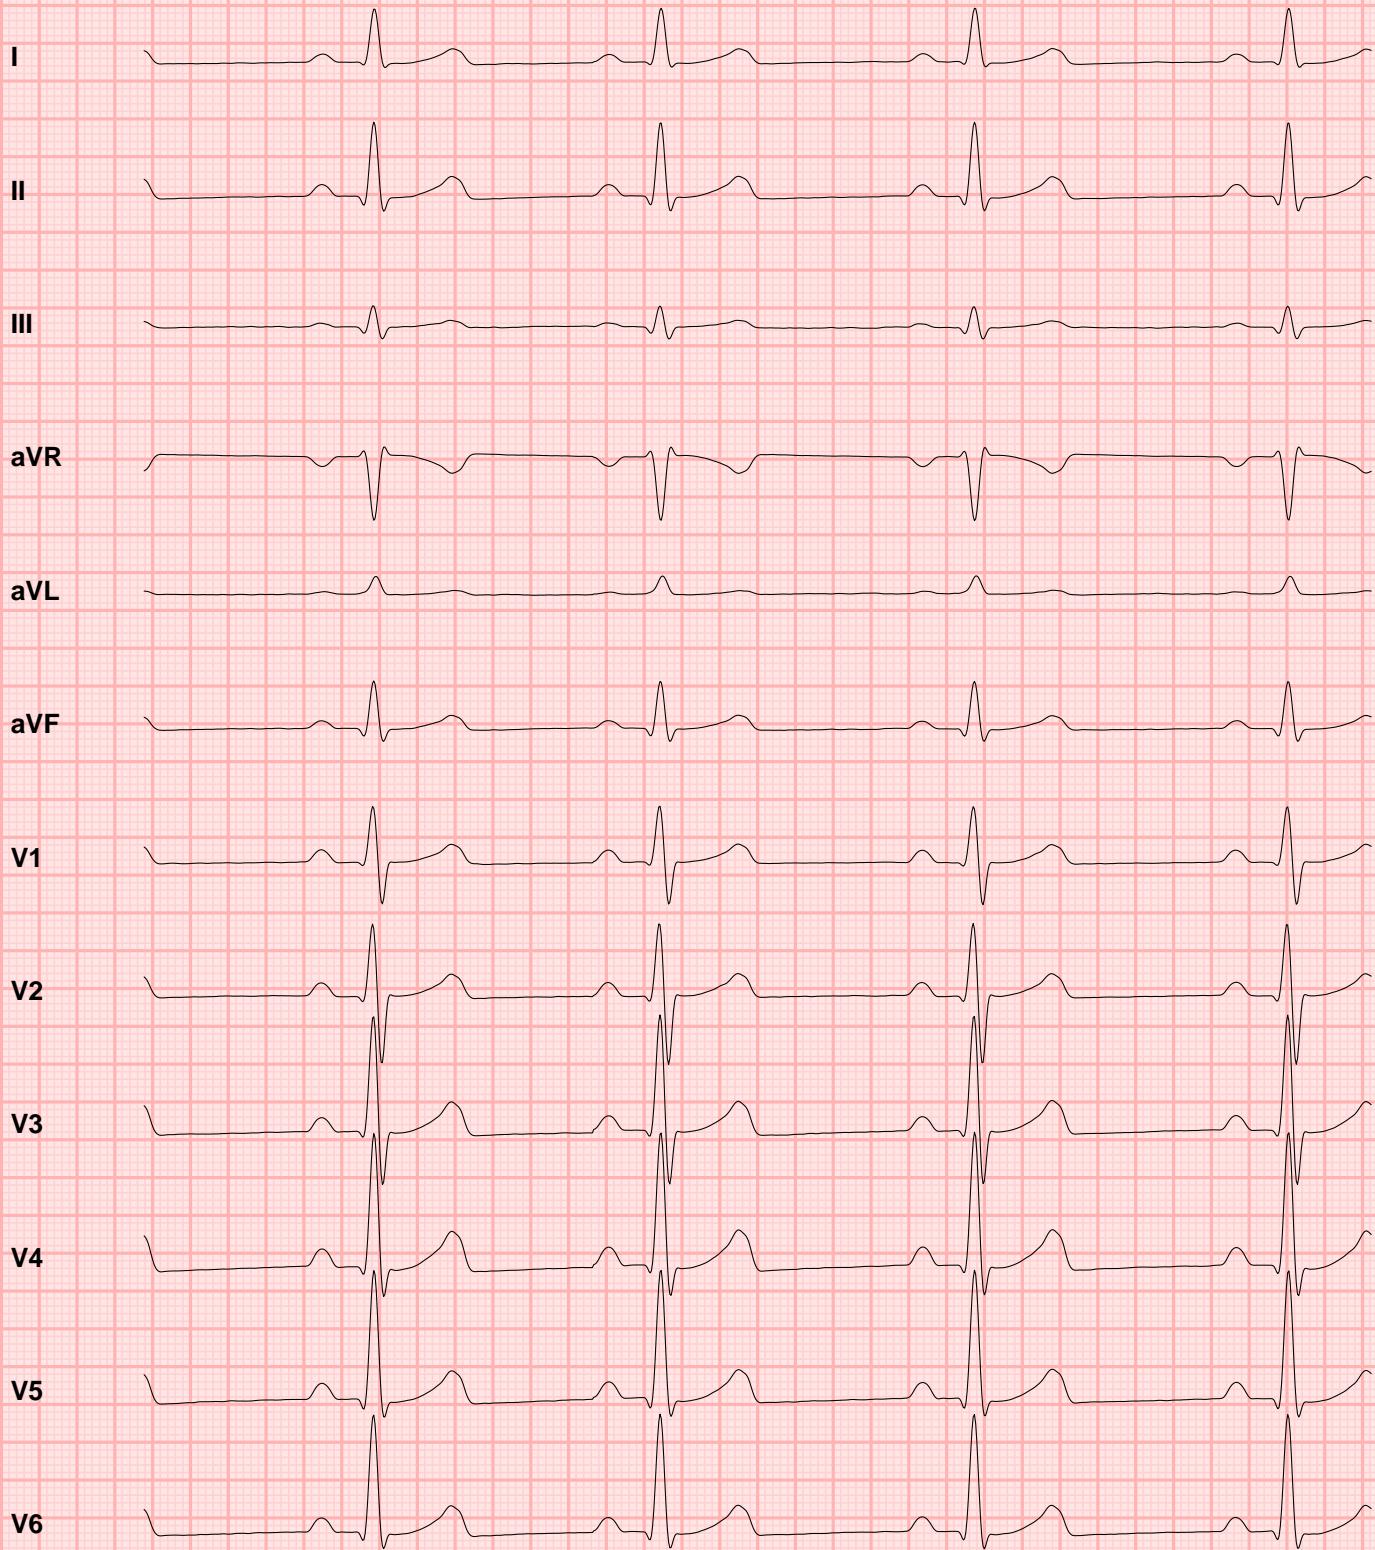

◆ CONCLUSION ◆

- |                              |   |
|------------------------------|---|
| <b>Doctor Name:</b> Divyansh | <b>CONCLUSION</b>   |
| <b>Doctor Sign:</b>          |   |
|                              | <ul style="list-style-type: none"><li>1. Measured Values:</li><li>3. QTcB (Bazett): 369 ms (Normal)...<br/>5. Automated interpretation (cons...<br/>7. This is an automated ECG analy...</li><li>2. Normal sinus rhythm (HR ≈ 100 ...<br/>4. ST deviation: 0.00 mV (J+60ms)...<br/>6. Acquisition: Sampling rate 150...</li></ul> |

- 1. Measured Values:
- 3. QTcB (Bazett): 369 ms (Normal)...  
5. Automated interpretation (cons...  
7. This is an automated ECG analy...
- 2. Normal sinus rhythm (HR ≈ 100 ...  
4. ST deviation: 0.00 mV (J+60ms)...  
6. Acquisition: Sampling rate 150...