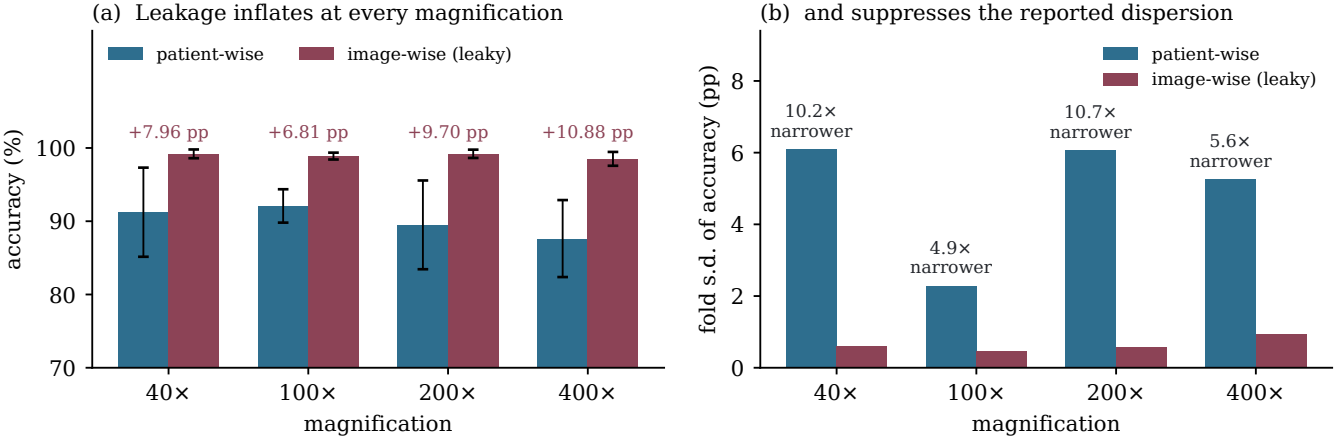
(a) Leakage inflates at every magnification
patient-wise
image-wise (leaky)
accuracy (%)
100
90
80
70
+7.96 pp
+6.81 pp
+9.70 pp
+10.88 pp
40×
100×
200×
400×
magnification
(b) and suppresses the reported dispersion
patient-wise
image-wise (leaky)
fold s.d. of accuracy (pp)
8
6
4
2
0
10.2× narrower
4.9× narrower
10.7× narrower
5.6× narrower
40×
100×
200×
400×
magnification