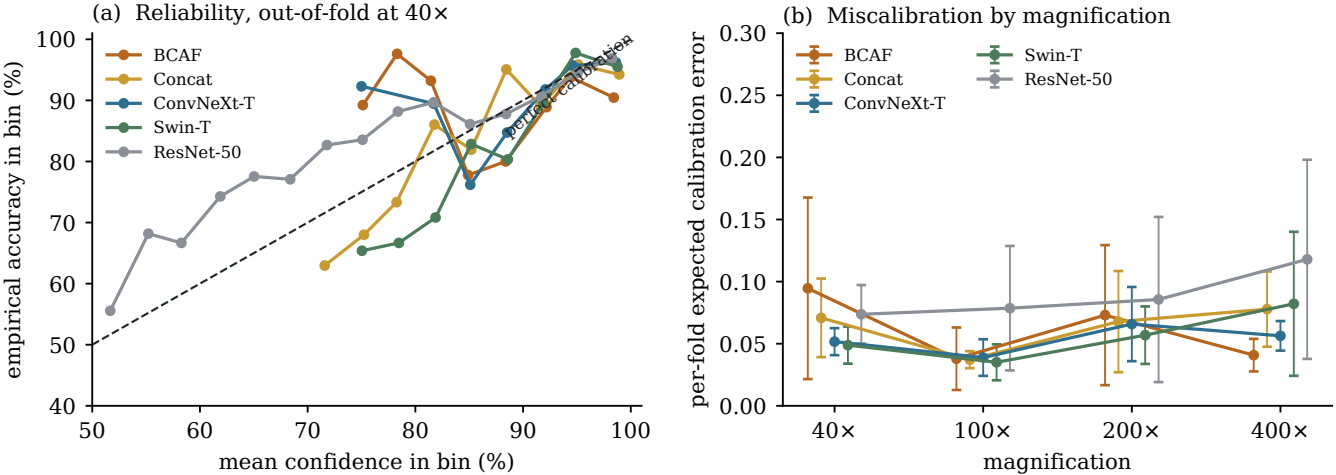
(a) Reliability, out-of-fold at 40×
BCAF
Concat
ConvNeXt-T
Swin-T
ResNet-50
perfect calibration
empirical accuracy in bin (%)
mean confidence in bin (%)
100
90
80
70
60
50
40
50
60
70
80
90
100
(b) Miscalibration by magnification
BCAF
Concat
ConvNeXt-T
Swin-T
ResNet-50
per-fold expected calibration error
magnification
0.30
0.25
0.20
0.15
0.10
0.05
0.00
40×
100×
200×
400×